


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090325\
Data File : BG064265.D
Acq On : 3 Sep 2025 23:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

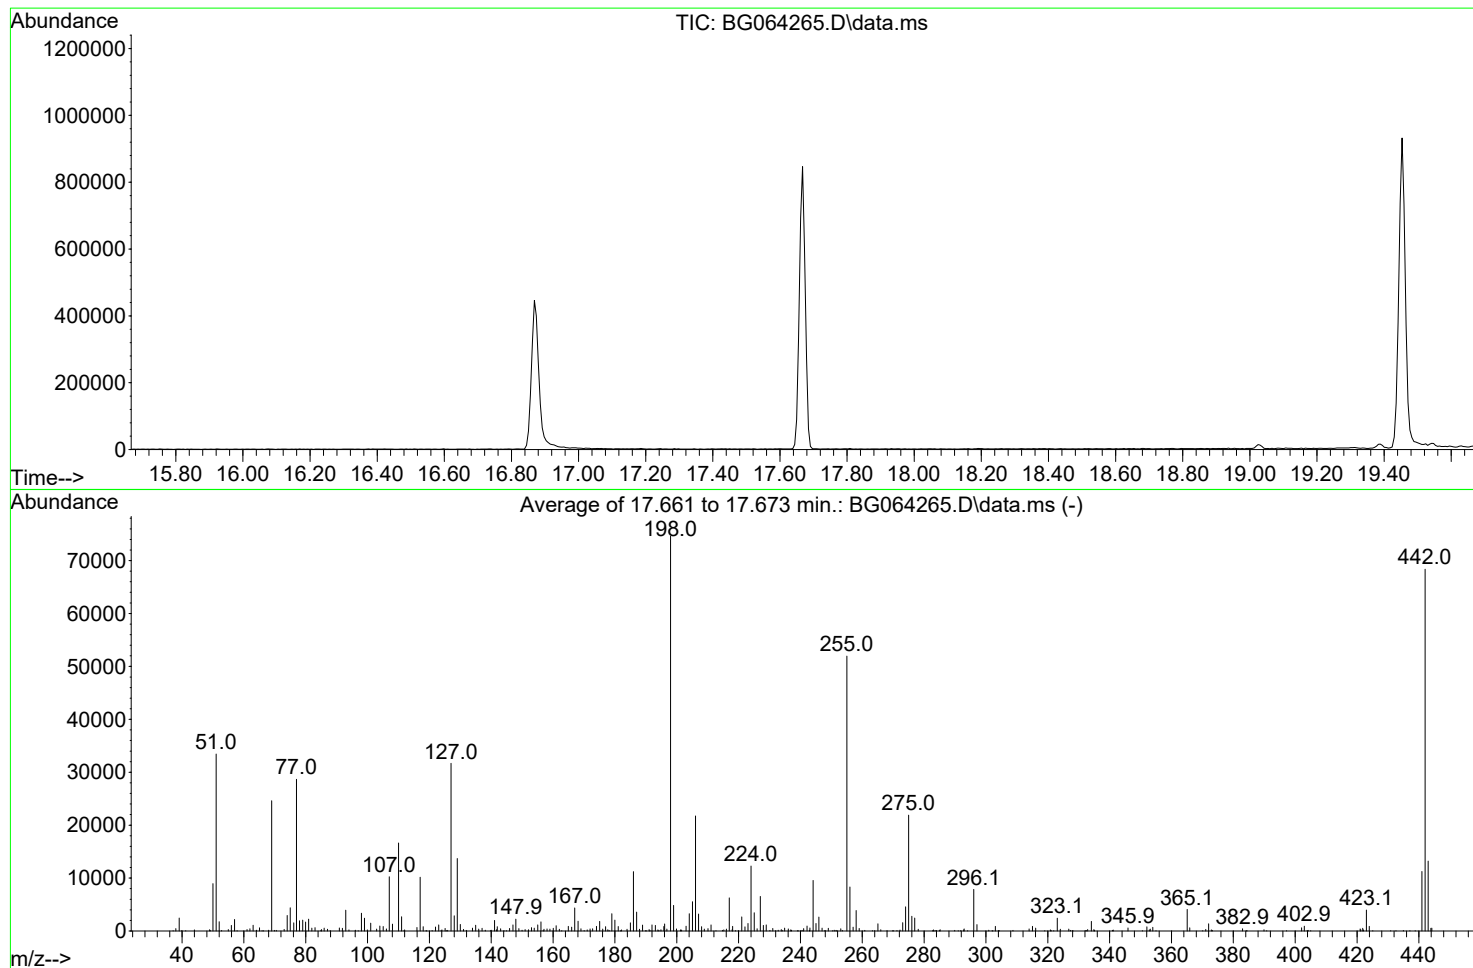

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.6	150	PASS
69	69	100	100	100.0	24613	PASS
70	69	0.00	2	0.5	130	PASS
197	198	0.00	2	0.5	366	PASS
198	198	100	100	100.0	74616	PASS
199	198	5	9	6.5	4851	PASS
365	198	1	100	5.5	4073	PASS
441	443	0.01	150	85.2	11266	PASS
442	442	100	100	100.0	68376	PASS
443	442	15	24	19.3	13222	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/3/2025	BNA_G	<u>BG064265.D</u>
Compound Name	Response	Retention Time
DDT	274532	20.687
DDD	7153	20.253
DDE	61	19.771
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7214	281746	2.56

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090325\
Data File : BG064265.D
Acq On : 3 Sep 2025 23:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 04 01:49:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

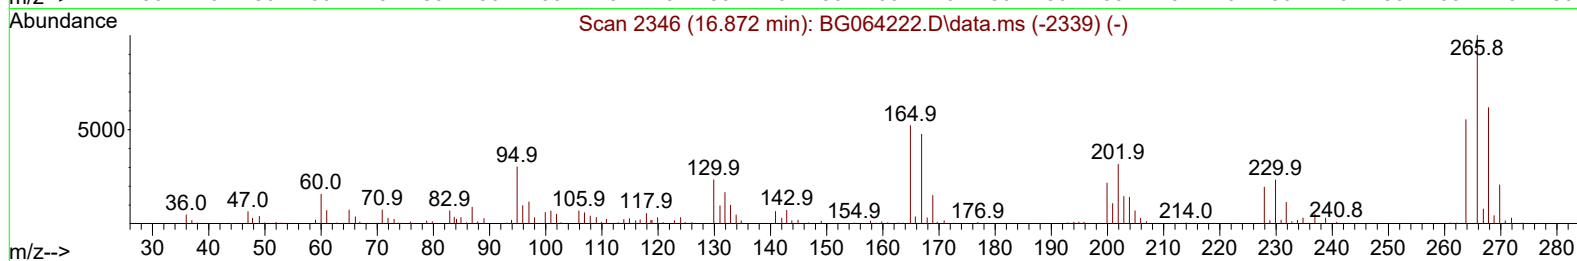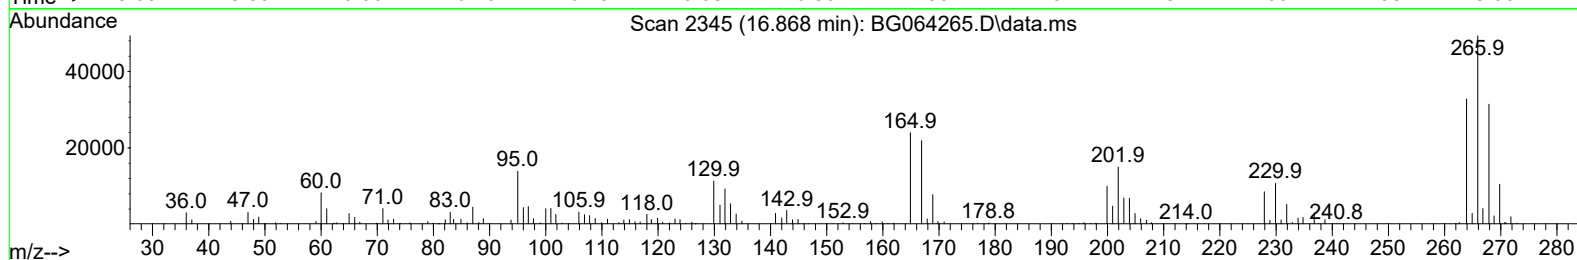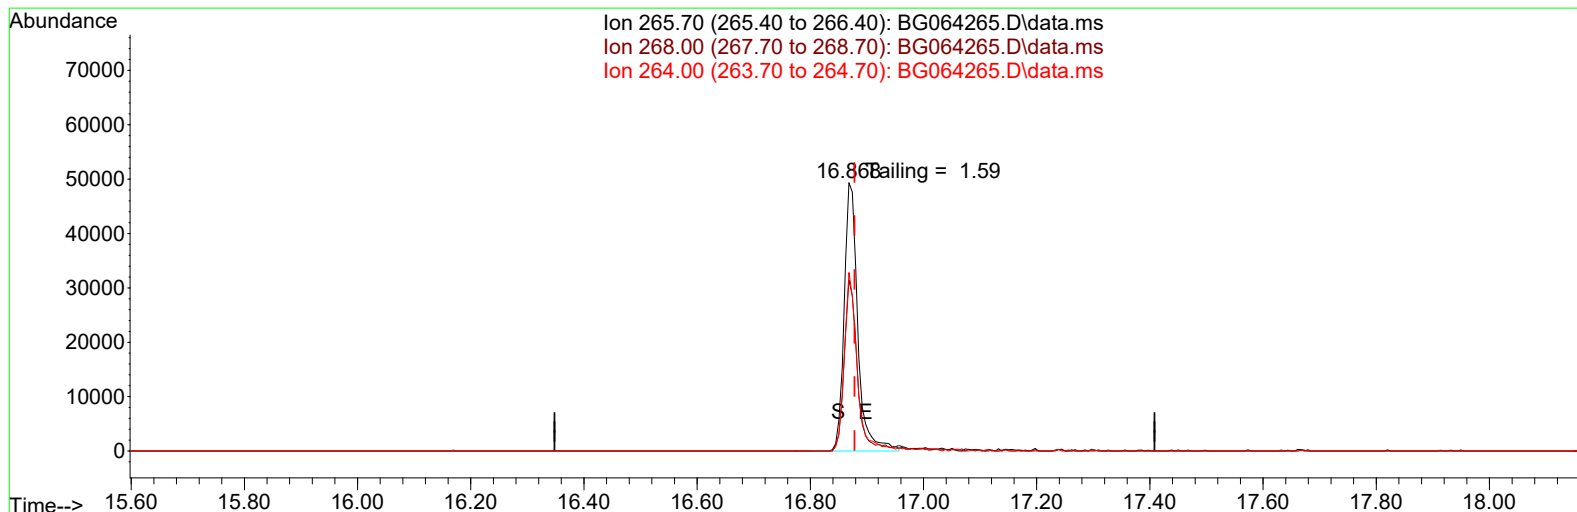

TIC: BG064265.D\data.ms

(70) Pentachlorophenol (C)

16.868min (-0.010) 195043.33 ng




response 82298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.66
264.00	55.40	66.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090325\
Data File : BG064265.D
Acq On : 3 Sep 2025 23:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 04 01:49:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

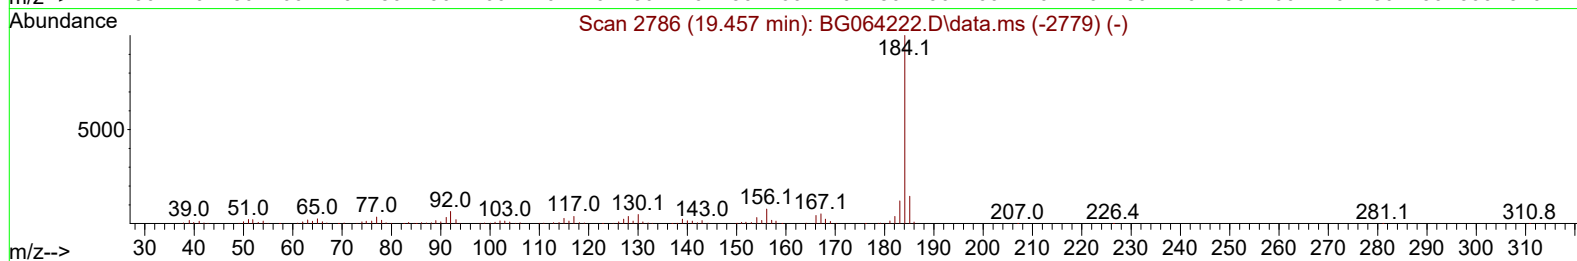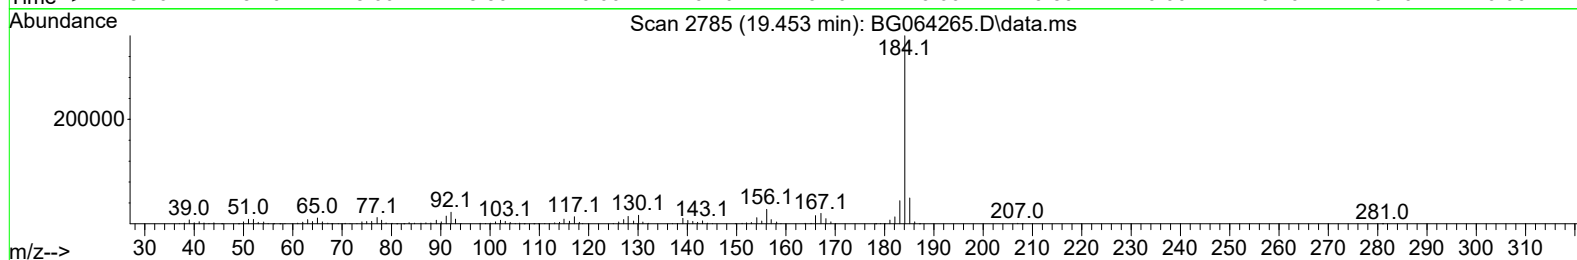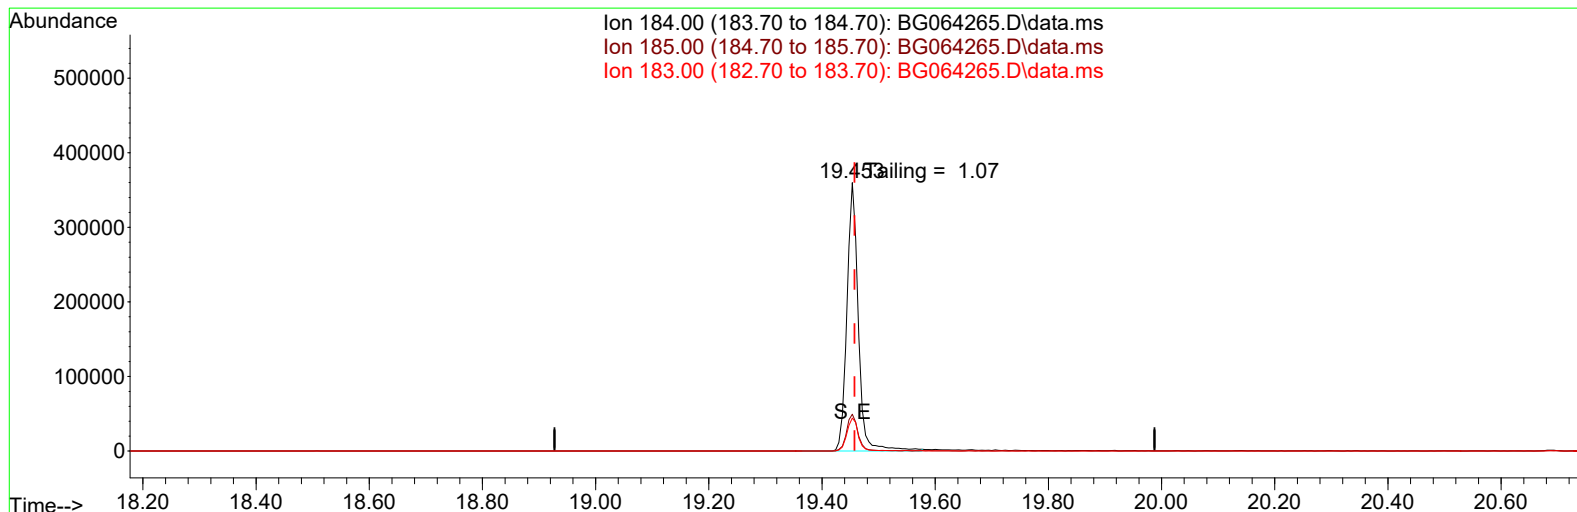

TIC: BG064265.D\data.ms

(77) Benzidine

19.453min (-0.004) 359802.62 ng

response 499553

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.71
183.00	12.10	12.29
0.00	0.00	0.00