


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090418\
 Data File : BG036523.D
 Acq On : 4 Sep 2018 9:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

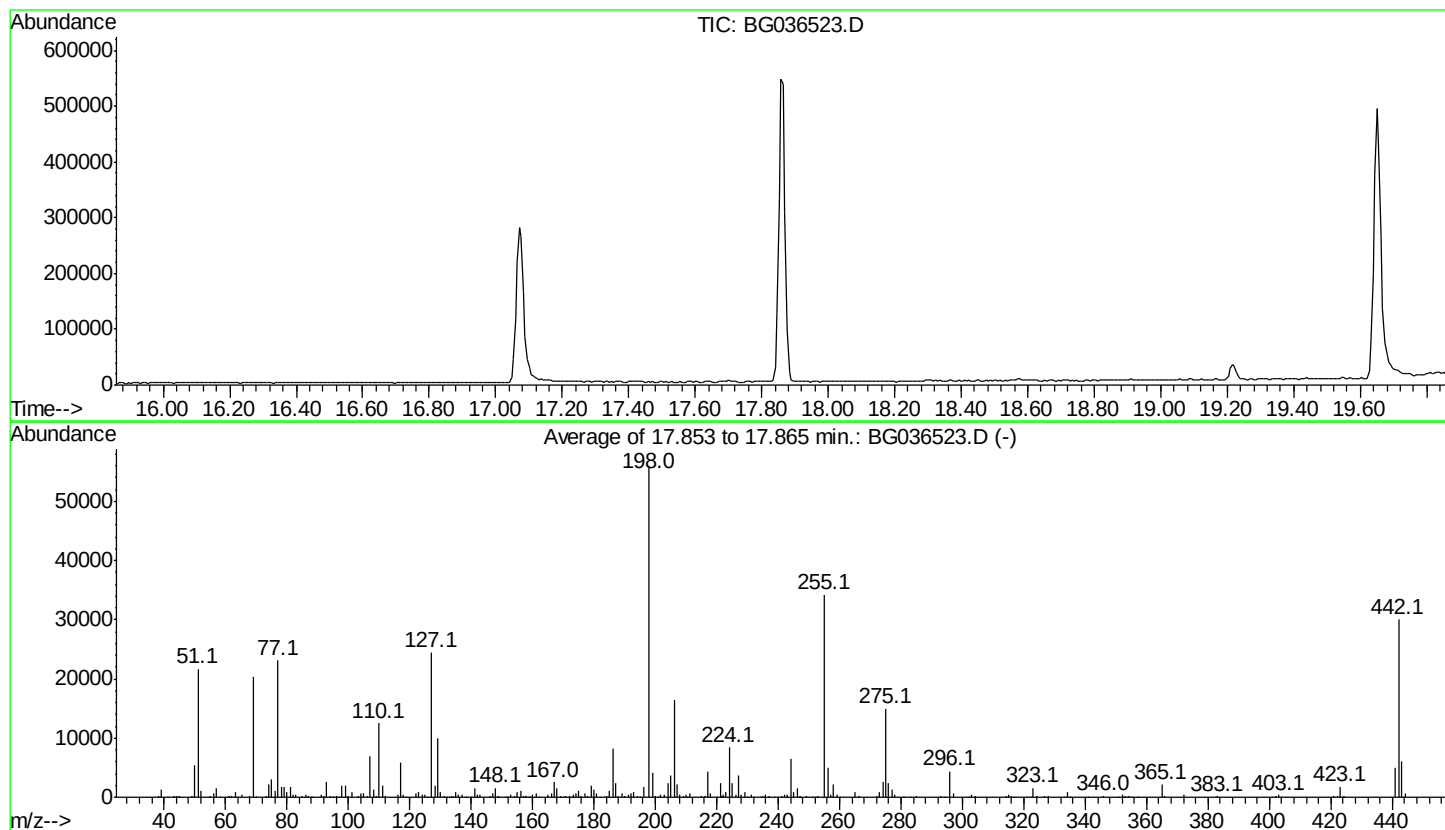

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	21698	PASS
68	69	0.00	2	1.3	275	PASS
69	198	0.00	100	36.4	20377	PASS
70	69	0.00	2	0.3	64	PASS
127	198	10	80	43.5	24360	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56005	PASS
199	198	5	9	7.4	4135	PASS
275	198	10	60	26.8	15025	PASS
365	198	1	100	3.8	2123	PASS
441	198	0.01	100	8.8	4907	PASS
442	198	50	100	53.6	30024	PASS
443	442	15	24	20.0	5998	PASS