
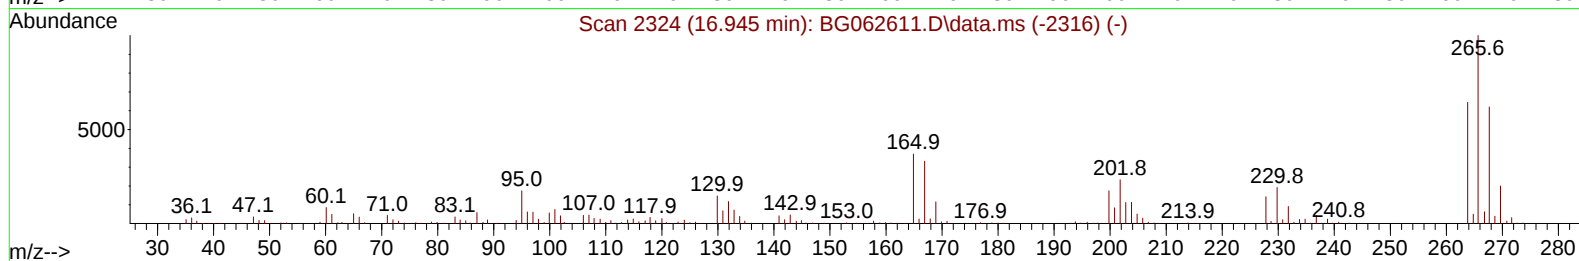
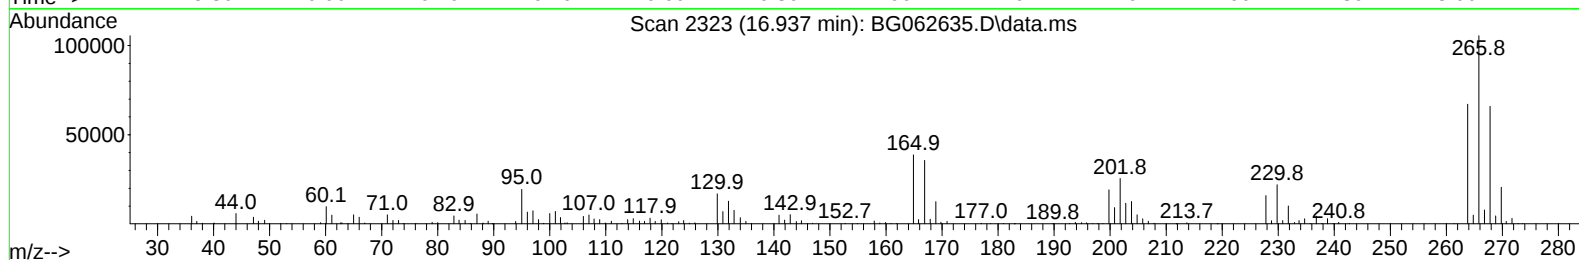


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062635.D
Acq On : 4 Sep 2024 9:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 10:21:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

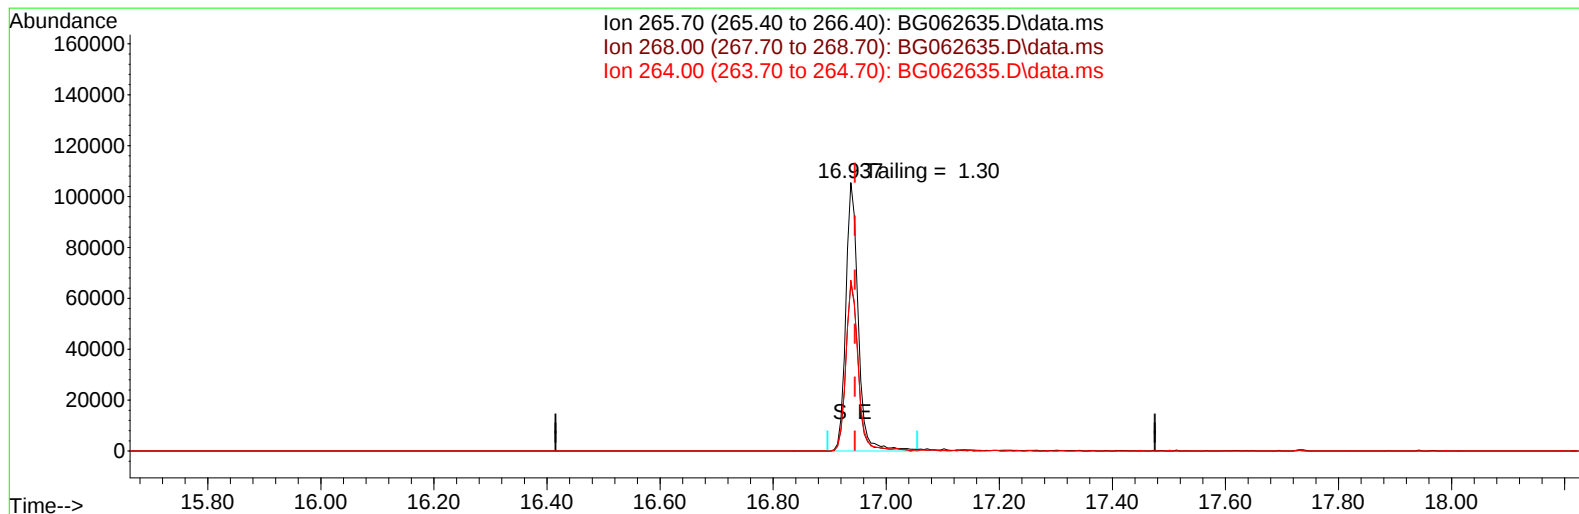

TIC: BG062635.D\data.ms

(70) Pentachlorophenol (C)




16.937min (-0.008) 29529.70 ng

response 160896

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.54
264.00	64.50	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062635.D
Acq On : 4 Sep 2024 9:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 10:21:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

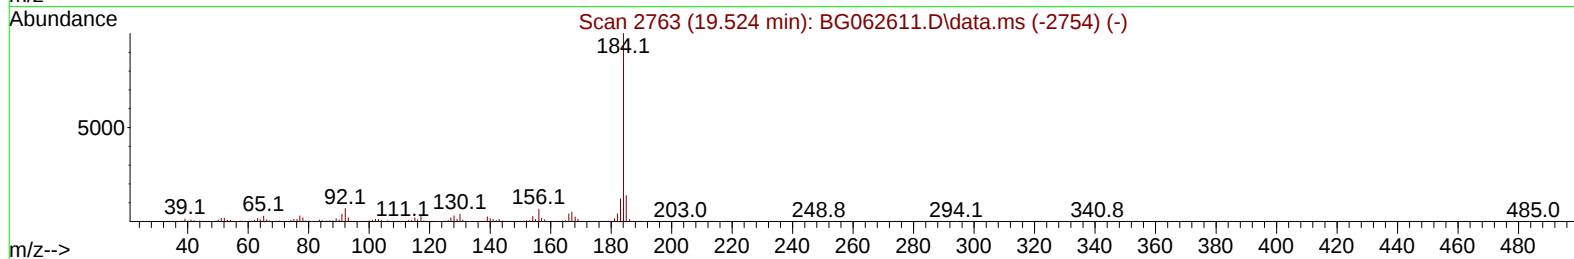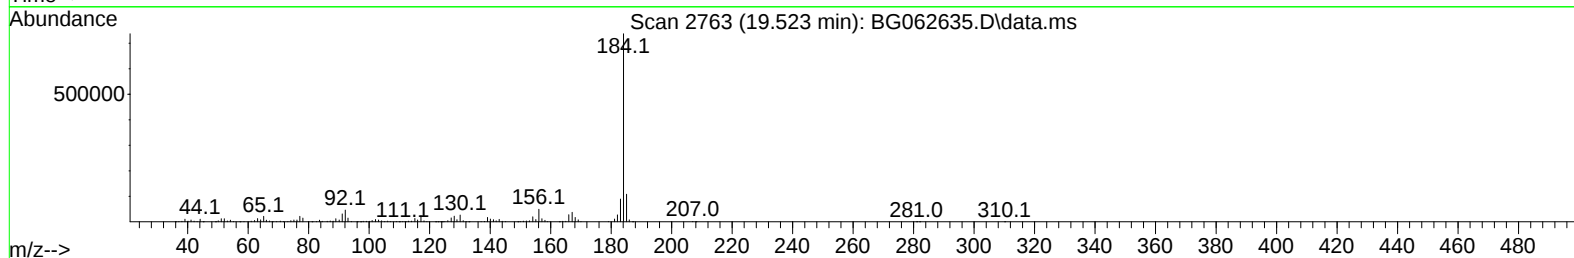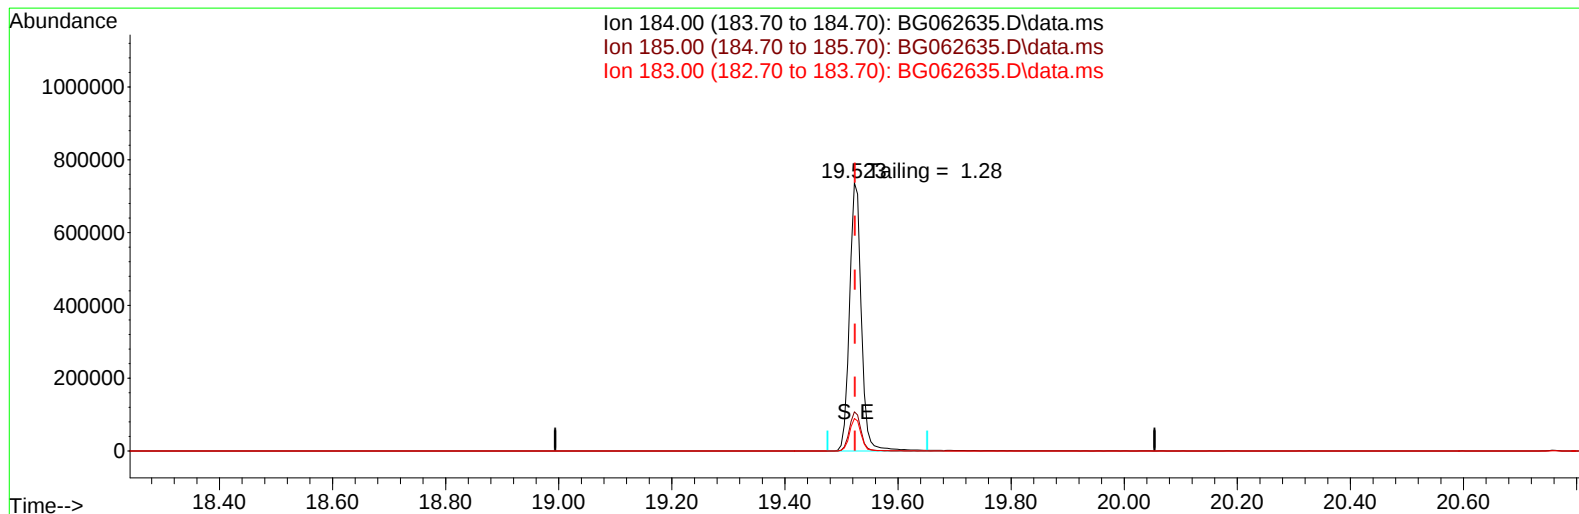

TIC: BG062635.D\data.ms

(77) Benzidine**19.523min (-0.001) 0.00 ng****response 1071822**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.64
183.00	12.10	12.11
0.00	0.00	0.00