
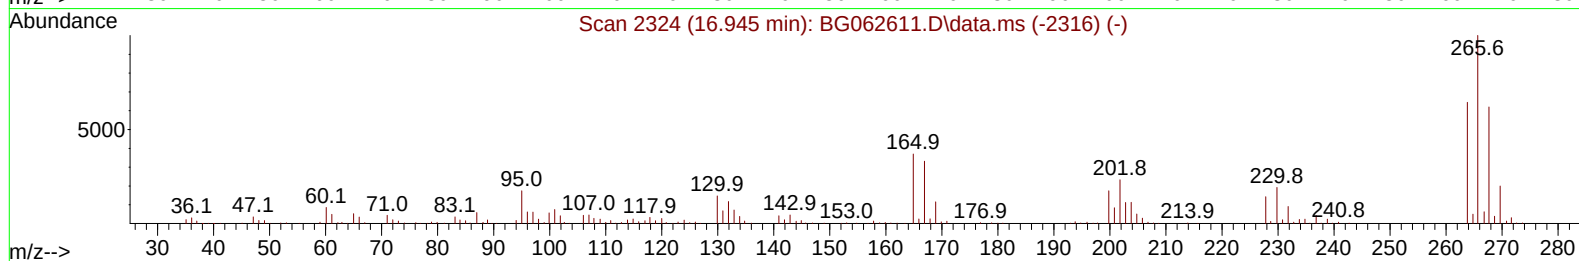
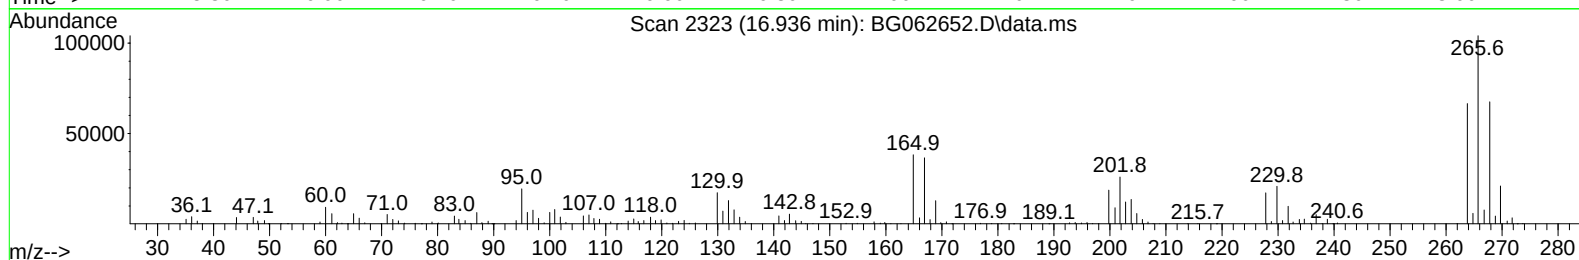


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062652.D
Acq On : 4 Sep 2024 21:04
Operator : MA/JU
Sample : DFTPP
Misc : LOD-MDL-WATER-8 ng
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 16:37:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

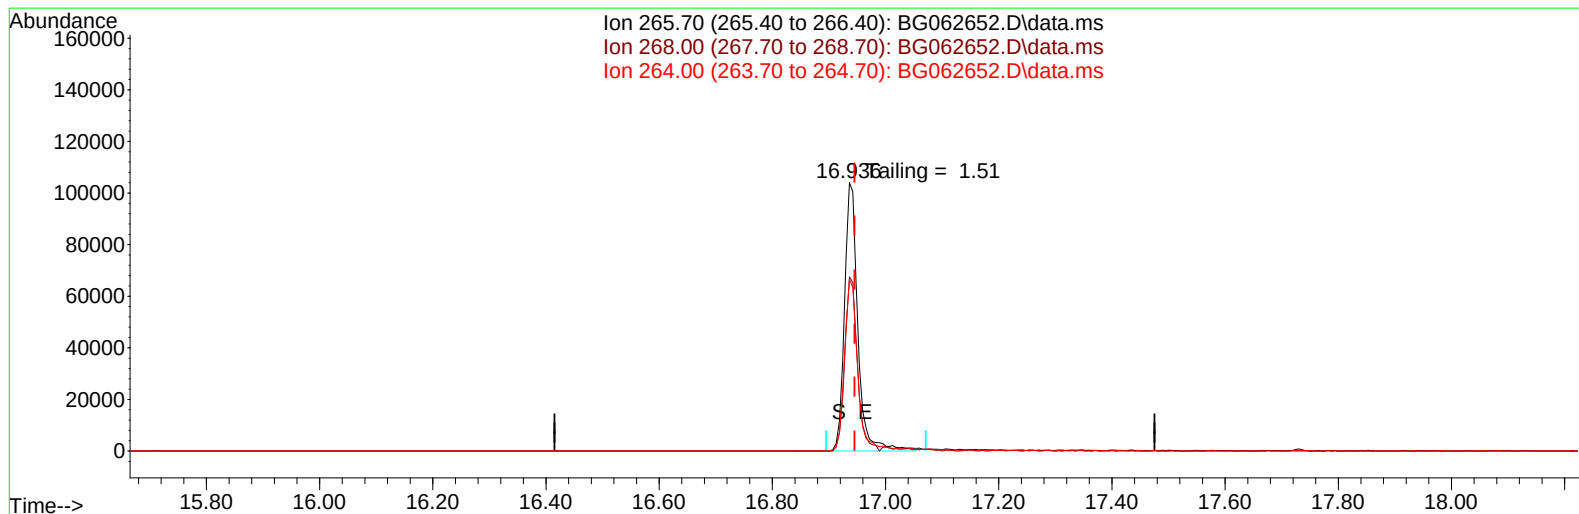

TIC: BG062652.D\data.ms

(70) Pentachlorophenol (C)




16.936min (-0.009) 22047.44 ng

response 172080

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.87
264.00	64.50	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062652.D
Acq On : 4 Sep 2024 21:04
Operator : MA/JU
Sample : DFTPP
Misc : LOD-MDL-WATER-8 ng
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 16:37:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

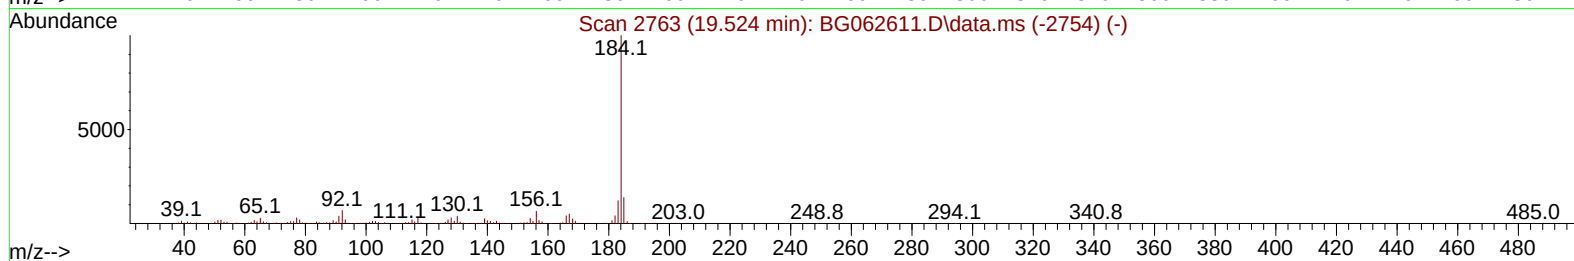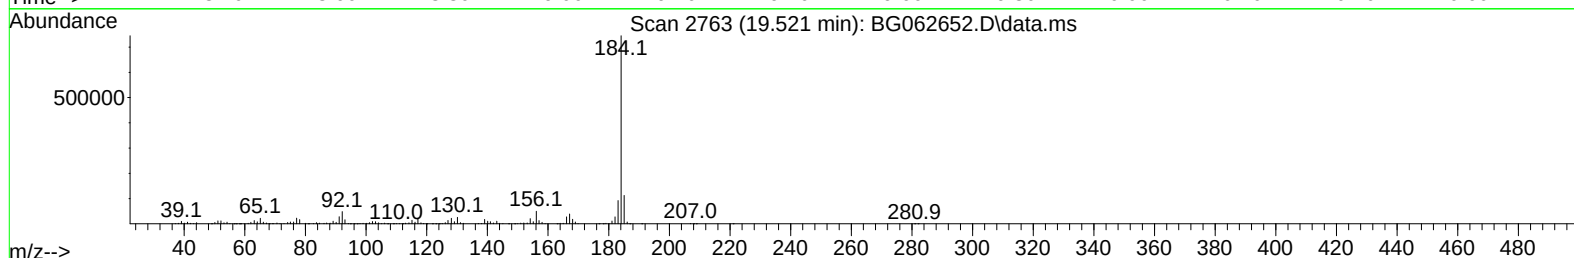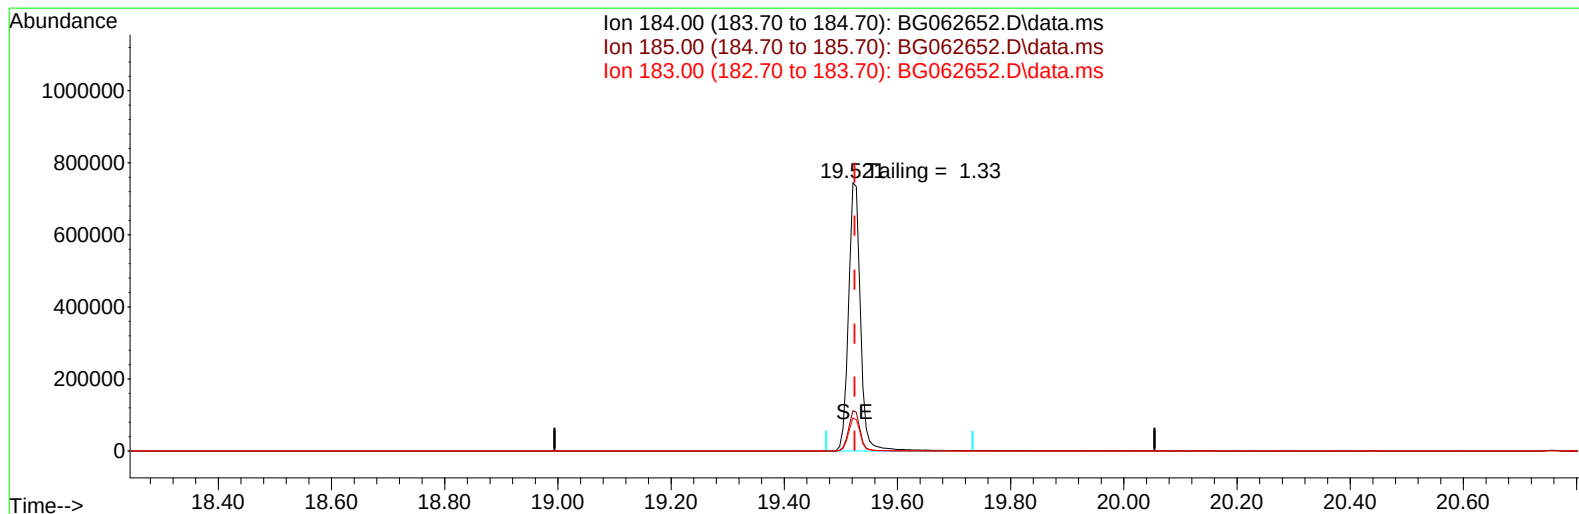

TIC: BG062652.D\data.ms

(77) Benzidine

19.521min (-0.003) 0.00 ng

response 1098745

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	15.05
183.00	12.10	12.33
0.00	0.00	0.00