


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062635.D
Acq On : 4 Sep 2024 9:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 31 02:36:01 2024

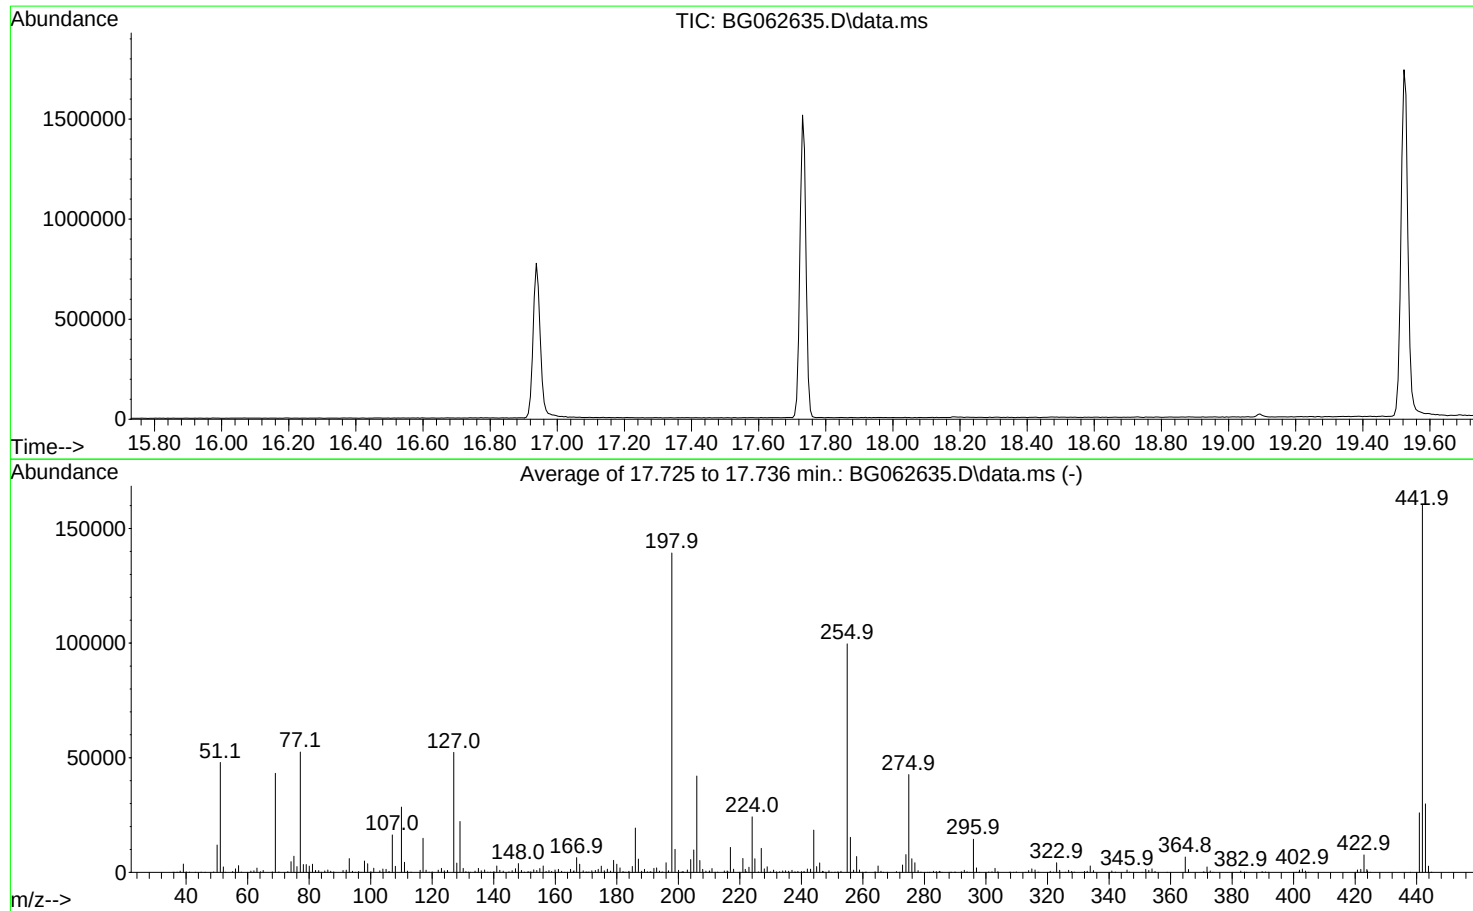




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	47955	PASS
68	69	0.00	2	0.5	234	PASS
69	198	0.00	100	31.0	43187	PASS
70	69	0.00	2	0.5	196	PASS
127	198	10	80	37.6	52320	PASS
197	198	0.00	2	0.5	681	PASS
198	198	100	100	100.0	139320	PASS
199	198	5	9	7.2	10029	PASS
275	198	10	60	30.6	42651	PASS
365	198	1	100	4.8	6743	PASS
441	198	0.01	100	18.7	26000	PASS
442	442	50	100	100.0	160483	PASS
443	442	15	24	18.6	29869	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062635.D
Acq On : 4 Sep 2024 9:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 04 10:21:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

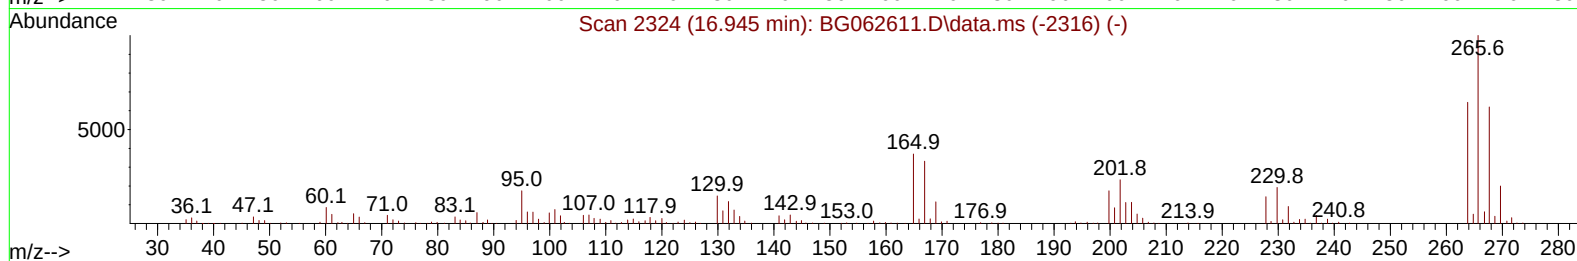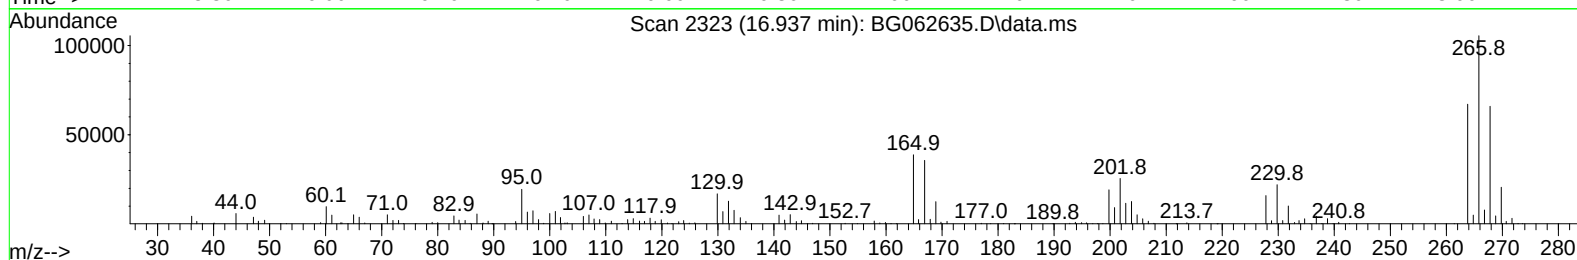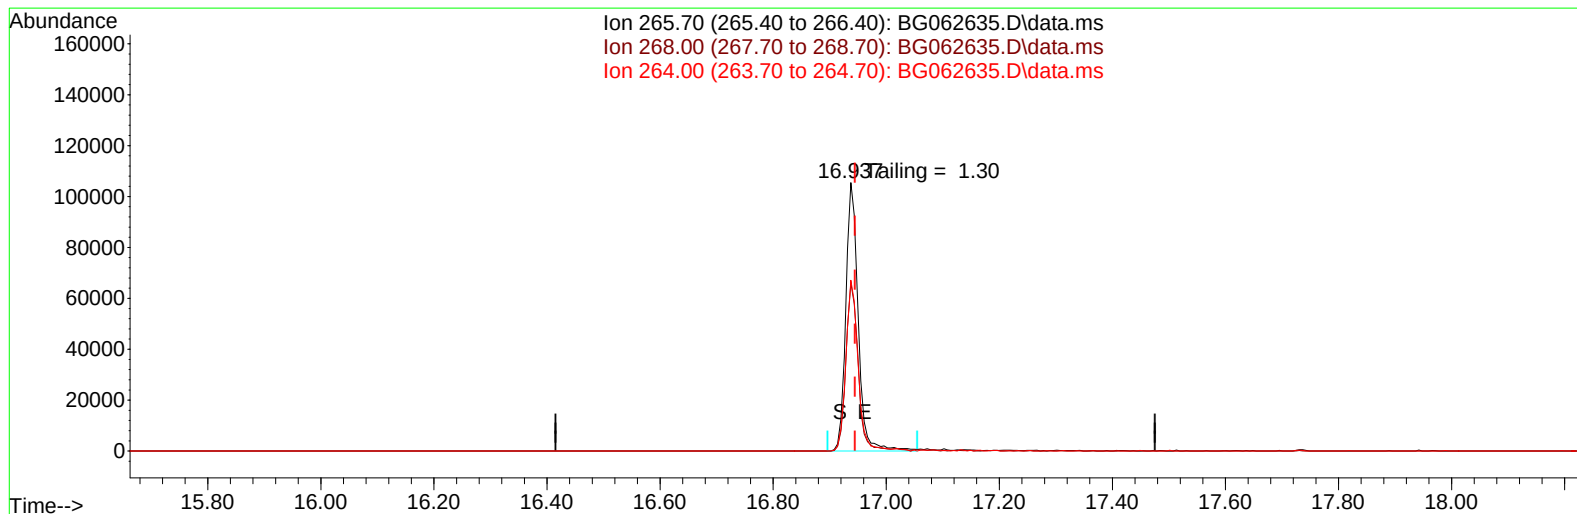

TIC: BG062635.D\data.ms

(70) Pentachlorophenol (C)

16.937min (-0.008) 29529.70 ng




response 160896

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.54
264.00	64.50	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062635.D
Acq On : 4 Sep 2024 9:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 04 10:21:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

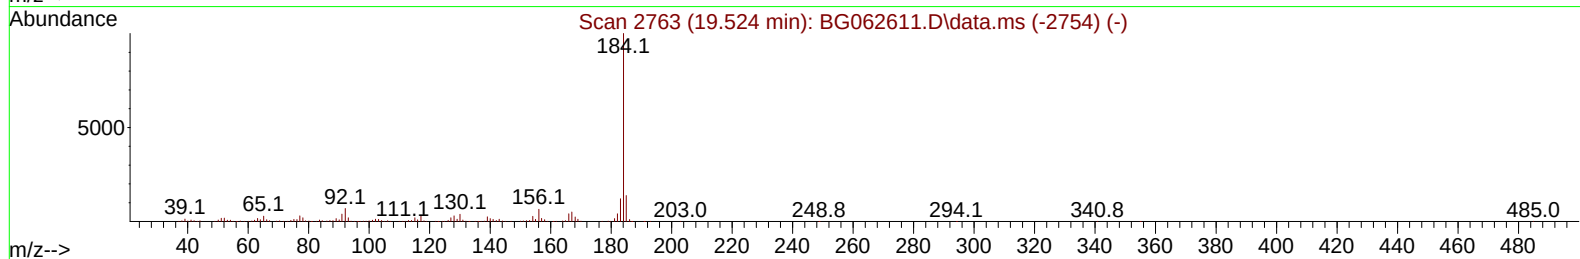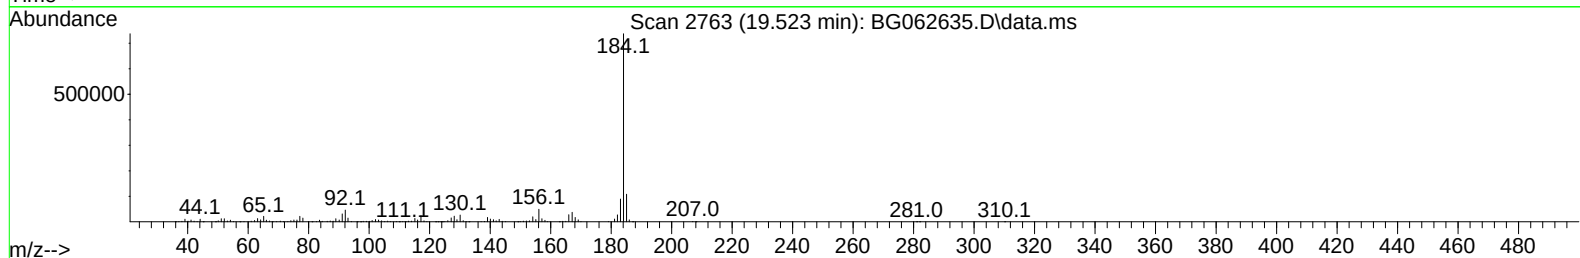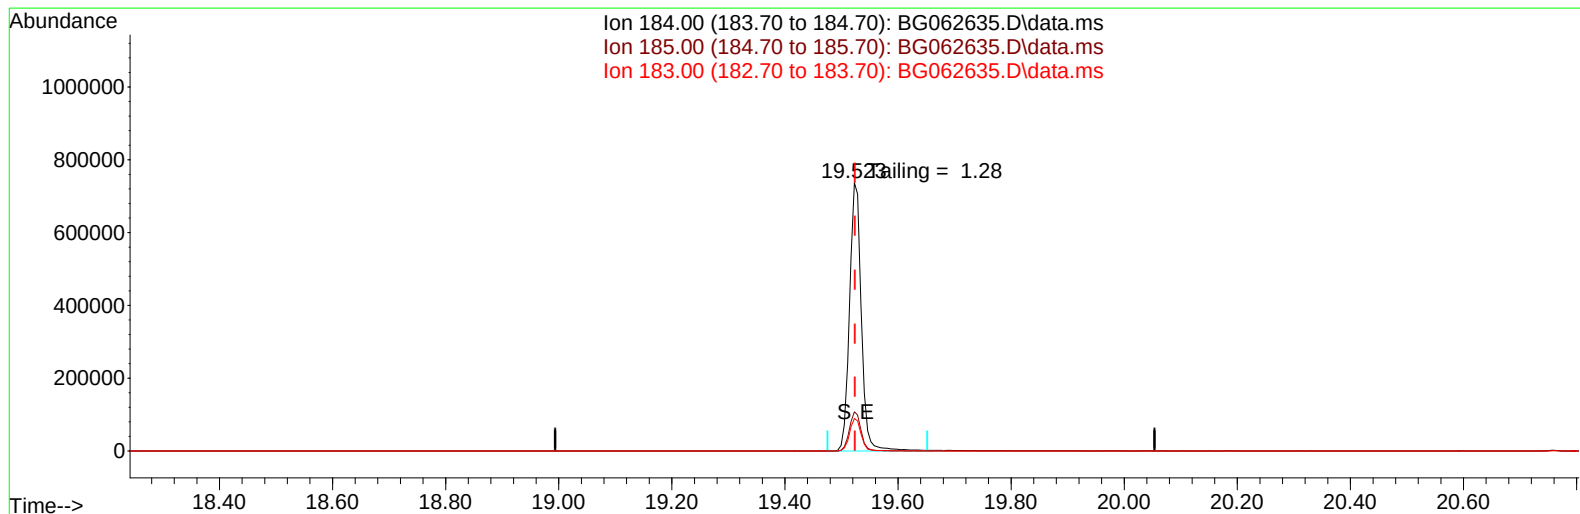

TIC: BG062635.D\data.ms

(77) Benzidine

19.523min (-0.001) 0.00 ng

response 1071822

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.64
183.00	12.10	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/4/2024	BNA_G	<u>BG062635.D</u>
Compound Name	Response	Retention Time
DDT	465057	20.756
DDD	9887	20.322
DDE	447	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10334	475391	2.17

Instrument :
BNA_G
ClientSampleId :
DFTPP