


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062652.D
Acq On : 4 Sep 2024 21:04
Operator : MA/JU
Sample : DFTPP
Misc : LOD-MDL-WATER-8 ng
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 31 02:36:01 2024

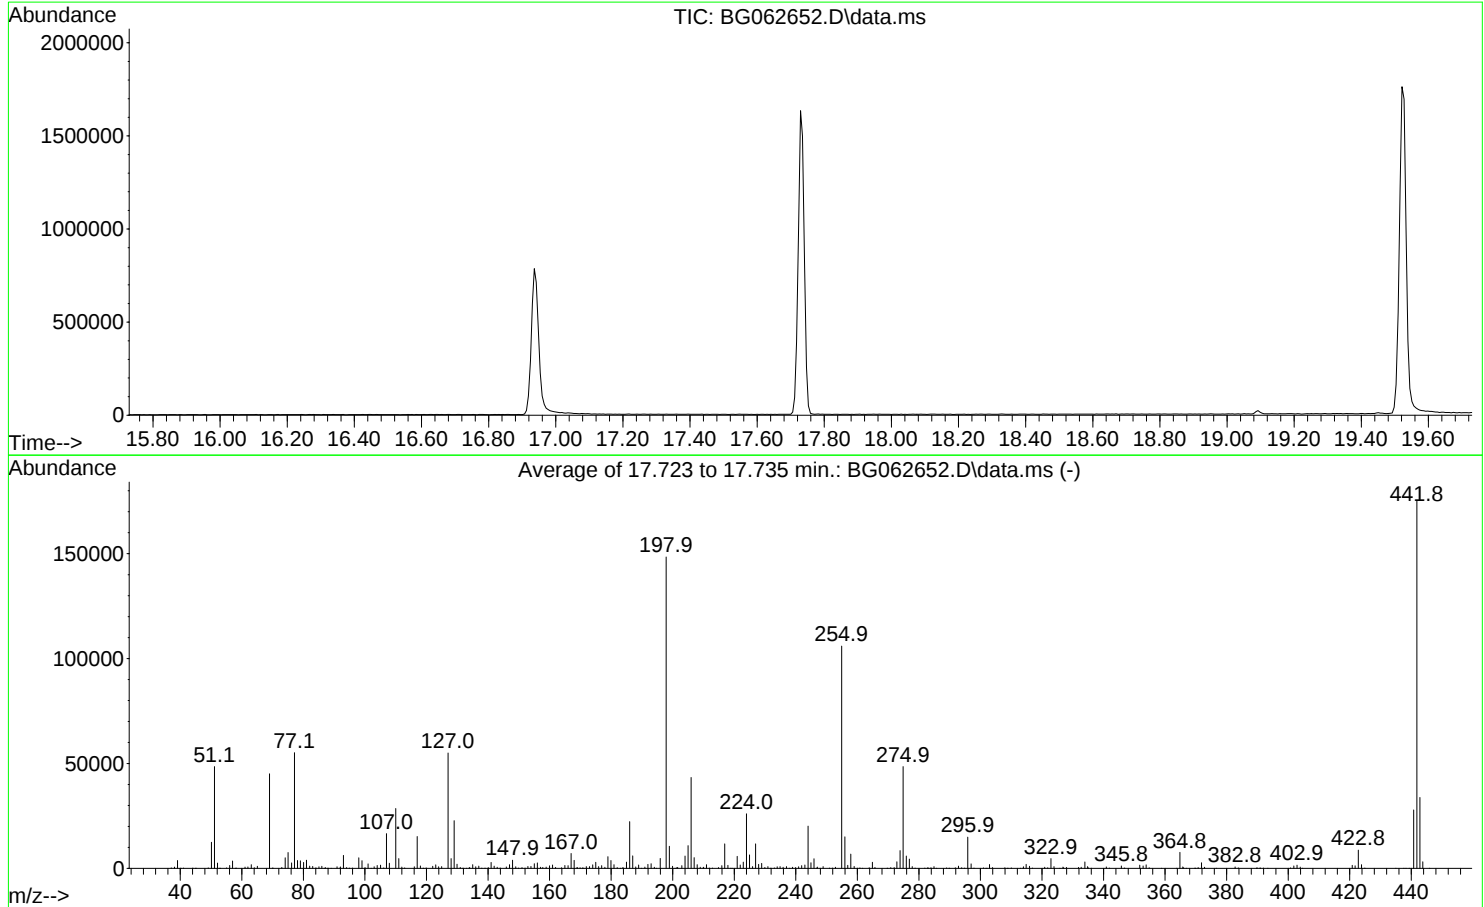




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	48531	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.4	45104	PASS
70	69	0.00	2	0.4	179	PASS
127	198	10	80	37.0	54976	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148424	PASS
199	198	5	9	7.1	10503	PASS
275	198	10	60	32.7	48493	PASS
365	198	1	100	5.1	7616	PASS
441	198	0.01	100	18.8	27862	PASS
442	442	50	100	100.0	175360	PASS
443	442	15	24	19.3	33789	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062652.D
Acq On : 4 Sep 2024 21:04
Operator : MA/JU
Sample : DFTPP
Misc : LOD-MDL-WATER-8 ng
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 05 16:37:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

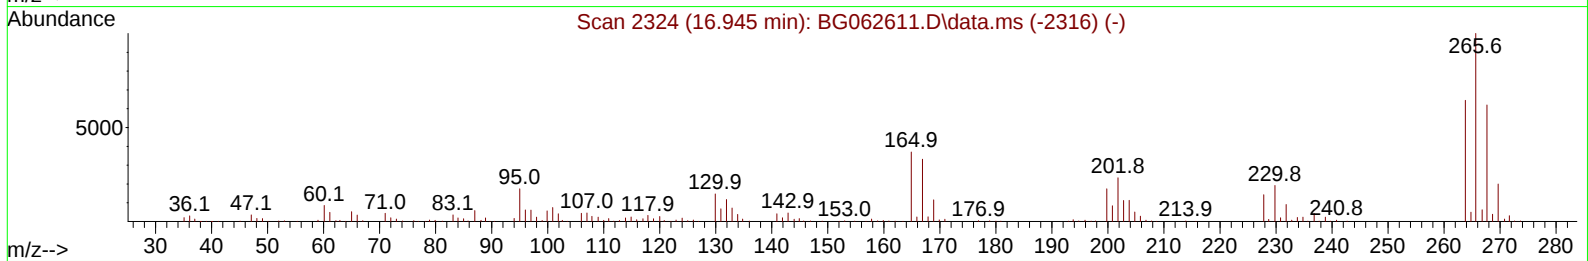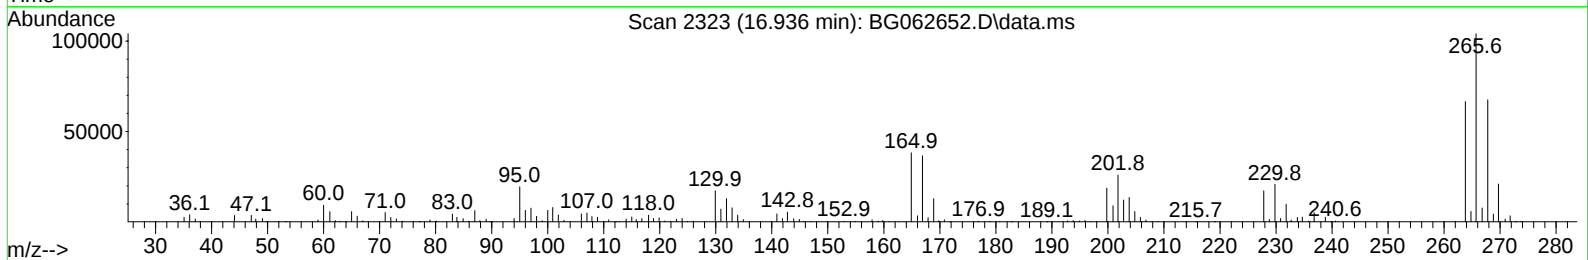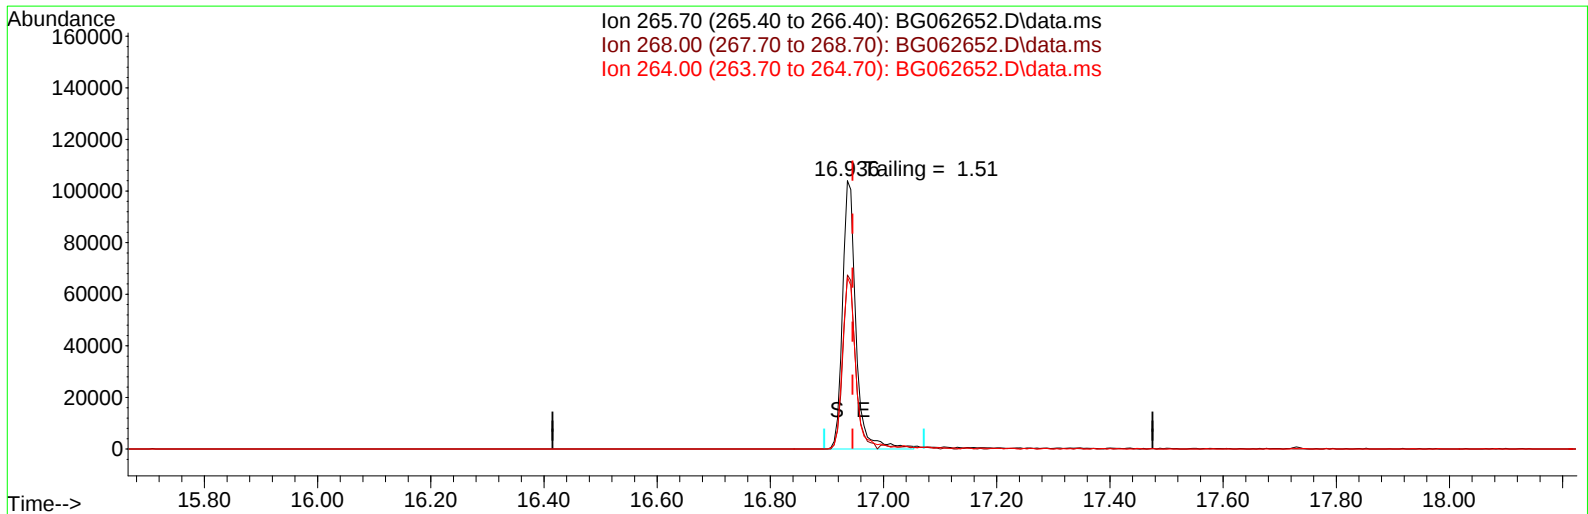

TIC: BG062652.D\data.ms

(70) Pentachlorophenol (C)

16.936min (-0.009) 22047.44 ng




response 172080

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.87
264.00	64.50	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090424\
Data File : BG062652.D
Acq On : 4 Sep 2024 21:04
Operator : MA/JU
Sample : DFTPP
Misc : LOD-MDL-WATER-8 ng
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 05 16:37:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

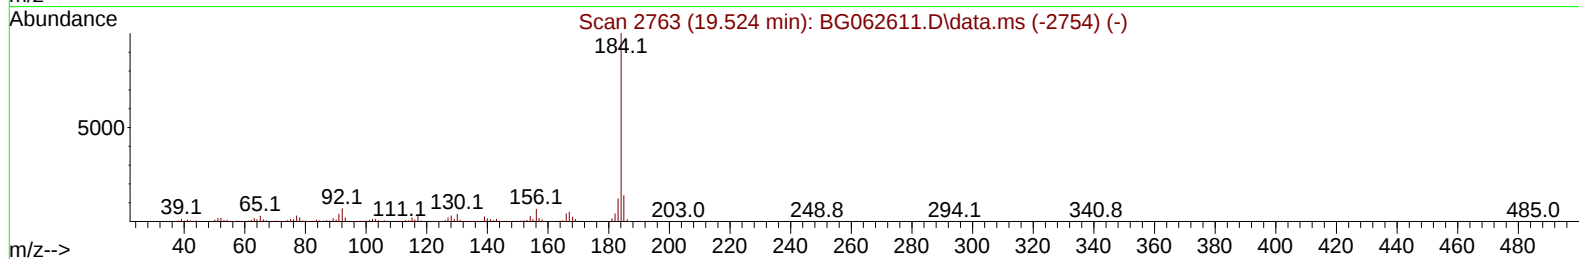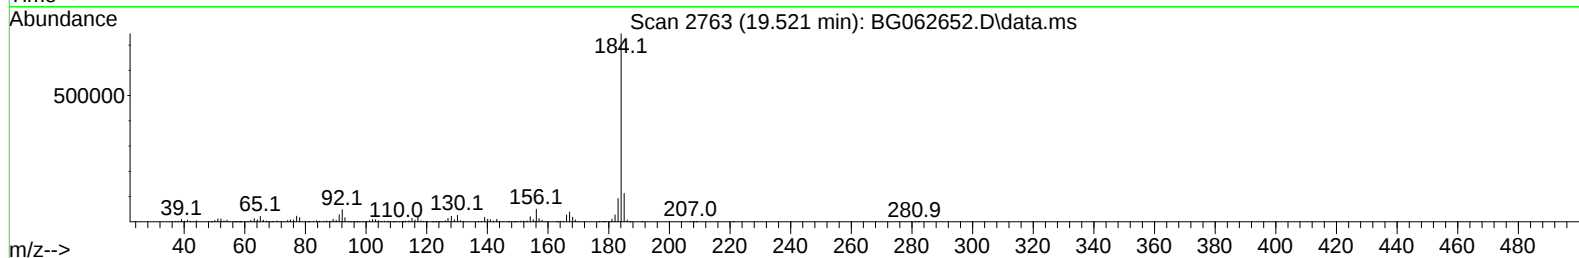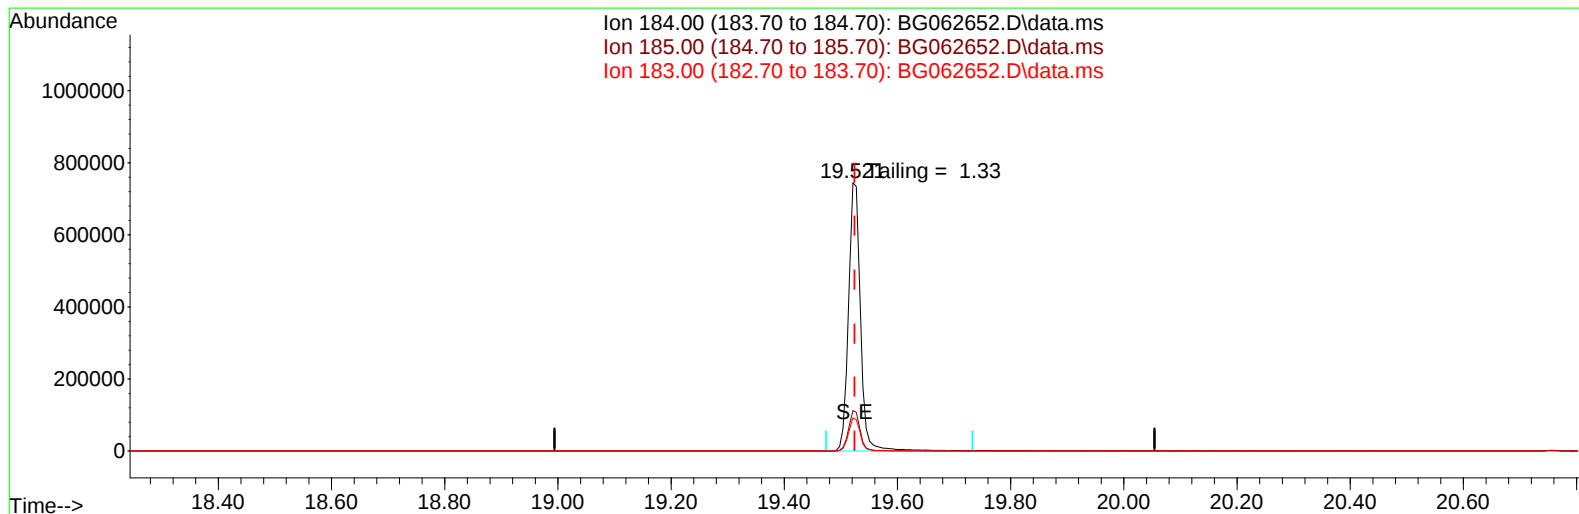

TIC: BG062652.D\data.ms

(77) Benzidine

19.521min (-0.003) 0.00 ng

response 1098745

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	15.05
183.00	12.10	12.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/4/2024	BNA_G	<u>BG062652.D</u>
Compound Name	Response	Retention Time
DDT	526957	20.761
DDD	14378	20.32
DDE	402	19.815
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14780	541737	2.73

Instrument :
BNA_G
ClientSampleId :
DFTPP