
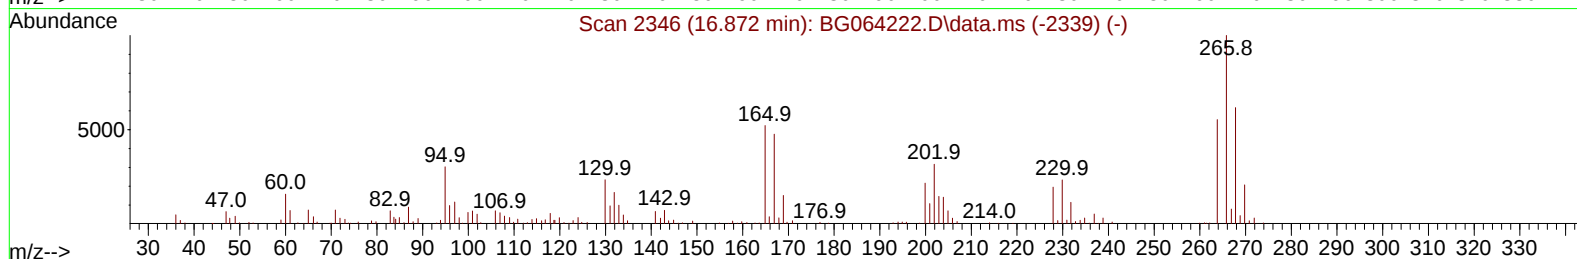
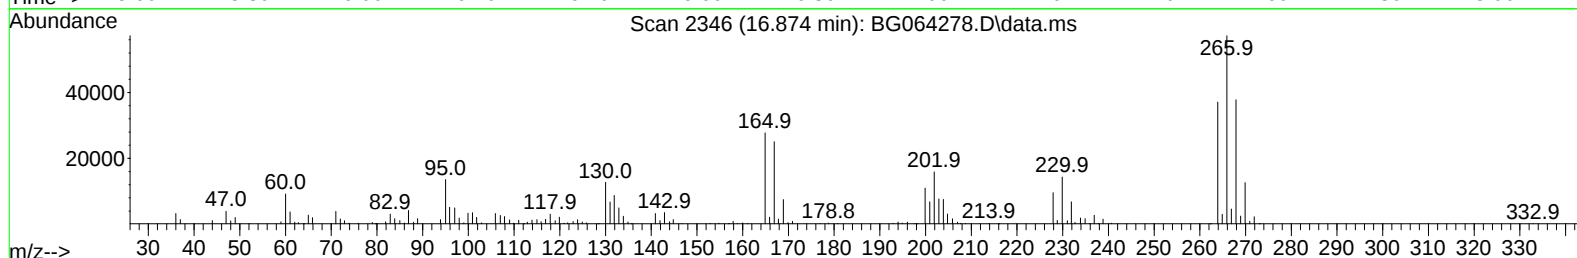


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090425\
Data File : BG064278.D
Acq On : 4 Sep 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 10:53:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

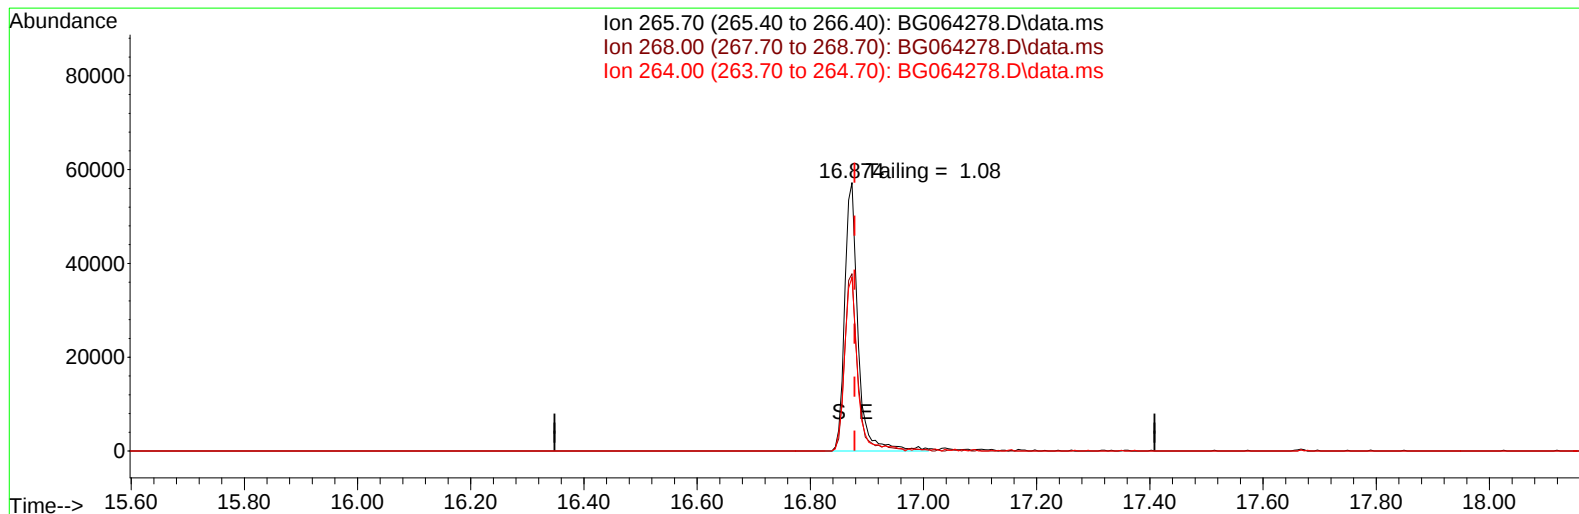

TIC: BG064278.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.004) 197424.28 ng

response 93186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	66.08
264.00	55.40	64.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090425\
Data File : BG064278.D
Acq On : 4 Sep 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 10:53:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

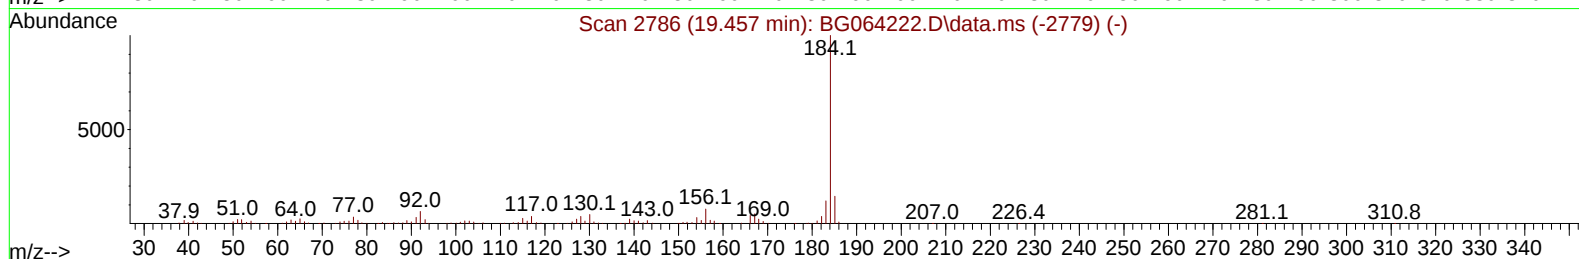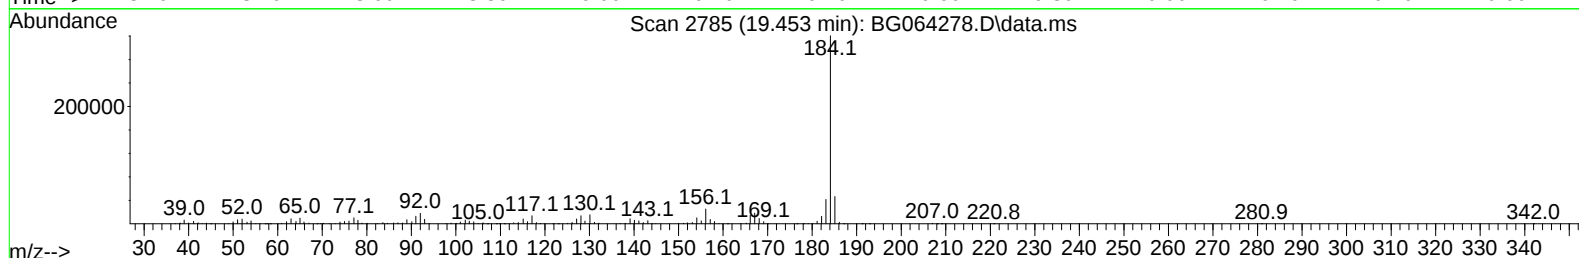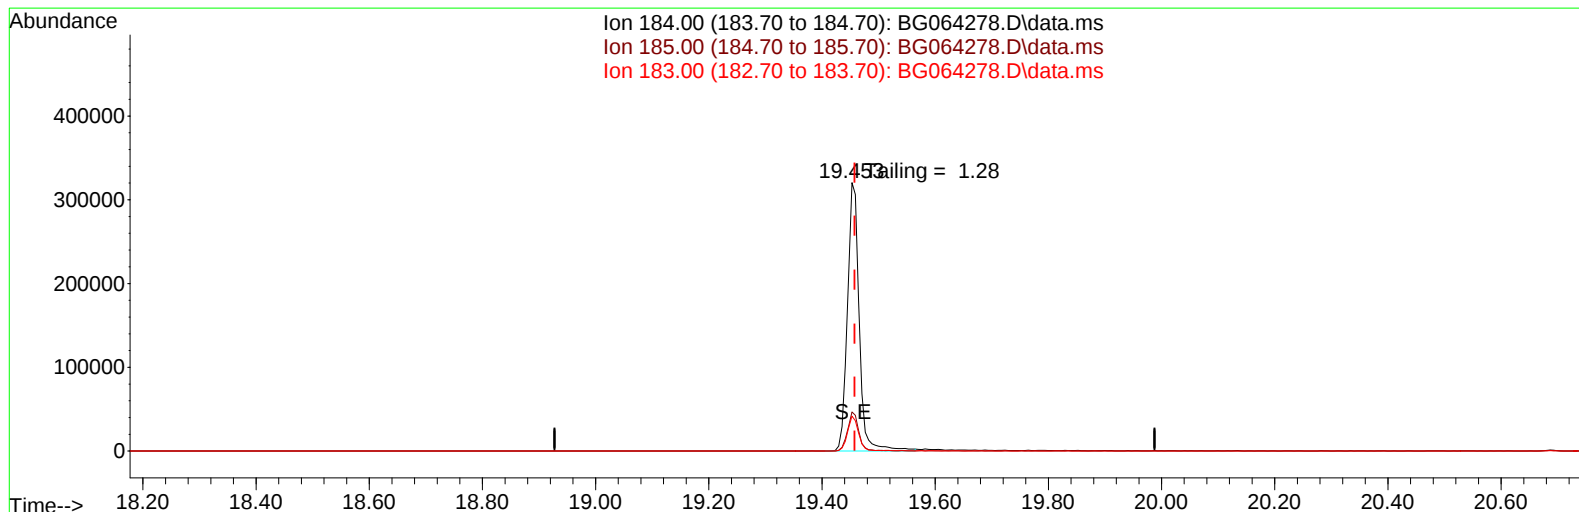

TIC: BG064278.D\data.ms

(77) Benzidine**19.453min (-0.004) 104401.69 ng****response 465604**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.55
183.00	12.10	12.99
0.00	0.00	0.00