


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090425\
Data File : BG064278.D
Acq On : 4 Sep 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

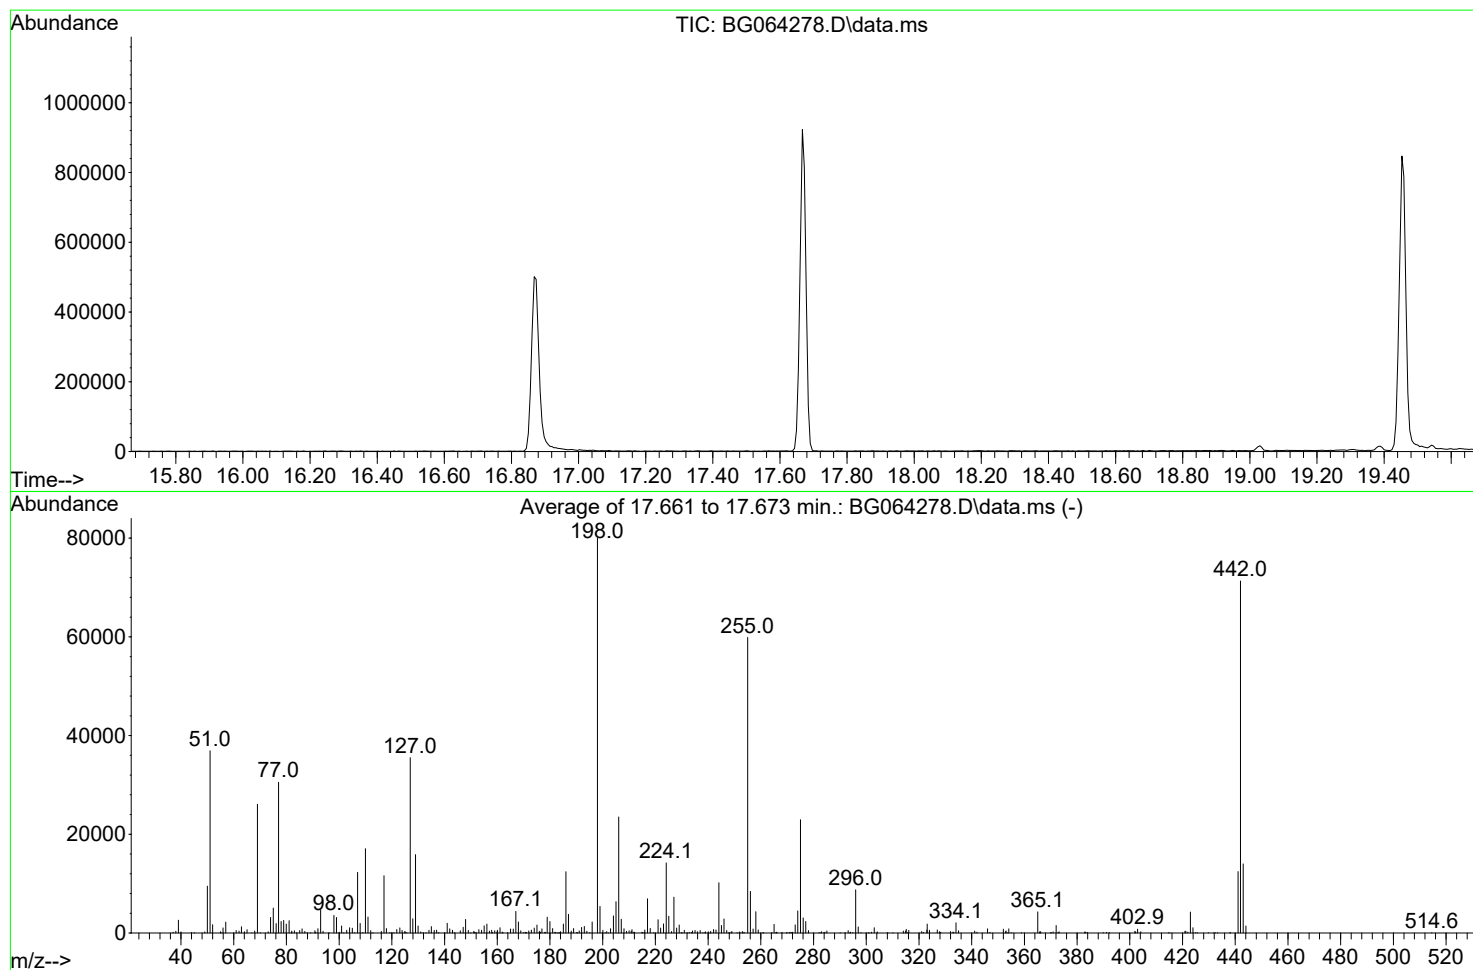

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	396	PASS
69	69	100	100	100.0	26088	PASS
70	69	0.00	2	0.3	73	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79992	PASS
199	198	5	9	6.7	5383	PASS
365	198	1	100	5.3	4274	PASS
441	443	0.01	150	88.9	12457	PASS
442	442	100	100	100.0	71304	PASS
443	442	15	24	19.6	14005	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/4/2025	BNA_G	<u>BG064278.D</u>
Compound Name	Response	Retention Time
DDT	263628	20.687
DDD	6263	20.252
DDE	58	19.964
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6321	269949	2.34

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090425\
Data File : BG064278.D
Acq On : 4 Sep 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 04 10:53:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

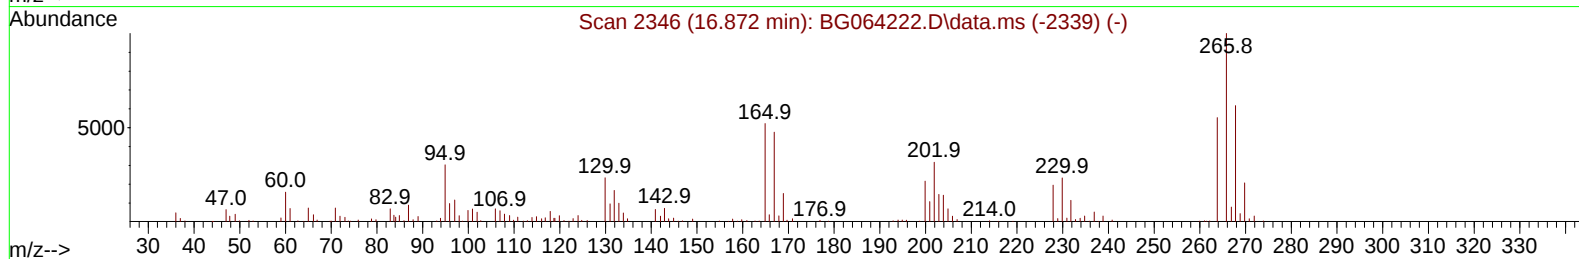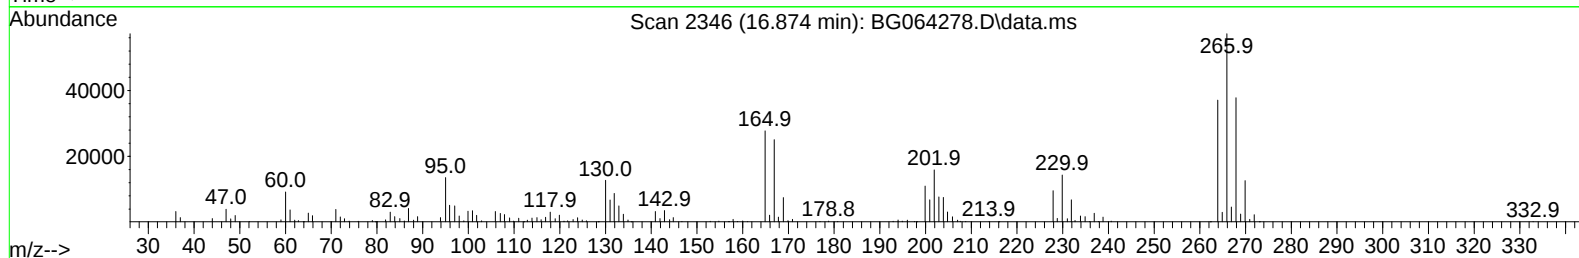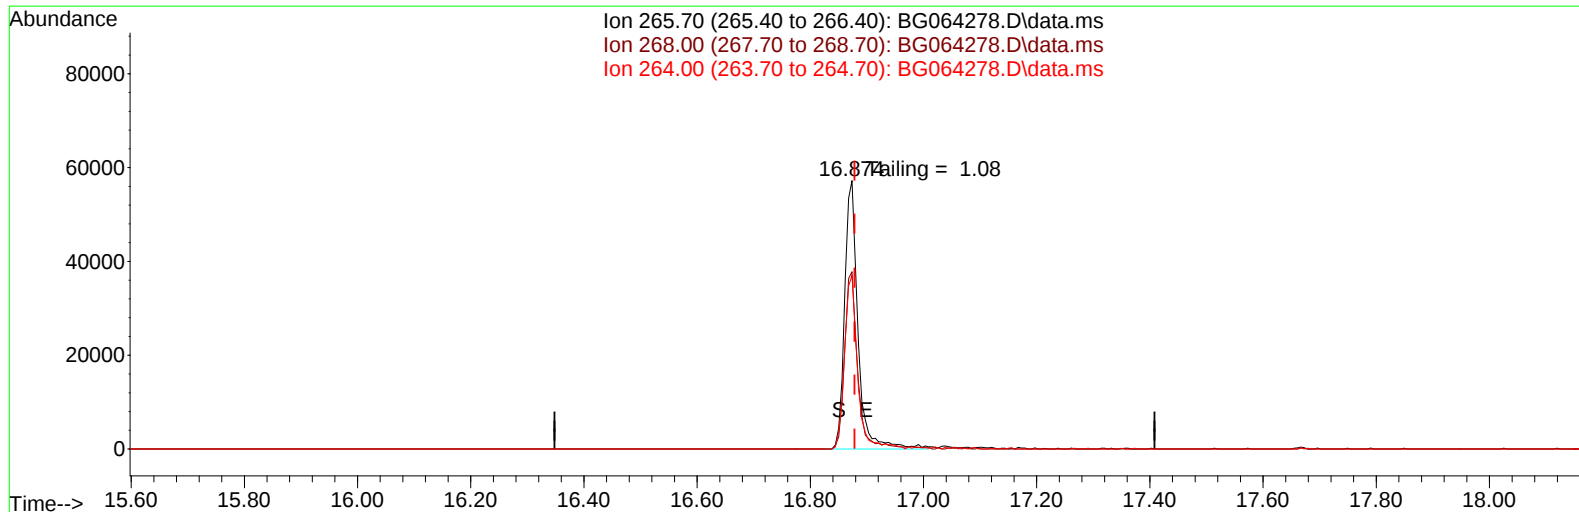

TIC: BG064278.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.004) 197424.28 ng




response 93186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	66.08
264.00	55.40	64.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090425\
Data File : BG064278.D
Acq On : 4 Sep 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 04 10:53:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

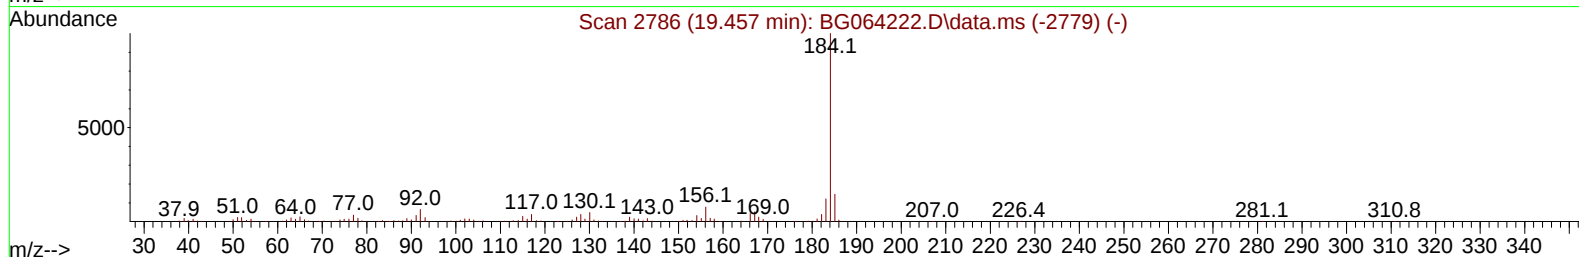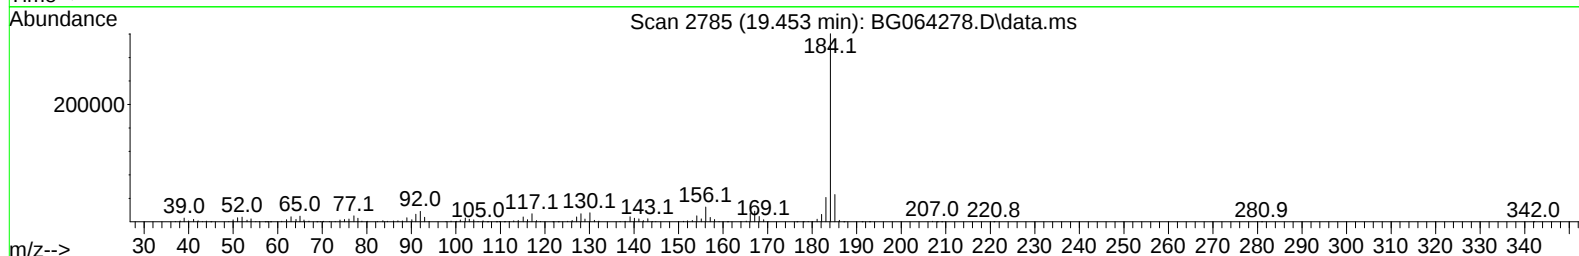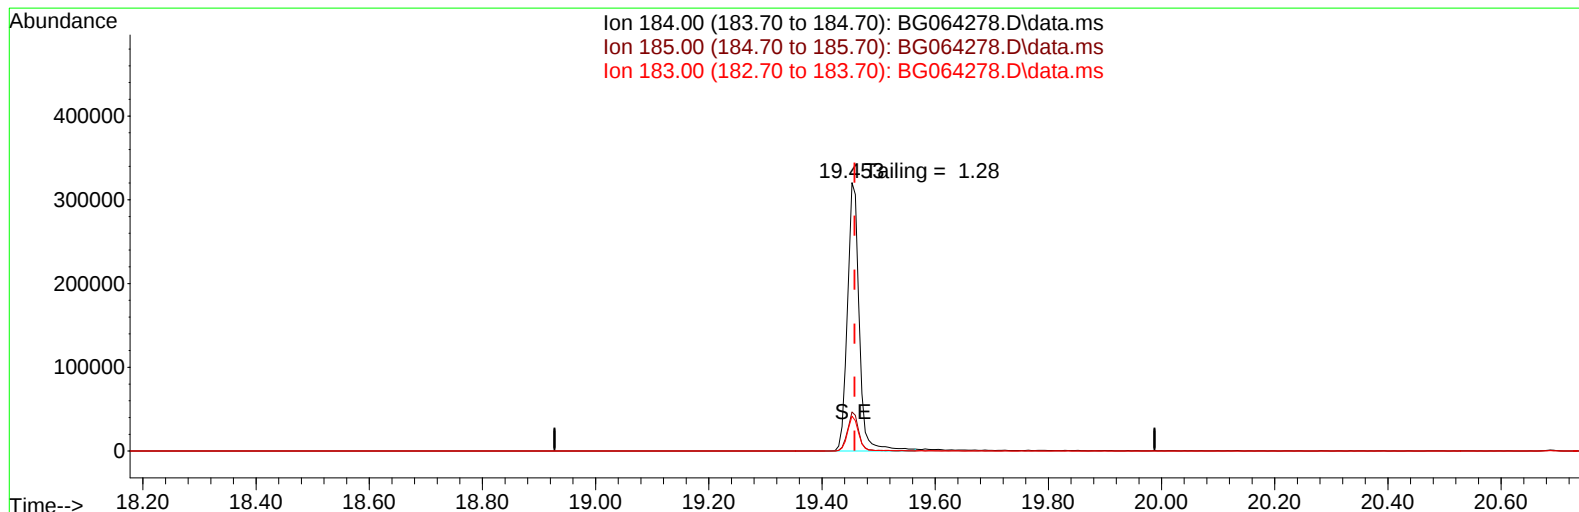

TIC: BG064278.D\data.ms

(77) Benzidine

19.453min (-0.004) 104401.69 ng

response 465604

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.55
183.00	12.10	12.99
0.00	0.00	0.00