


Data Path : Z:\HPCHEM1\BNA_G\Data\BG090517\
 Data File : BG028571.D
 Acq On : 5 Sep 2017 9:40
 Operator : SJ/JU
 Sample : DFTPP75
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP75

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION
 Last Update : Wed Sep 06 04:00:37 2017

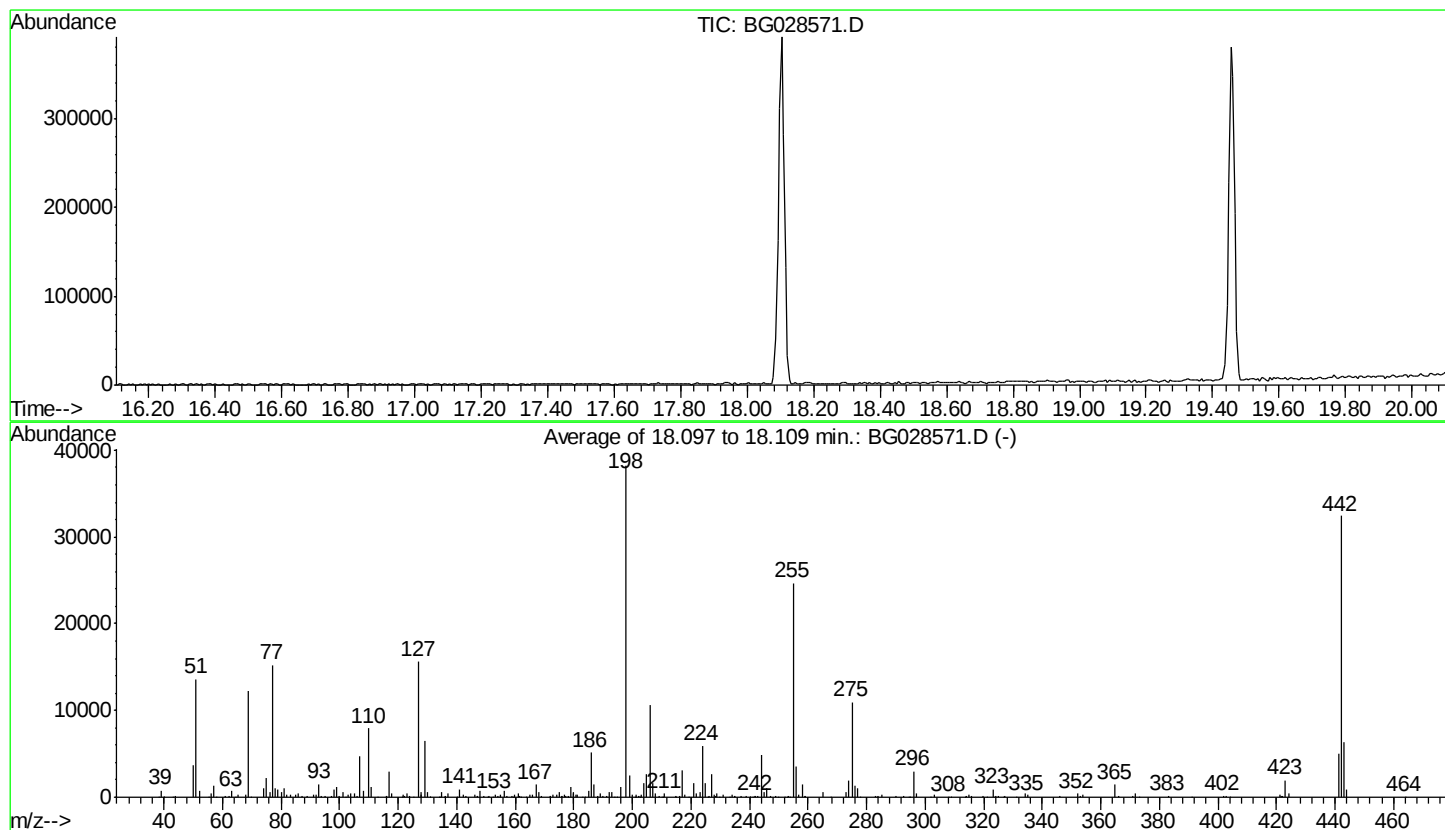

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	13642	PASS
68	69	0.00	2	1.9	231	PASS
69	198	0.00	100	31.9	12201	PASS
70	69	0.00	2	0.5	60	PASS
127	198	10	80	40.9	15629	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38224	PASS
199	198	5	9	6.5	2500	PASS
275	198	10	60	28.6	10937	PASS
365	198	1	100	3.8	1456	PASS
441	442	0.01	100	15.4	5003	PASS
442	198	50	100	84.9	32445	PASS
443	442	15	24	19.6	6363	PASS

m/z	Abundance
39.10	679.0
41.10	225.0
44.00	218.0
50.10	3885.0
51.10	14368.0
52.10	874.0
55.00	357.0
56.10	417.0
57.10	1133.0
61.00	184.0
62.10	257.0
63.10	580.0
64.30	182.0
65.20	243.0
69.00	14355.0
74.10	1383.0
75.00	2228.0
76.10	693.0
77.10	16230.0
78.10	1036.0
79.00	663.0
80.00	604.0
81.10	1328.0
82.00	150.0
83.10	285.0
85.10	430.0
86.10	360.0
91.00	254.0
92.10	403.0
93.10	1394.0
98.00	707.0
99.00	1334.0
101.10	677.0
103.00	460.0
104.00	365.0
105.10	453.0
106.00	203.0
107.00	4729.0
108.00	812.0
110.00	8170.0
111.00	985.0
113.00	190.0
115.90	320.0
117.00	3151.0
118.00	564.0
122.00	506.0
123.00	188.0
124.10	339.0
127.00	15380.0
127.90	959.0
129.00	6322.0
130.10	565.0
131.10	235.0
134.00	192.0
135.10	525.0
137.10	418.0
140.00	180.0
141.00	913.0
142.10	382.0
143.10	151.0
146.20	604.0
146.90	264.0
147.10	252.0
148.00	855.0
149.10	295.0
150.40	172.0
150.90	215.0
152.40	168.0
153.10	273.0
154.90	361.0
156.10	853.0
157.00	179.0
160.00	292.0
161.10	627.0
163.90	239.0
165.10	494.0
166.00	377.0
167.00	1507.0
168.00	436.0
171.80	363.0
173.00	383.0
174.00	183.0
175.00	466.0
175.90	230.0
176.90	354.0
177.90	206.0
179.00	1302.0
179.90	1172.0
180.90	708.0
183.90	186.0
185.00	746.0

Instrument :
BNA_G
ClientSampleId :
DFTPP75

186.00	5605.0
187.00	1539.0
188.10	220.0
189.00	462.0
191.20	220.0
192.00	653.0
193.10	540.0
196.10	778.0
198.00	33704.0
198.90	2405.0
200.10	205.0
201.20	662.0
202.10	257.0
202.90	295.0
204.00	1807.0
205.00	2576.0
206.00	9383.0
207.10	1778.0
207.90	360.0
209.10	292.0
210.10	172.0
211.00	293.0
214.80	207.0
217.00	2825.0
218.10	230.0
221.00	1604.0
222.00	304.0
223.10	578.0
224.00	4601.0
225.00	1596.0
227.00	2849.0
228.00	269.0
229.00	578.0
229.90	153.0
231.00	190.0
233.10	167.0
234.00	334.0
234.80	462.0
237.10	229.0
240.00	190.0
241.10	187.0
241.90	327.0
244.10	4196.0
245.00	647.0
246.10	1036.0
247.10	326.0
248.90	178.0
252.20	224.0
255.00	23880.0
256.00	3200.0
257.00	237.0
258.00	1742.0
258.90	547.0
265.10	507.0
267.60	193.0
273.00	462.0
274.00	1775.0
275.10	10232.0
276.00	1133.0
277.00	903.0
283.30	205.0
285.00	302.0
292.80	194.0
296.00	2799.0
297.10	470.0
302.00	206.0
303.10	279.0
308.10	203.0
314.00	253.0
315.00	189.0
319.80	159.0
323.10	739.0
323.70	225.0
324.20	248.0
327.10	209.0
331.20	177.0
334.00	320.0
346.00	174.0
351.90	486.0
353.10	255.0
354.00	366.0
365.00	1448.0
371.90	340.0
391.00	198.0
422.10	378.0
423.10	1468.0
424.10	384.0
441.10	4071.0
442.10	24024.0
443.10	5250.0
444.10	948.0

Instrument :
BNA_G
ClientSampleId :
DFTPP75

m/z	Abundance
38.00	164.0
39.10	1193.0
39.80	174.0
43.10	160.0
44.10	523.0
50.10	4060.0
51.10	15899.0
52.10	834.0
55.10	162.0
56.10	549.0
57.10	1817.0
57.90	182.0
61.10	173.0
63.10	688.0
65.10	415.0
68.10	332.0
69.00	13943.0
69.90	181.0
73.00	232.0
74.10	1198.0
75.00	2798.0
76.10	592.0
77.10	18528.0
78.10	934.0
79.10	1049.0
80.00	869.0
81.00	1419.0
82.00	426.0
83.00	430.0
85.00	201.0
86.10	482.0
87.00	174.0
88.90	168.0
91.00	466.0
92.00	215.0
93.00	1982.0
93.90	220.0
98.00	1215.0
99.10	1418.0
100.10	178.0
101.10	637.0
102.00	178.0
103.00	238.0
103.90	565.0
105.00	332.0
106.10	161.0
107.00	5701.0
108.10	1066.0
110.00	9679.0
111.00	1473.0
116.10	306.0
117.10	3323.0
117.90	416.0
121.30	195.0
121.80	356.0
123.00	606.0
124.10	248.0
125.00	171.0
127.10	18656.0
128.10	1173.0
129.10	7637.0
130.00	730.0
130.80	150.0
134.20	164.0
135.00	530.0
136.20	395.0
137.10	473.0
141.10	814.0
142.10	199.0
143.10	271.0
146.00	158.0
147.00	475.0
148.00	1015.0
151.00	219.0
152.90	319.0
154.10	210.0
155.10	480.0
156.10	921.0
156.90	250.0
158.90	240.0
159.90	429.0
161.20	432.0
161.40	455.0
164.90	283.0
166.10	440.0
167.00	1584.0
168.10	676.0
168.90	248.0
172.10	157.0
173.00	265.0
174.00	575.0

Instrument :
BNA_G
ClientSampleId :
DFTPP75

174.90	866.0
176.10	410.0
176.90	559.0
178.10	266.0
179.00	1108.0
180.10	1082.0
181.10	589.0
183.10	170.0
185.00	1043.0
186.00	5549.0
187.00	1635.0
188.10	433.0
189.00	515.0
190.10	243.0
191.20	222.0
192.10	835.0
192.90	578.0
194.90	236.0
196.00	1769.0
198.00	47400.0
198.90	2707.0
200.10	335.0
200.90	165.0
201.50	238.0
202.30	299.0
203.00	279.0
204.10	2068.0
205.00	2961.0
206.10	13524.0
207.10	2092.0
208.00	512.0
211.10	490.0
215.00	338.0
216.00	316.0
217.00	3371.0
218.10	457.0
219.10	159.0
221.10	1953.0
221.90	661.0
223.00	607.0
224.00	7968.0
225.00	1687.0
225.90	239.0
227.10	2948.0
228.20	363.0
229.00	509.0
231.10	494.0
234.10	284.0
235.10	405.0
237.10	339.0
240.30	184.0
242.10	431.0
244.10	5092.0
245.00	657.0
246.00	1026.0
249.90	164.0
253.40	369.0
255.00	28696.0
256.00	4272.0
257.00	472.0
258.00	1640.0
259.10	241.0
265.00	761.0
273.00	820.0
274.00	2117.0
275.00	13295.0
276.00	1660.0
276.90	987.0
278.00	150.0
283.00	155.0
284.10	262.0
285.10	376.0
289.90	249.0
294.50	163.0
295.00	153.0
296.00	3542.0
296.90	491.0
303.10	339.0
308.90	166.0
315.10	235.0
316.00	300.0
321.00	228.0
323.10	1222.0
324.90	269.0
327.00	228.0
334.10	707.0
335.10	257.0
345.90	157.0
352.00	349.0
353.00	360.0
353.90	393.0
365.00	1374.0
366.10	264.0
371.00	169.0
371.90	359.0

Instrument :
BNA_G
ClientSampleId :
DFTPP75

383.00	415.0
401.90	328.0
403.00	404.0
404.20	232.0
421.00	505.0
421.80	161.0
423.00	2109.0
423.90	400.0
441.10	5659.0
442.10	39824.0
443.10	7550.0
444.00	920.0
463.90	166.0

Instrument :
BNA_G
ClientSampleId :
DFTPP75

m/z	Abundance
39.20	363.0
40.10	161.0
44.10	730.0
50.10	2995.0
51.10	10659.0
52.00	501.0
55.40	180.0
56.10	589.0
57.00	892.0
61.10	160.0
63.10	942.0
65.10	280.0
68.20	362.0
69.00	8889.0
73.10	167.0
74.00	675.0
75.00	1455.0
76.10	519.0
77.10	10982.0
78.10	939.0
79.10	874.0
80.00	311.0
81.00	899.0
82.00	265.0
83.00	265.0
84.90	178.0
85.90	417.0
87.00	209.0
89.00	159.0
92.00	267.0
93.00	1123.0
94.00	229.0
95.10	253.0
97.10	244.0
98.00	767.0
99.00	683.0
100.00	203.0
101.00	492.0
103.00	241.0
104.10	200.0
105.10	692.0
107.00	3560.0
108.00	457.0
110.00	5927.0
111.00	1030.0
116.00	248.0
117.00	2527.0
118.00	228.0
122.10	305.0
123.00	402.0
127.00	12851.0
128.00	791.0
129.00	5436.0
130.10	277.0
135.00	543.0
135.80	215.0
137.00	307.0
141.00	1044.0
142.20	270.0
142.90	255.0
147.00	426.0
148.10	582.0
151.10	184.0
153.00	324.0
154.00	304.0
154.90	523.0
156.00	455.0
159.20	197.0
160.00	254.0
161.10	319.0
162.00	182.0
164.90	194.0
167.00	1204.0
168.00	720.0
172.00	288.0
172.80	186.0
174.10	224.0
175.00	653.0
175.80	158.0
177.20	244.0
178.00	222.0
179.00	1307.0
180.00	907.0
181.10	362.0
184.90	340.0
186.00	4134.0
187.10	1297.0
189.00	193.0
192.10	513.0
193.10	501.0
193.80	202.0

Instrument :
BNA_G
ClientSampleId :
DFTPP75

196.00	1077.0
198.00	33568.0
199.00	2390.0
200.00	228.0
201.20	173.0
202.50	226.0
202.90	252.0
204.00	1033.0
205.00	2500.0
206.10	8898.0
207.10	1642.0
208.00	335.0
210.40	221.0
211.00	341.0
217.00	3233.0
217.90	189.0
221.00	1155.0
222.00	279.0
223.00	685.0
224.00	5191.0
225.00	1476.0
226.30	248.0
227.00	2224.0
228.00	510.0
228.90	426.0
230.90	260.0
234.20	285.0
239.10	326.0
242.00	165.0
242.80	338.0
244.00	5321.0
245.10	423.0
246.00	887.0
247.20	160.0
249.00	251.0
253.00	230.0
253.80	232.0
255.00	21520.0
256.00	3208.0
258.00	1185.0
259.00	324.0
265.00	409.0
273.00	363.0
274.10	1900.0
275.00	9284.0
276.00	1158.0
277.10	1220.0
282.90	164.0
285.10	223.0
292.90	153.0
296.00	2560.0
297.00	474.0
303.10	276.0
313.70	217.0
315.00	370.0
319.70	250.0
323.00	782.0
324.00	184.0
326.80	168.0
334.00	512.0
335.00	506.0
352.00	381.0
354.00	267.0
365.00	1547.0
366.00	188.0
371.00	157.0
372.00	487.0
373.10	207.0
382.90	224.0
401.80	258.0
421.10	250.0
421.80	309.0
423.00	2415.0
424.10	351.0
441.10	5280.0
442.00	33488.0
443.00	6289.0
443.90	647.0

Instrument :
BNA_G
ClientSampleId :
DFTPP75

Scan 2463 (18.062 min): BG028571.D
DFTPP75

m/z	Abundance
41.10	167.0
44.00	321.0
49.00	159.0
54.90	237.0
69.20	194.0
71.20	174.0
73.20	167.0
81.00	212.0
147.10	168.0
207.00	281.0

Instrument :
BNA_G
ClientSampleId :
DFTPP75