
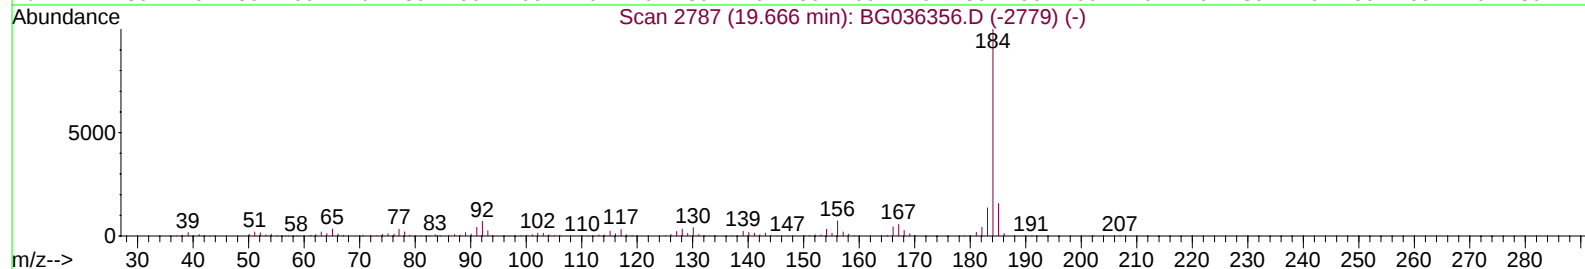
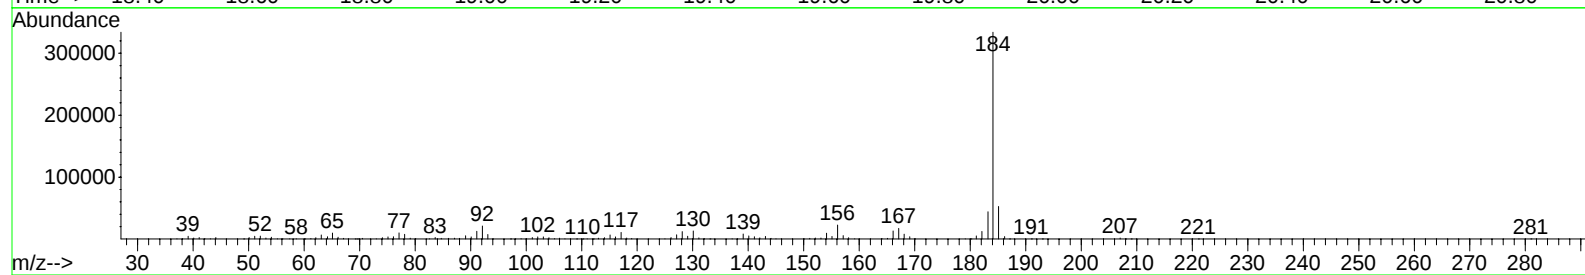


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090518\
Data File : BG036561.D
Acq On : 5 Sep 2018 14:57
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 17:44:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

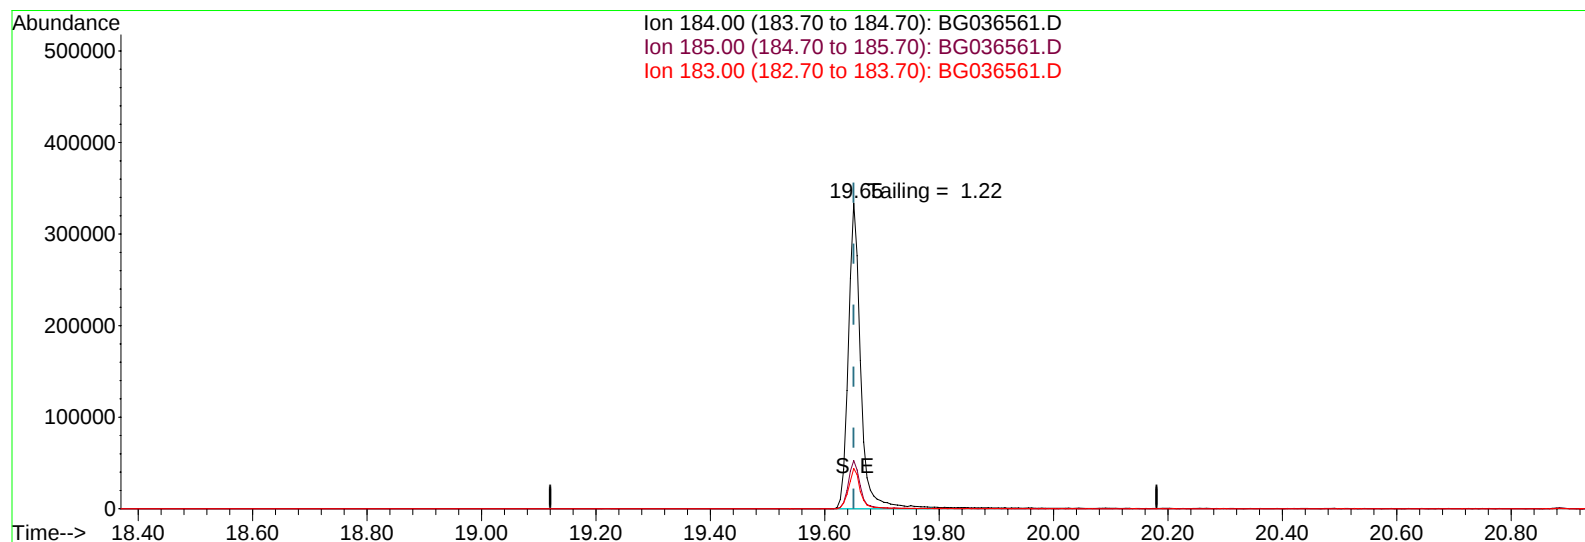

TIC: BG036561.D

(76) Benzidine




19.651min (+0.000) 12750.16ng

response 495060

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.73
183.00	13.60	13.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090518\
Data File : BG036561.D
Acq On : 5 Sep 2018 14:57
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 17:44:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

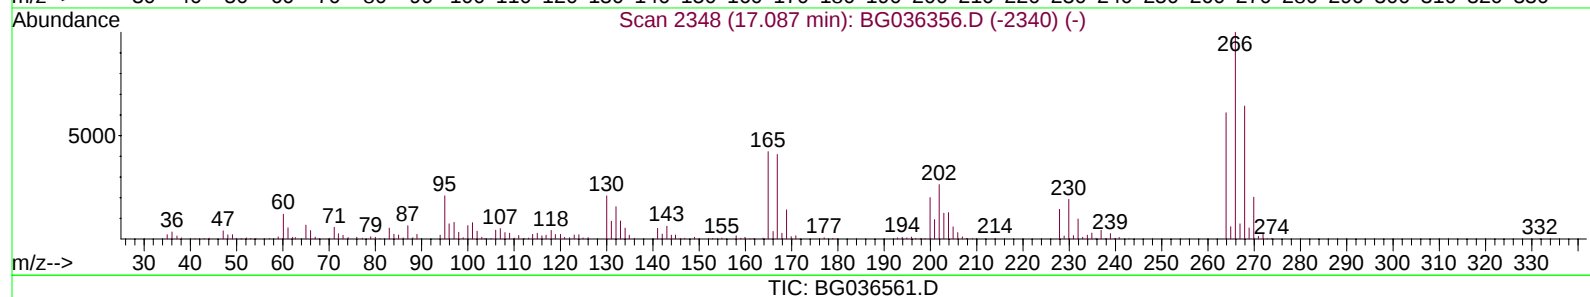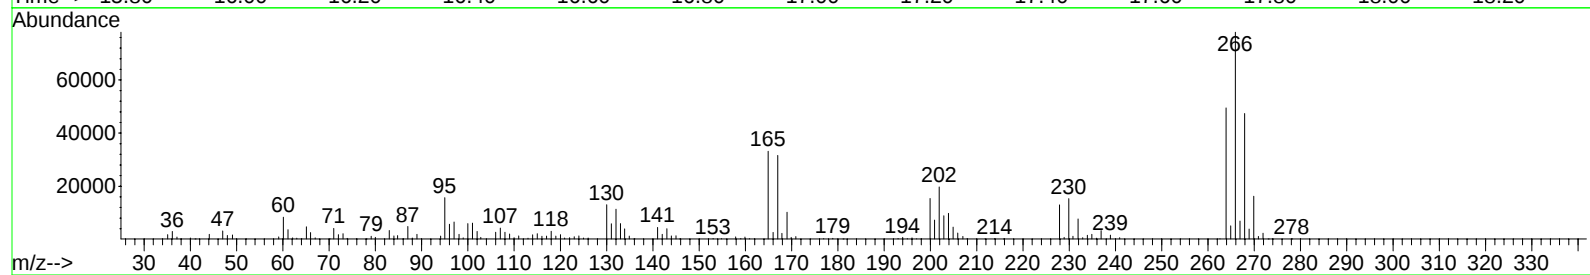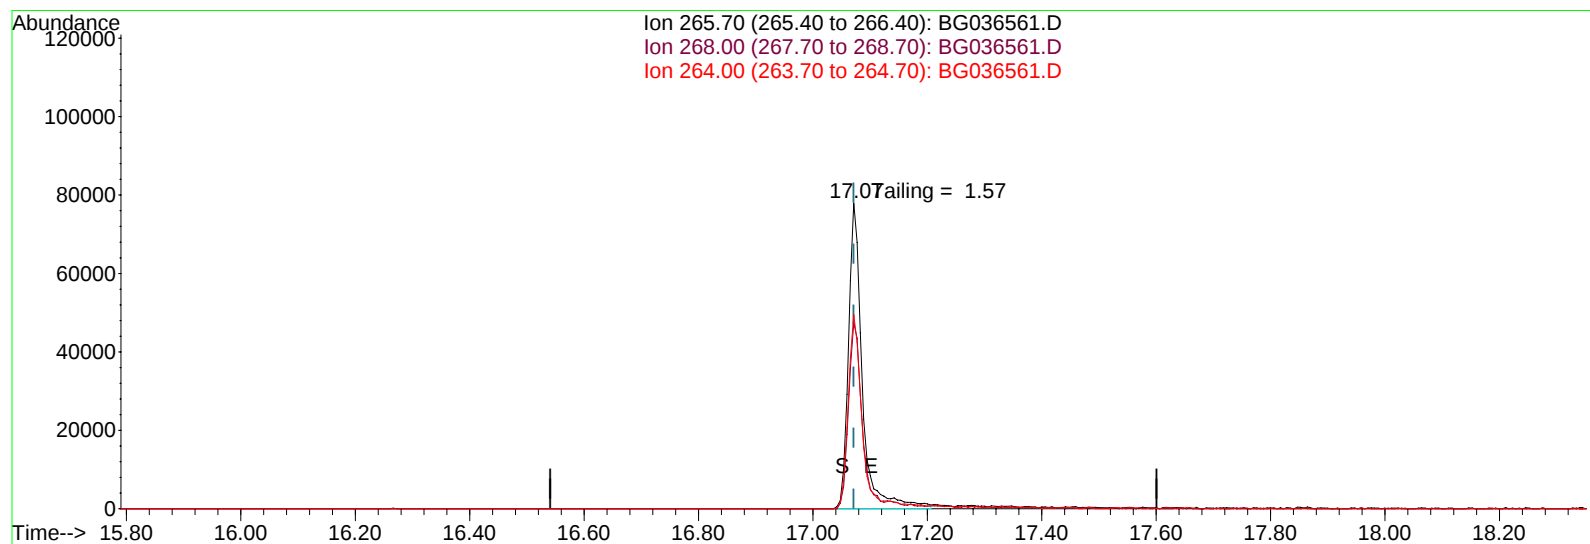

(69) Pentachlorophenol (C)

17.071min (+0.000) 12392.17ng

response 134707

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	60.74
264.00	61.10	63.46
0.00	0.00	0.00