


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090518\
 Data File : BG036561.D
 Acq On : 5 Sep 2018 14:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

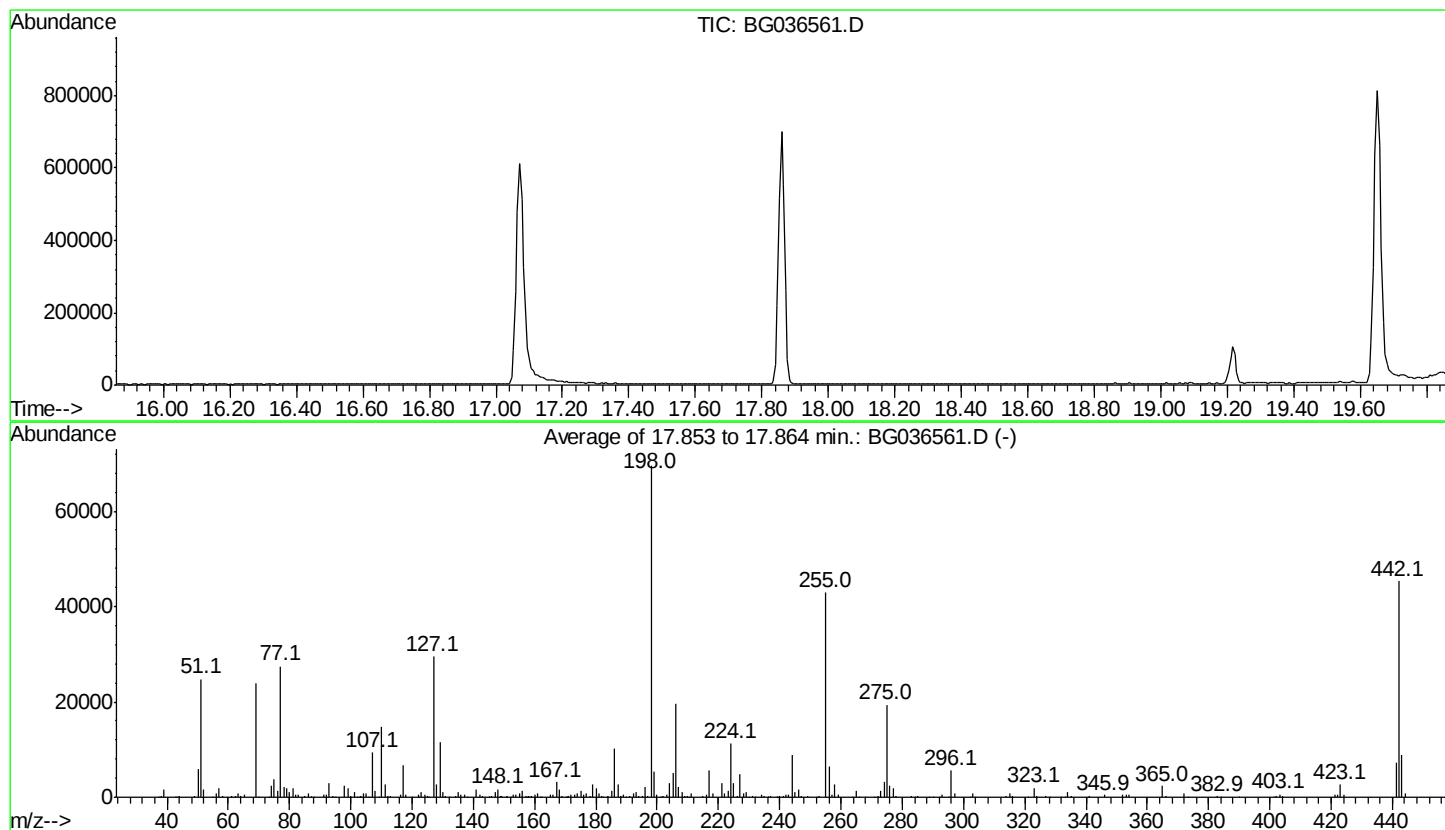

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	24712	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.4	23938	PASS
70	69	0.00	2	0.3	80	PASS
127	198	10	80	42.3	29461	PASS
197	198	0.00	2	0.4	256	PASS
198	198	100	100	100.0	69568	PASS
199	198	5	9	7.6	5302	PASS
275	198	10	60	27.8	19345	PASS
365	198	1	100	3.4	2387	PASS
441	198	0.01	100	10.4	7247	PASS
442	198	50	100	65.1	45280	PASS
443	442	15	24	19.5	8840	PASS