
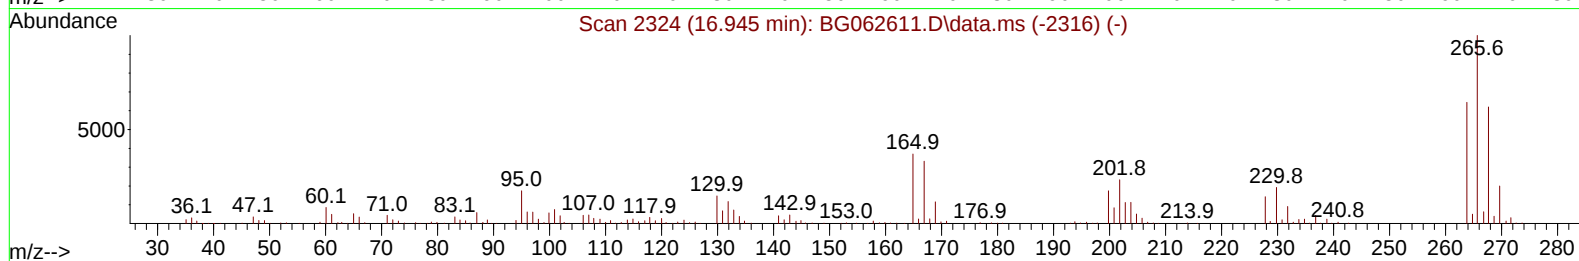
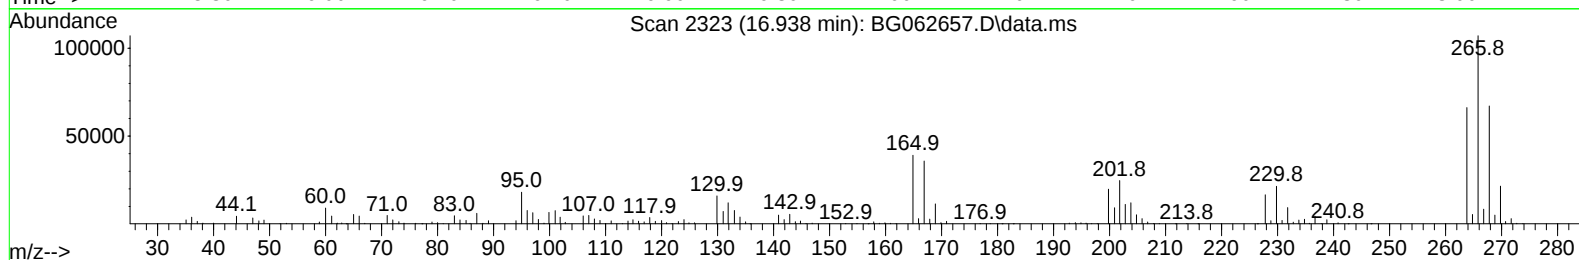


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090524\
Data File : BG062657.D
Acq On : 5 Sep 2024 8:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 11:09:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

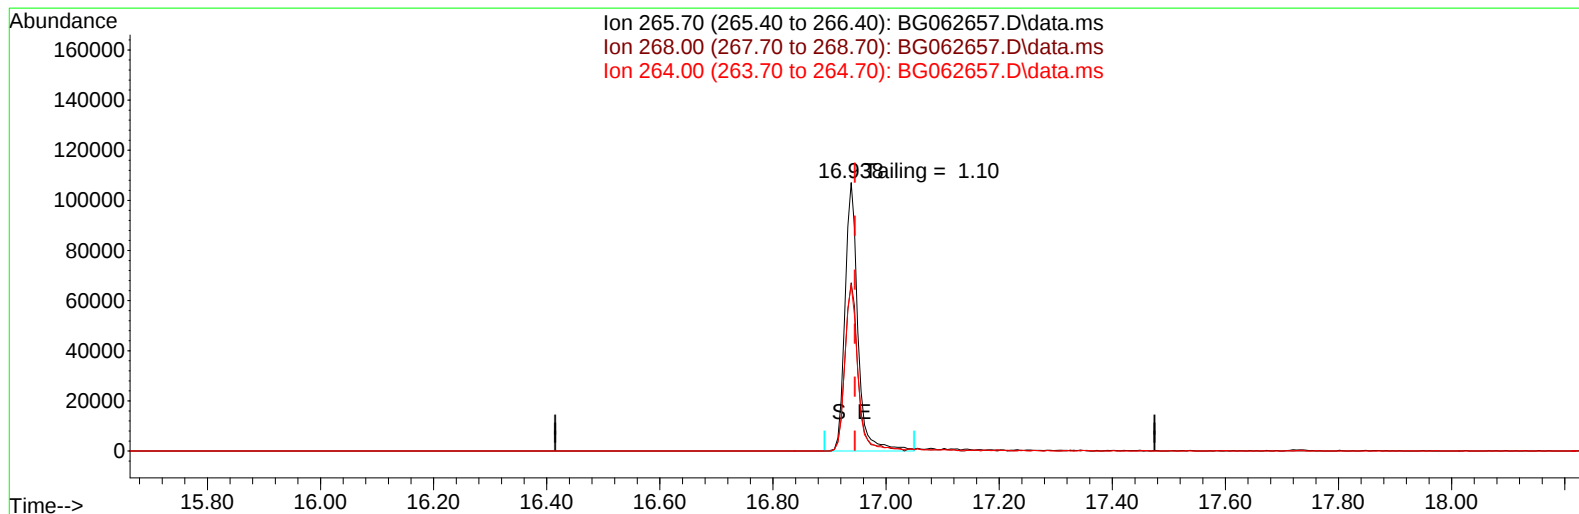

TIC: BG062657.D\data.ms

(70) Pentachlorophenol (C)




16.938min (-0.007) 0.00 ng

response 170111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.69
264.00	64.50	61.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090524\
Data File : BG062657.D
Acq On : 5 Sep 2024 8:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 11:09:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

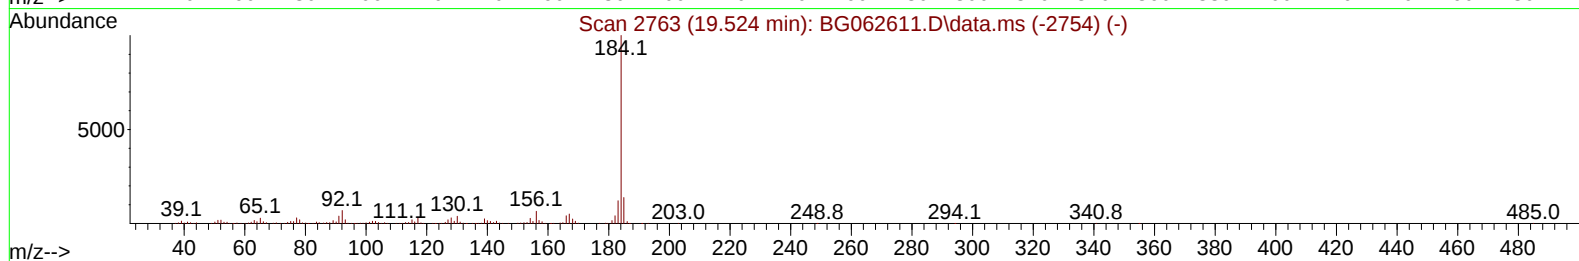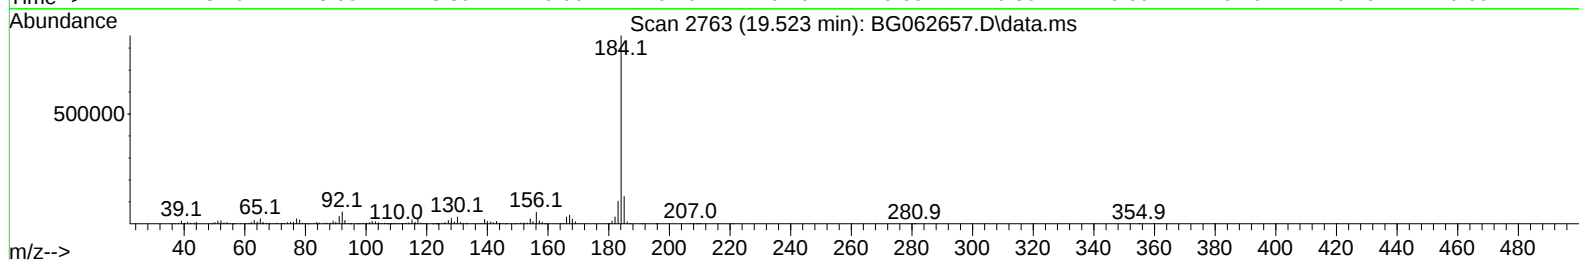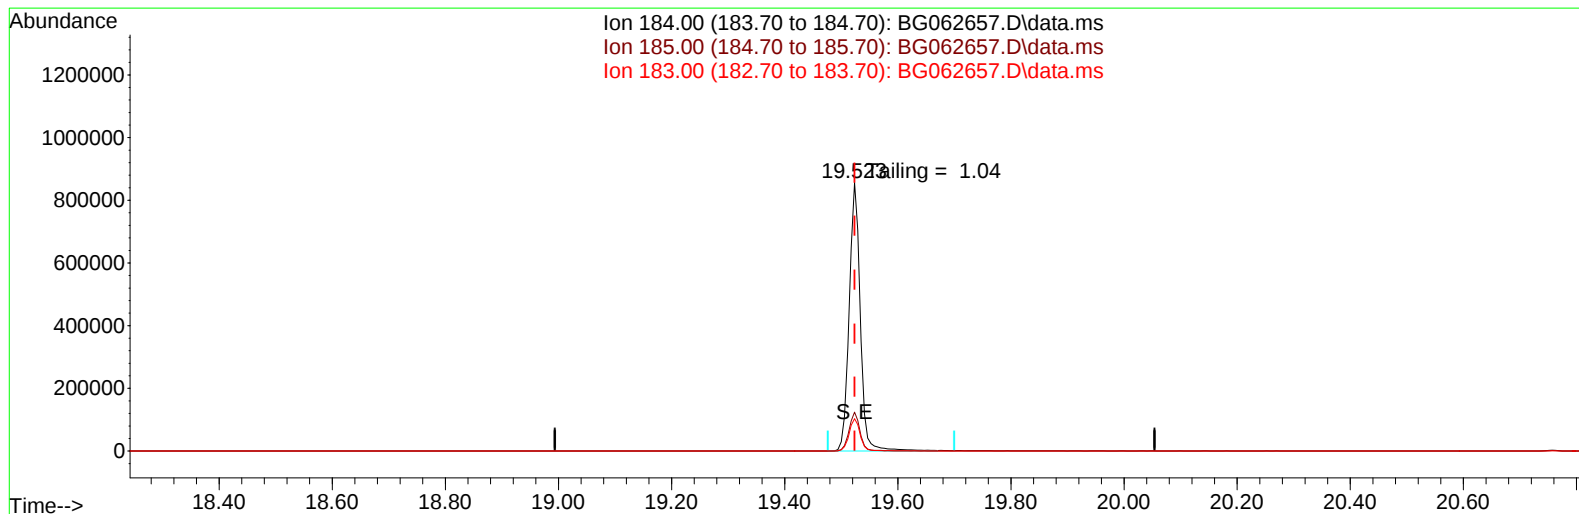

TIC: BG062657.D\data.ms

(77) Benzidine

19.523min (-0.001) 0.00 ng

response 1174680

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.51
183.00	12.10	12.06
0.00	0.00	0.00