
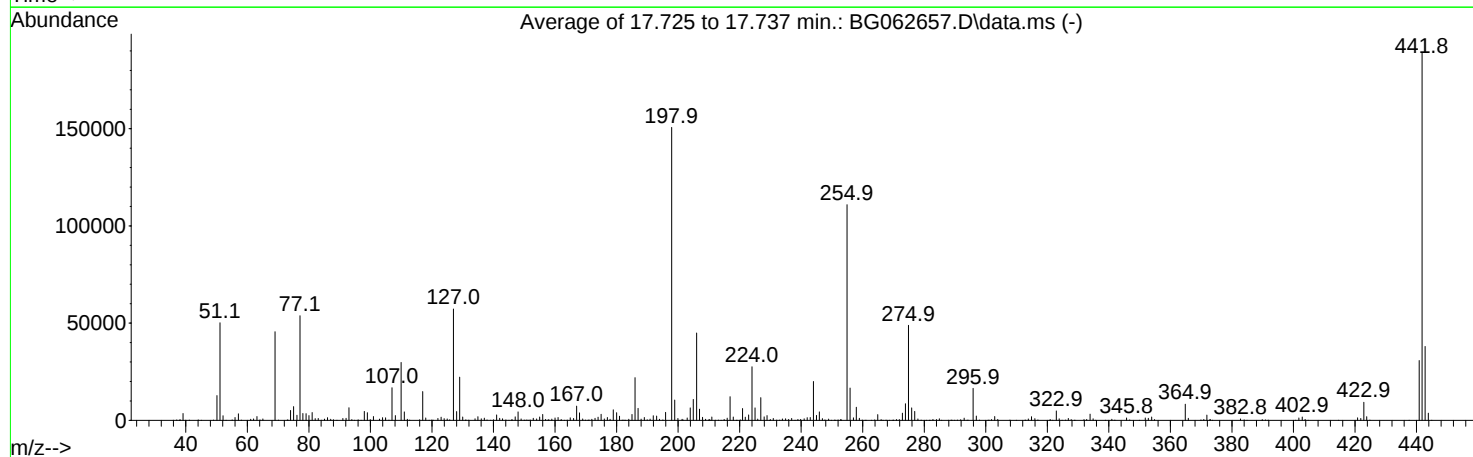


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090524\
Data File : BG062657.D
Acq On : 5 Sep 2024 8:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 31 02:36:01 2024

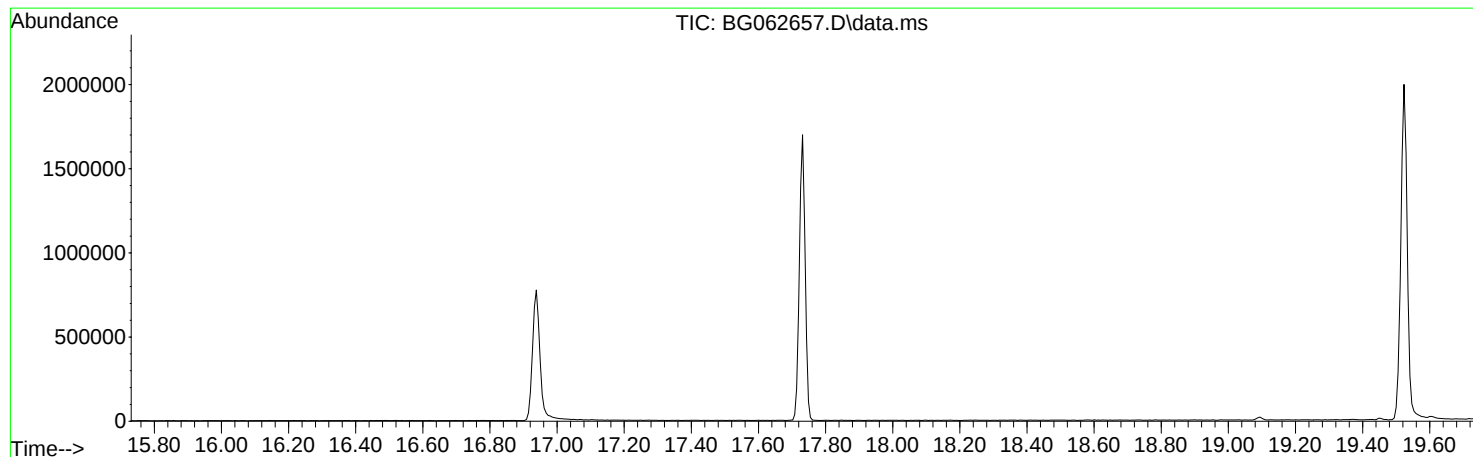




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	50179	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.2	45560	PASS
70	69	0.00	2	0.4	190	PASS
127	198	10	80	38.0	57291	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	150643	PASS
199	198	5	9	6.9	10457	PASS
275	198	10	60	32.4	48864	PASS
365	198	1	100	5.5	8331	PASS
441	198	0.01	100	20.4	30797	PASS
442	442	50	100	100.0	189184	PASS
443	442	15	24	20.1	38008	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090524\
Data File : BG062657.D
Acq On : 5 Sep 2024 8:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 05 11:09:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

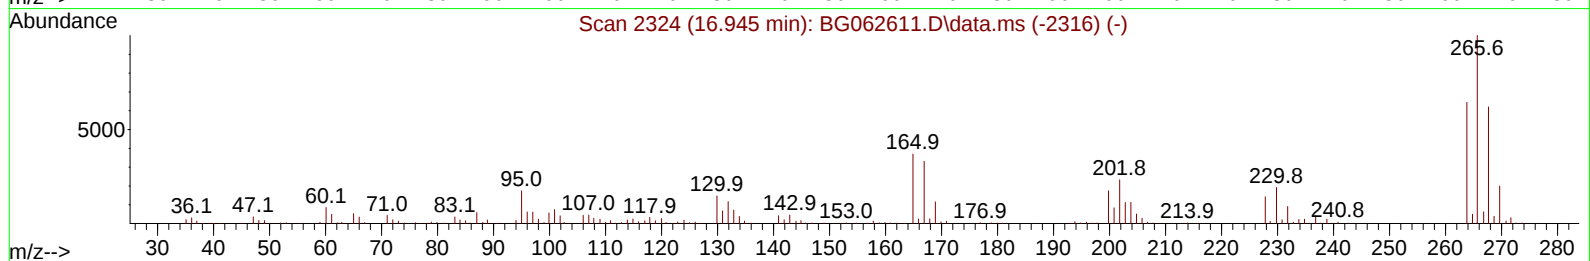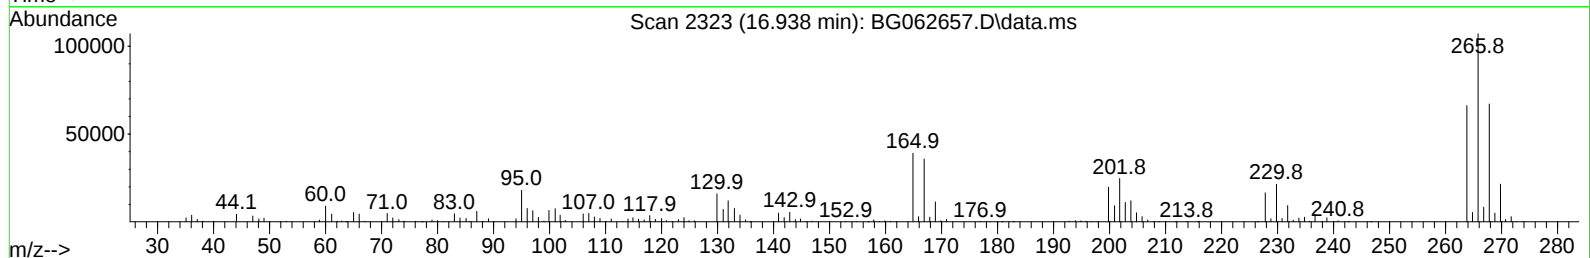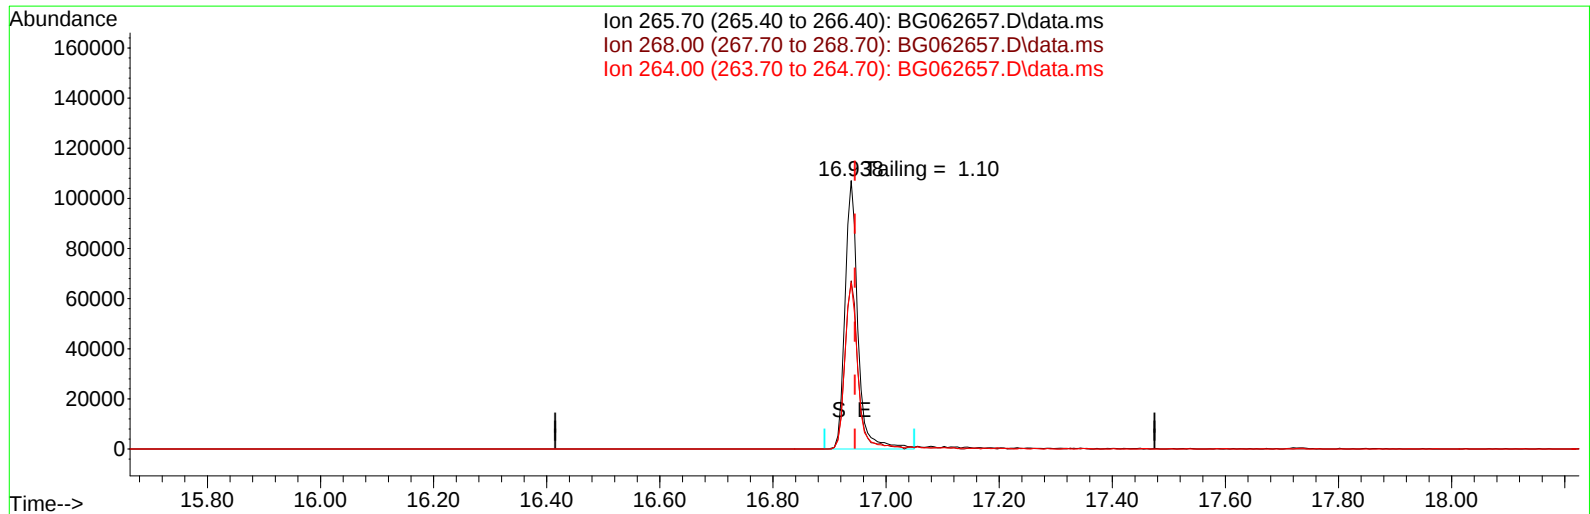

TIC: BG062657.D\data.ms

(70) Pentachlorophenol (C)

16.938min (-0.007) 0.00 ng




response 170111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.69
264.00	64.50	61.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090524\
Data File : BG062657.D
Acq On : 5 Sep 2024 8:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 05 11:09:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

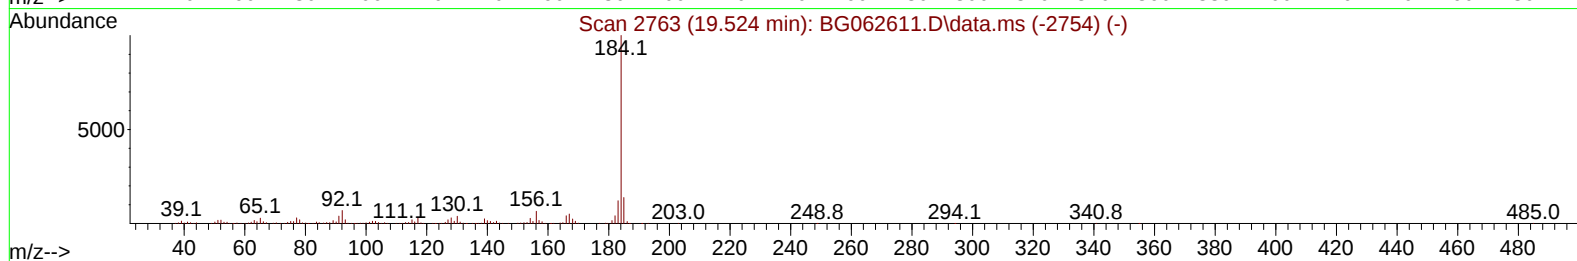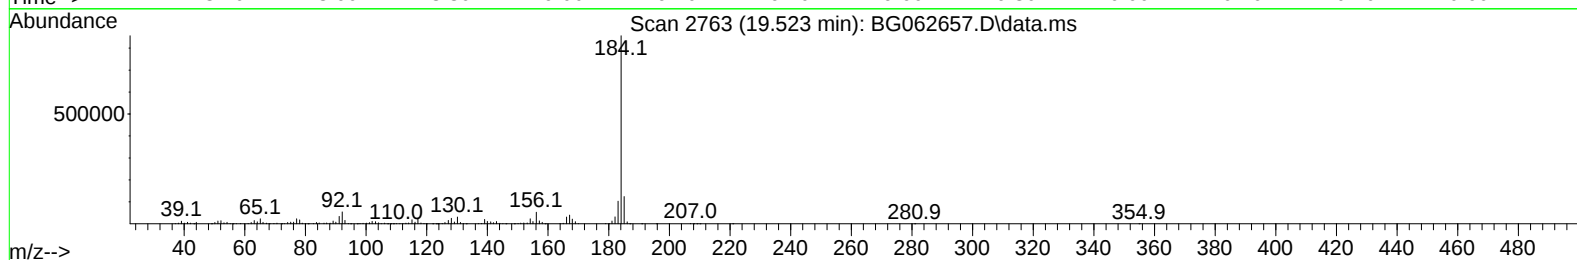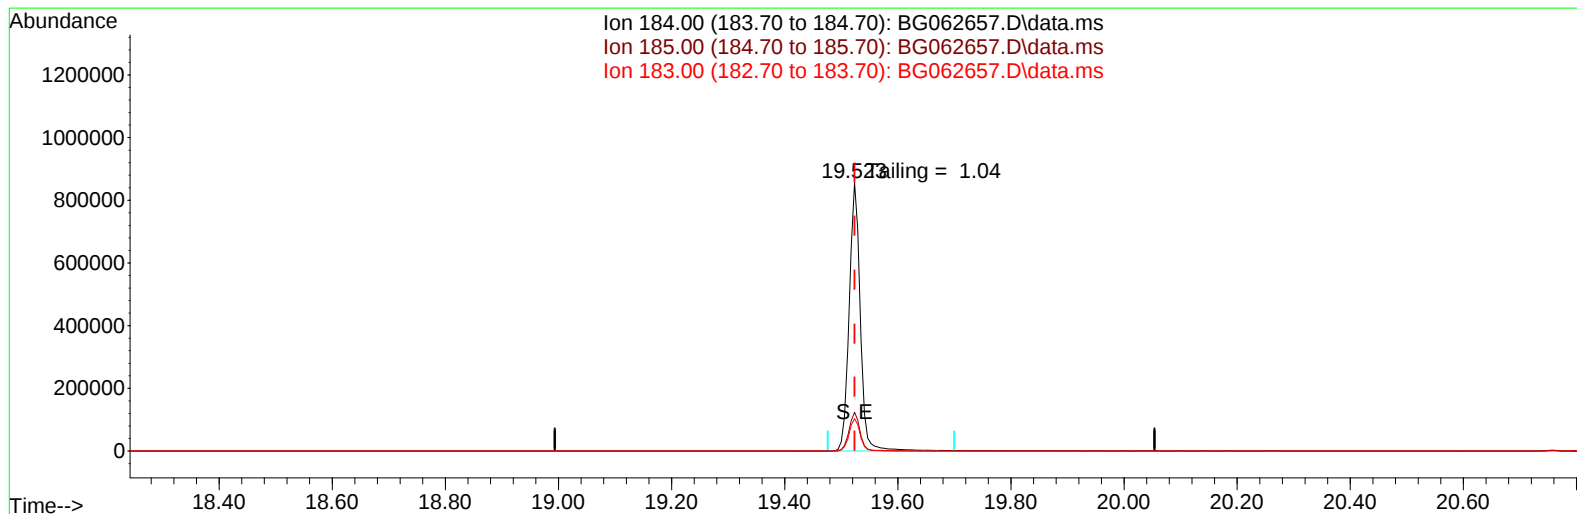

TIC: BG062657.D\data.ms

(77) Benzidine

19.523min (-0.001) 0.00 ng

response 1174680

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.51
183.00	12.10	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/5/2024	BNA_G	<u>BG062657.D</u>
Compound Name	Response	Retention Time
DDT	543064	20.757
DDD	13686	20.317
DDE	534	19.811
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14220	557284	2.55

Instrument :
BNA_G
ClientSampleId :
DFTPP