
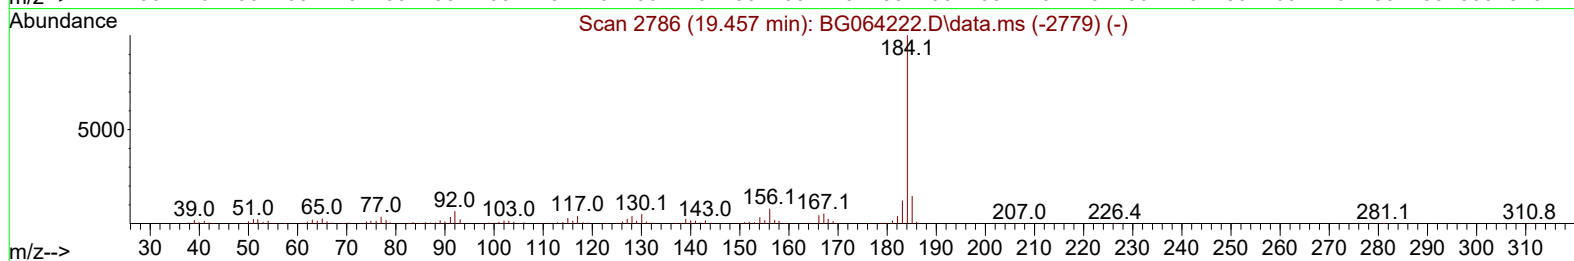
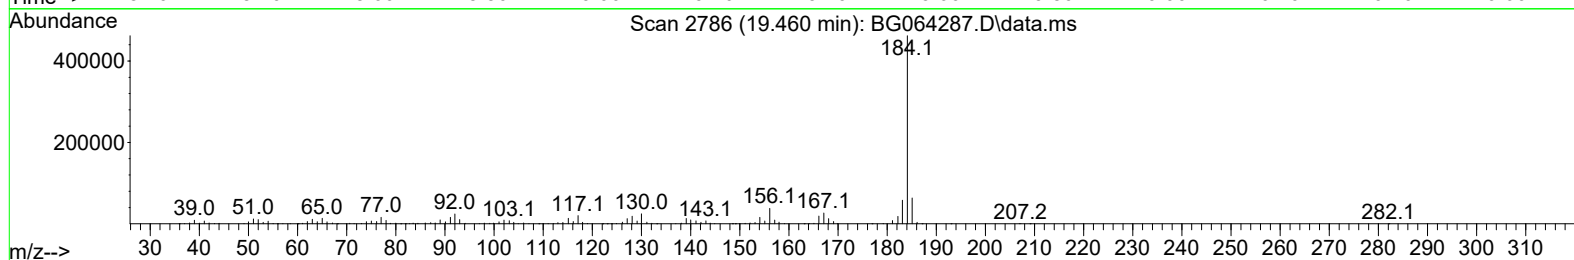


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090525\
Data File : BG064287.D
Acq On : 5 Sep 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 12:43:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

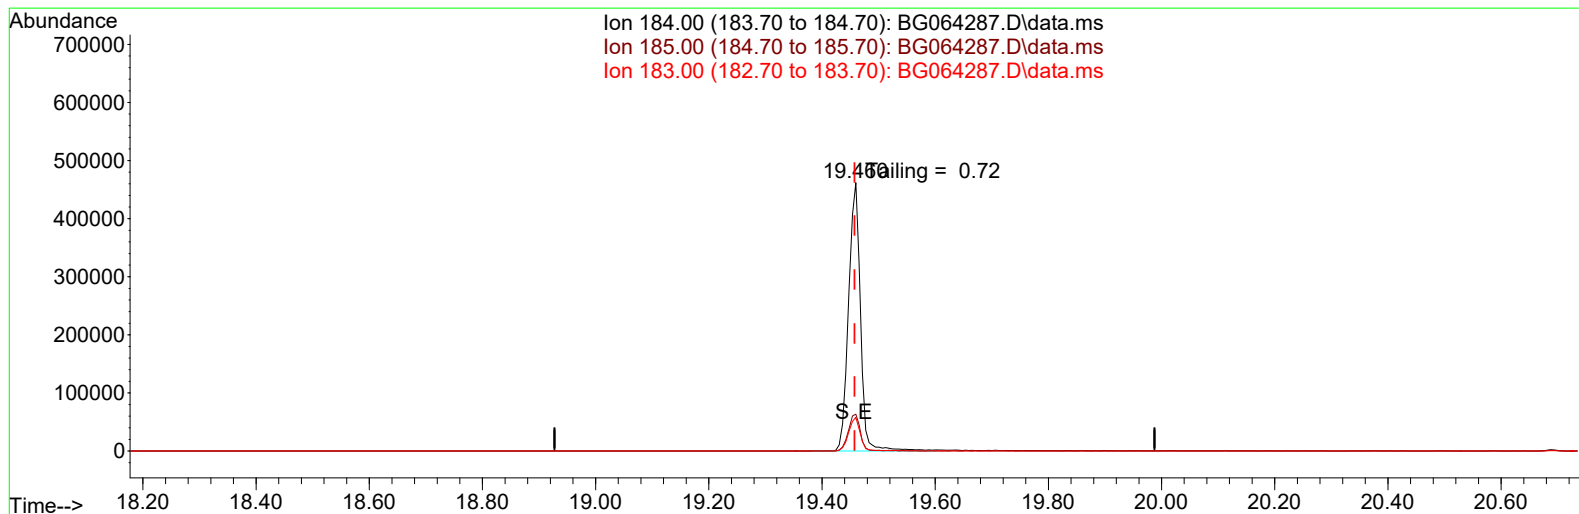




TIC: BG064287.D\data.ms

(77) Benzidine**19.460min (+ 0.002) 584971.38 ng****response 676816**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.73
183.00	12.10	12.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090525\
Data File : BG064287.D
Acq On : 5 Sep 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 12:43:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

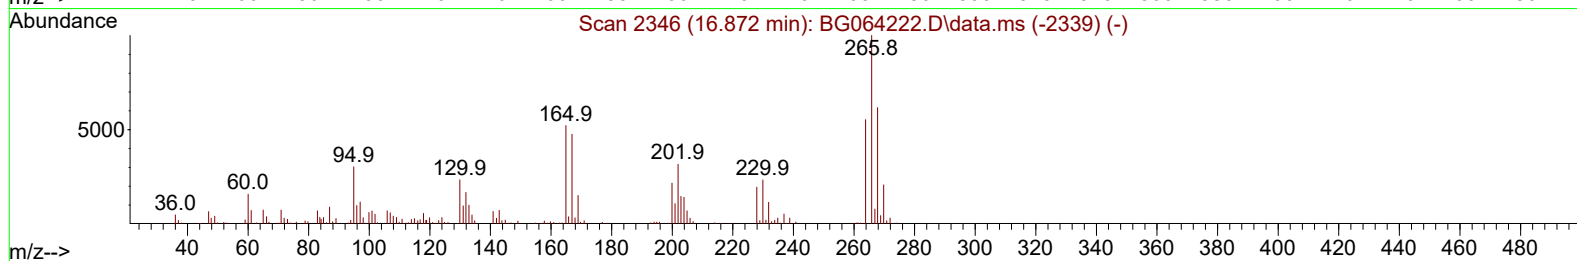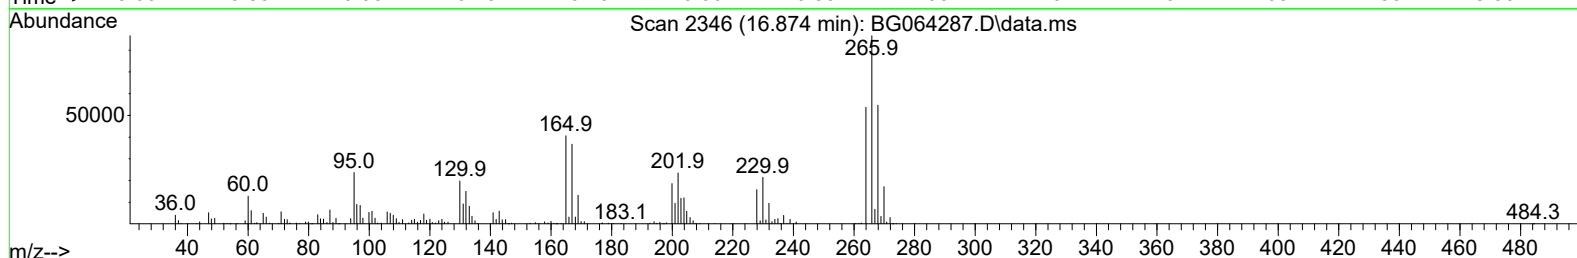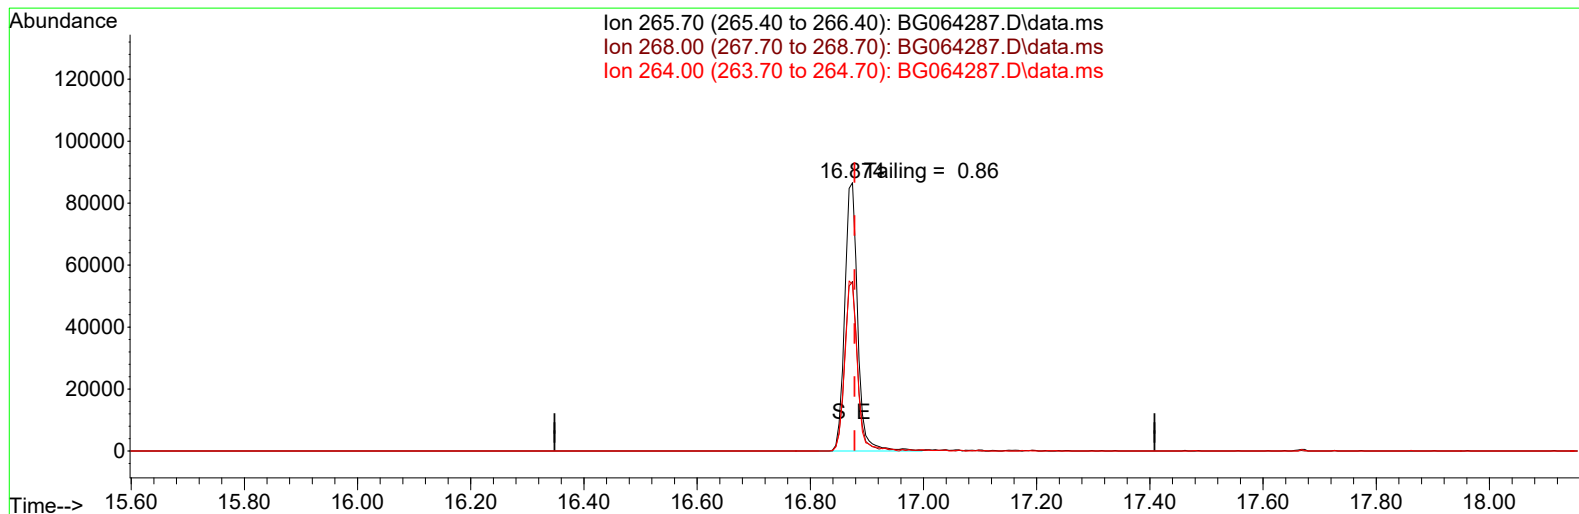

TIC: BG064287.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.004) 334985.94 ng

response 136555

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.13
264.00	55.40	62.05
0.00	0.00	0.00