


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090525\
Data File : BG064287.D
Acq On : 5 Sep 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

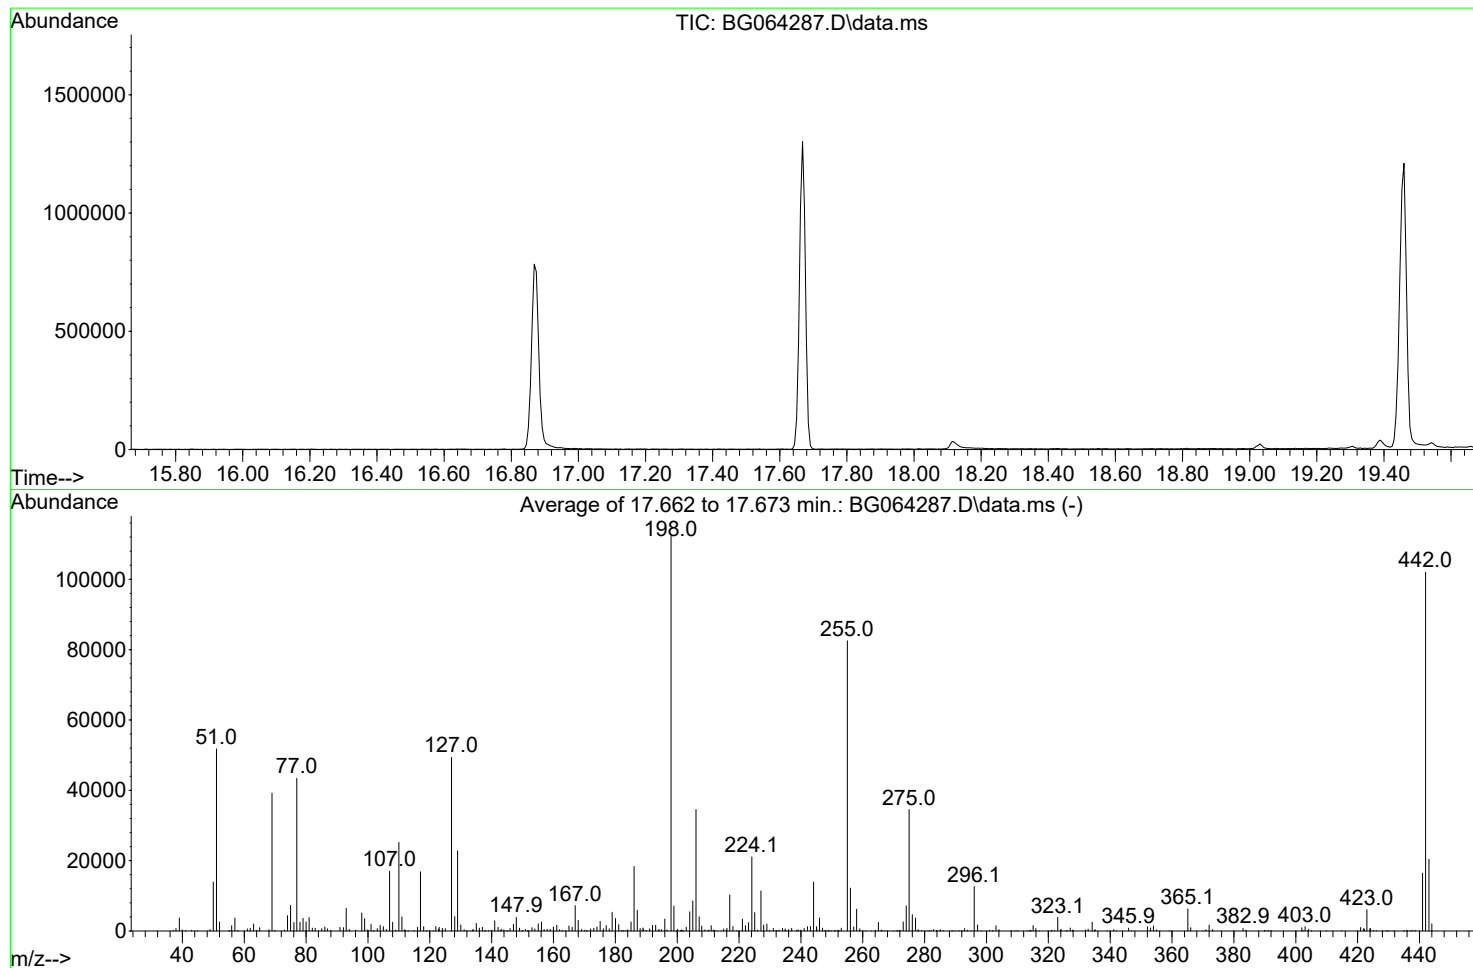

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	369	PASS
69	69	100	100	100.0	39229	PASS
70	69	0.00	2	0.5	212	PASS
197	198	0.00	2	0.3	317	PASS
198	198	100	100	100.0	112272	PASS
199	198	5	9	6.3	7080	PASS
365	198	1	100	5.6	6279	PASS
441	443	0.01	150	80.7	16441	PASS
442	442	100	100	100.0	102053	PASS
443	442	15	24	20.0	20380	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/5/2025	BNA_G	BG064287.D
Compound Name	Response	Retention Time
DDT	397066	20.688
DDD	7926	20.253
DDE	544	19.748
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8470	405536	2.09

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090525\
Data File : BG064287.D
Acq On : 5 Sep 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 05 12:43:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

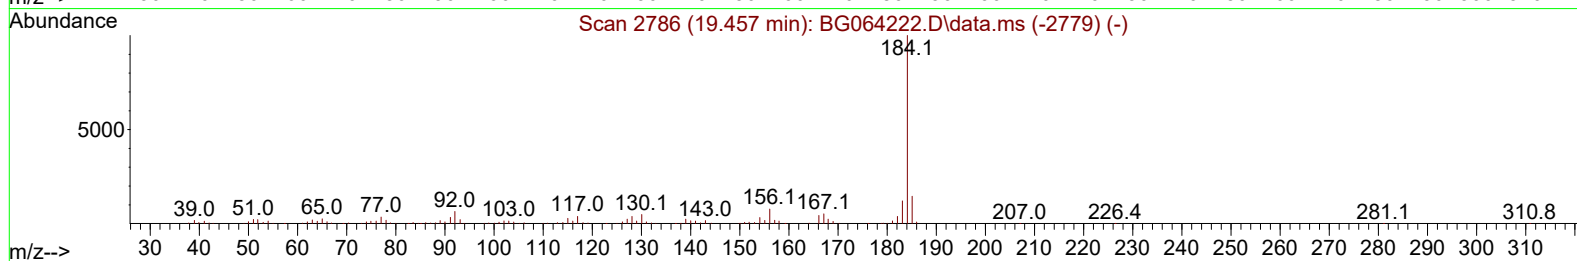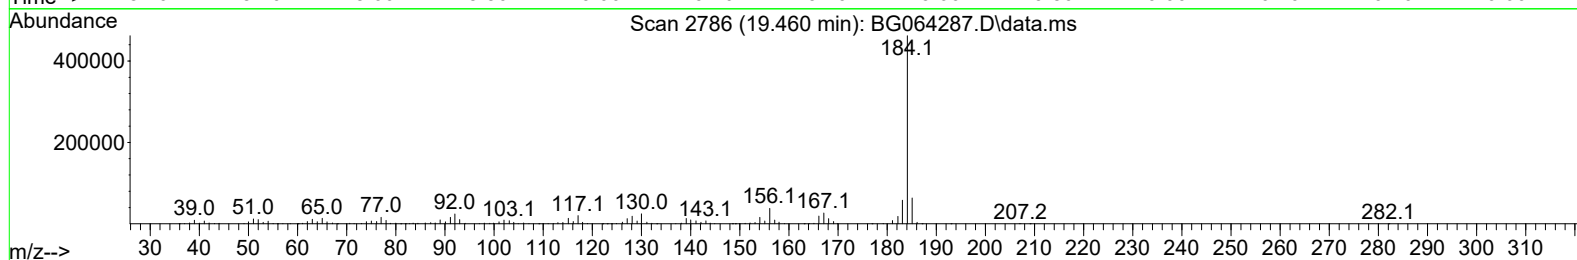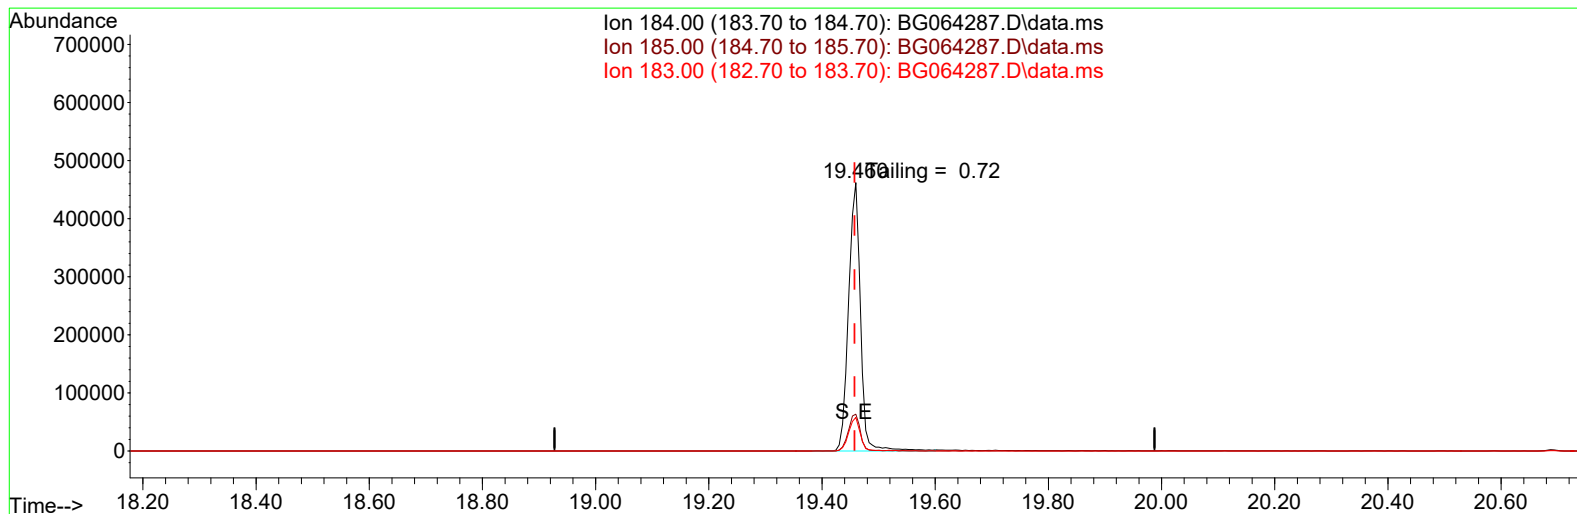

TIC: BG064287.D\data.ms

(77) Benzidine

19.460min (+ 0.002) 584971.38 ng




response 676816

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.73
183.00	12.10	12.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090525\
Data File : BG064287.D
Acq On : 5 Sep 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 05 12:43:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

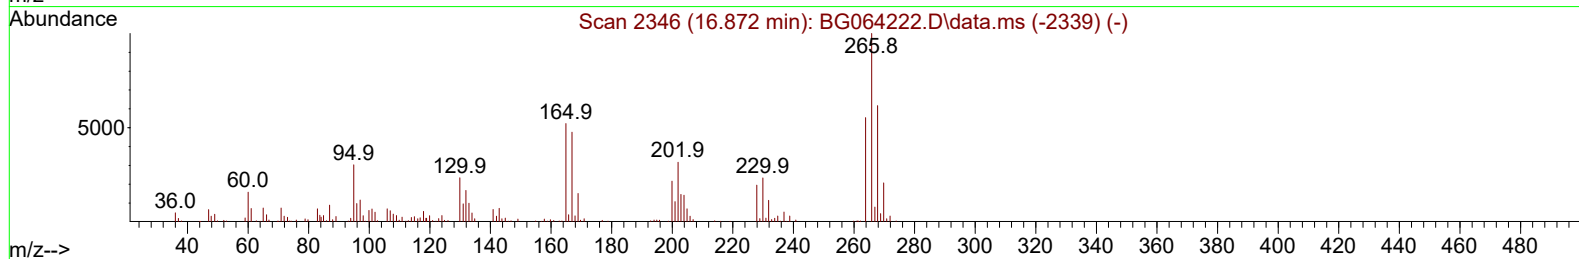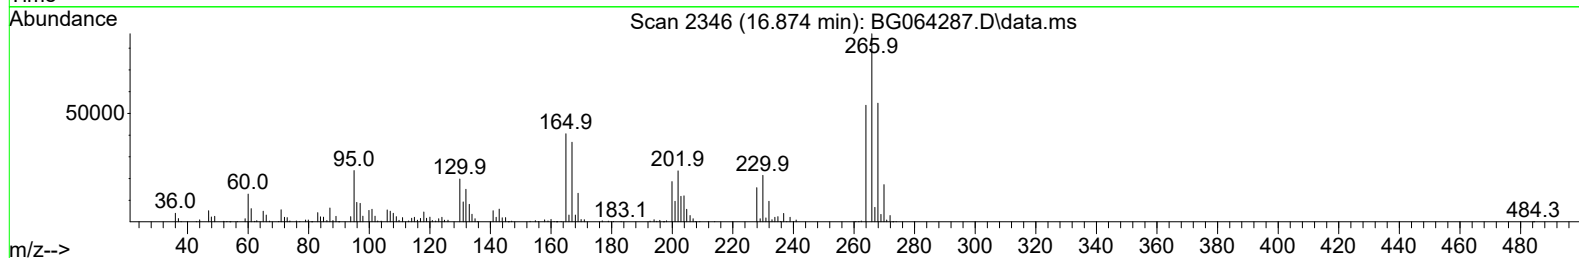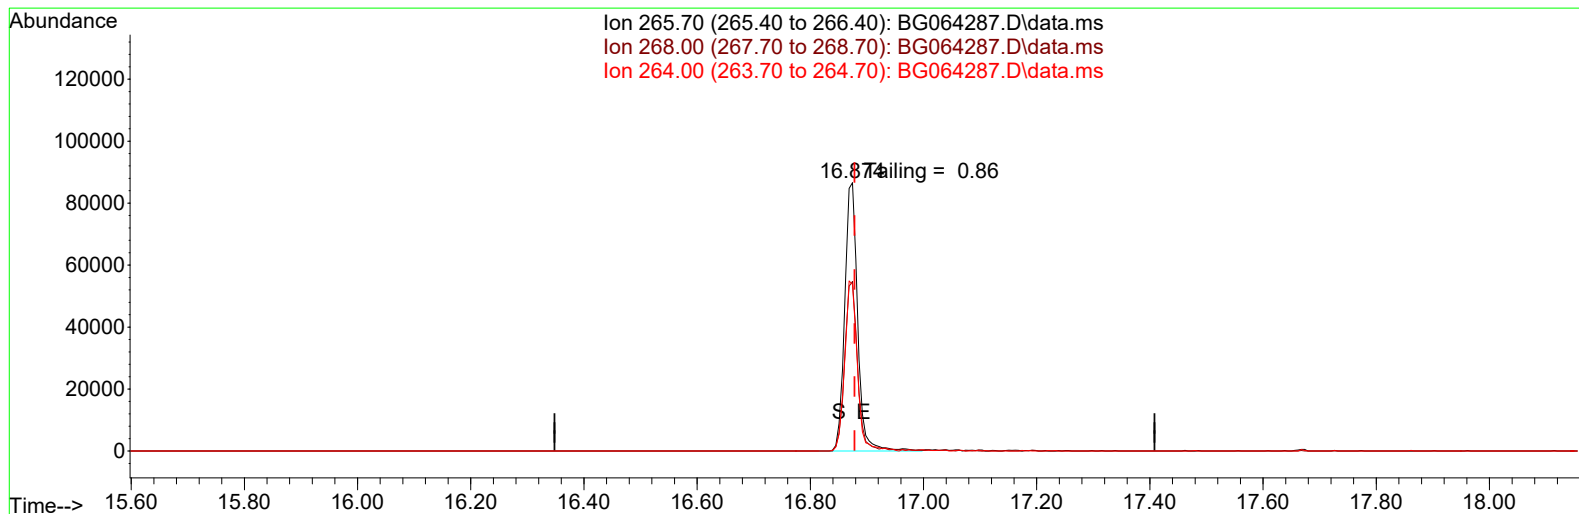

TIC: BG064287.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.004) 334985.94 ng

response 136555

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.13
264.00	55.40	62.05
0.00	0.00	0.00