
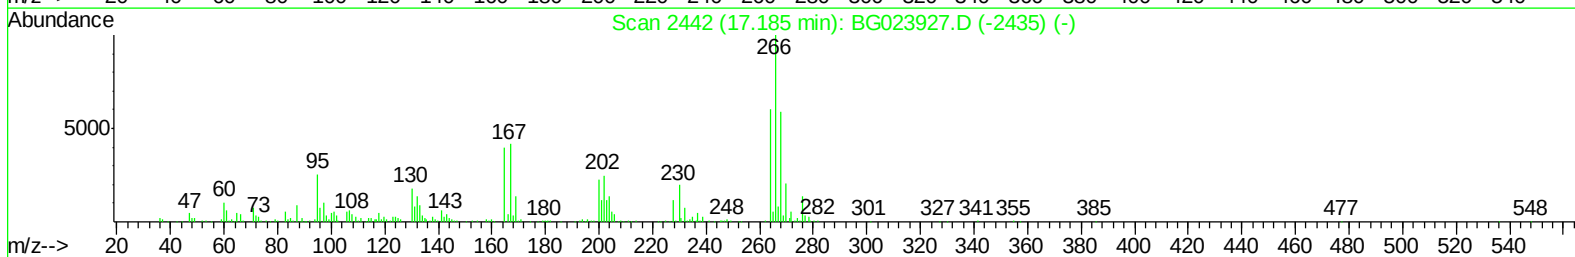
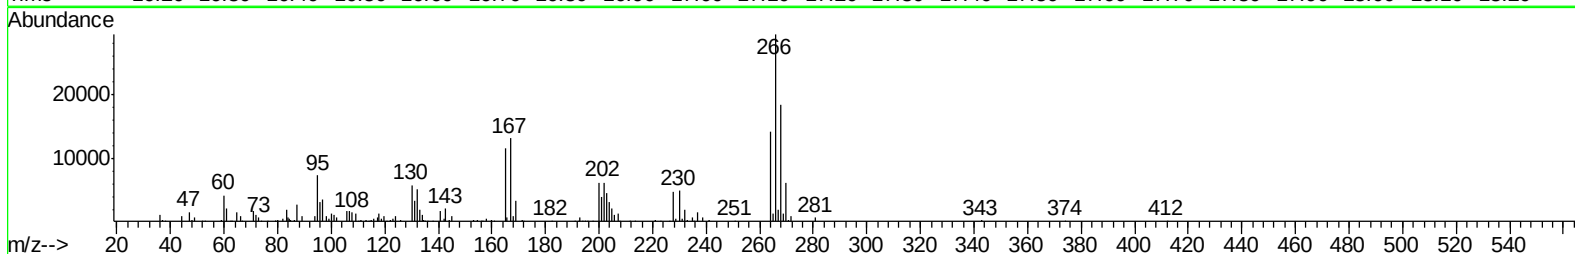


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090616\
Data File : BG023946.D
Acq On : 6 Sep 2016 13:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 01:07:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 20:05:47 2016
Response via : Initial Calibration

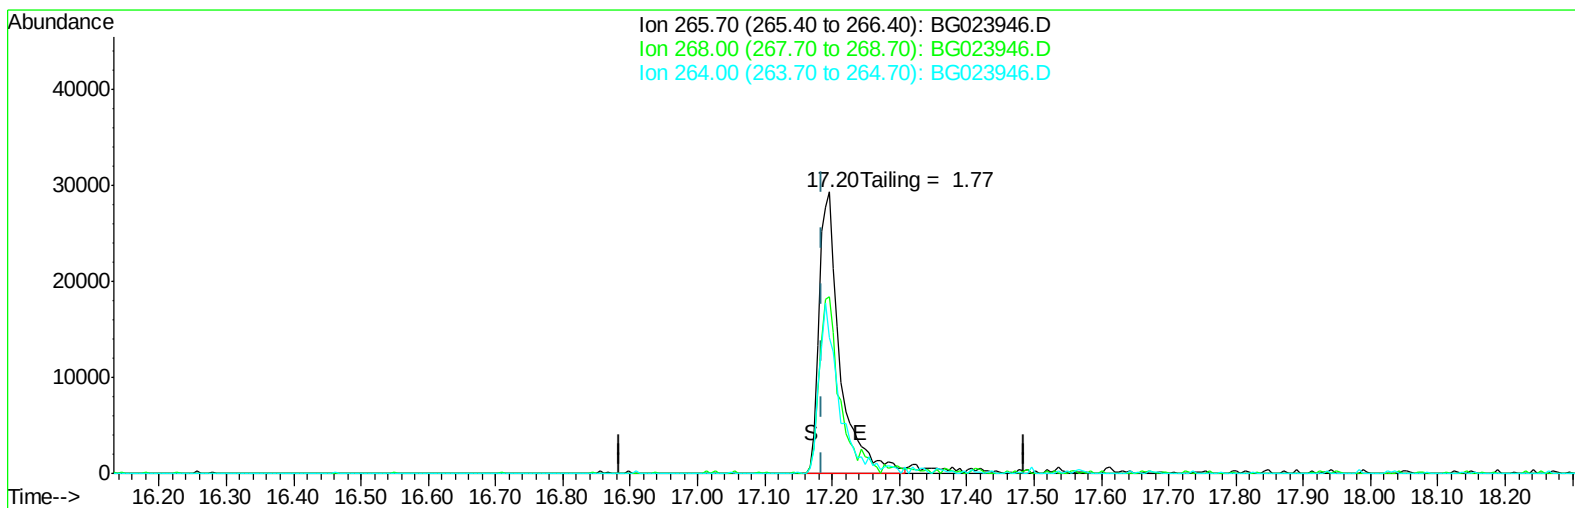

TIC: BG023946.D

(69) Pentachlorophenol (C)




17.196min (+0.011) 73037.06ng

response 64207

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	62.78
264.00	63.20	48.12#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090616\
Data File : BG023946.D
Acq On : 6 Sep 2016 13:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 01:07:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 20:05:47 2016
Response via : Initial Calibration

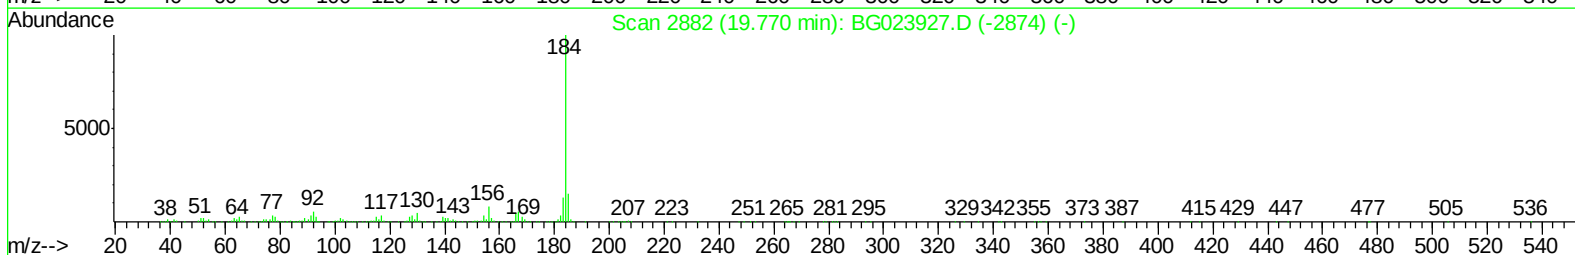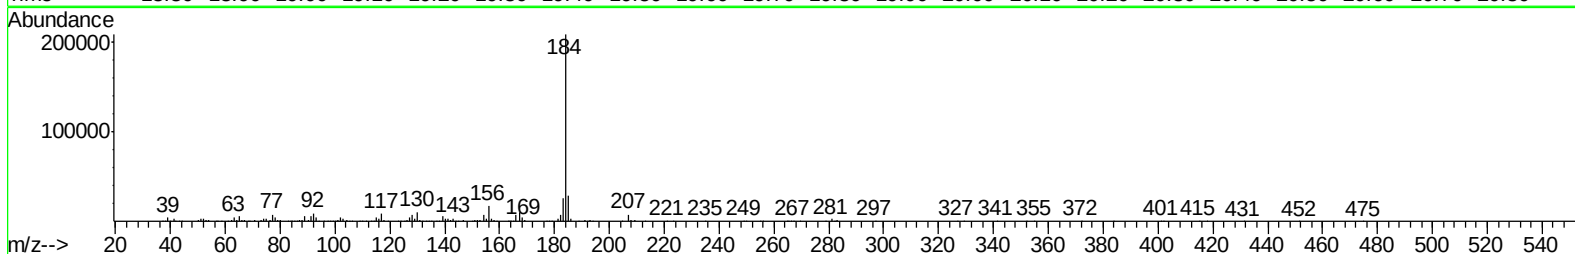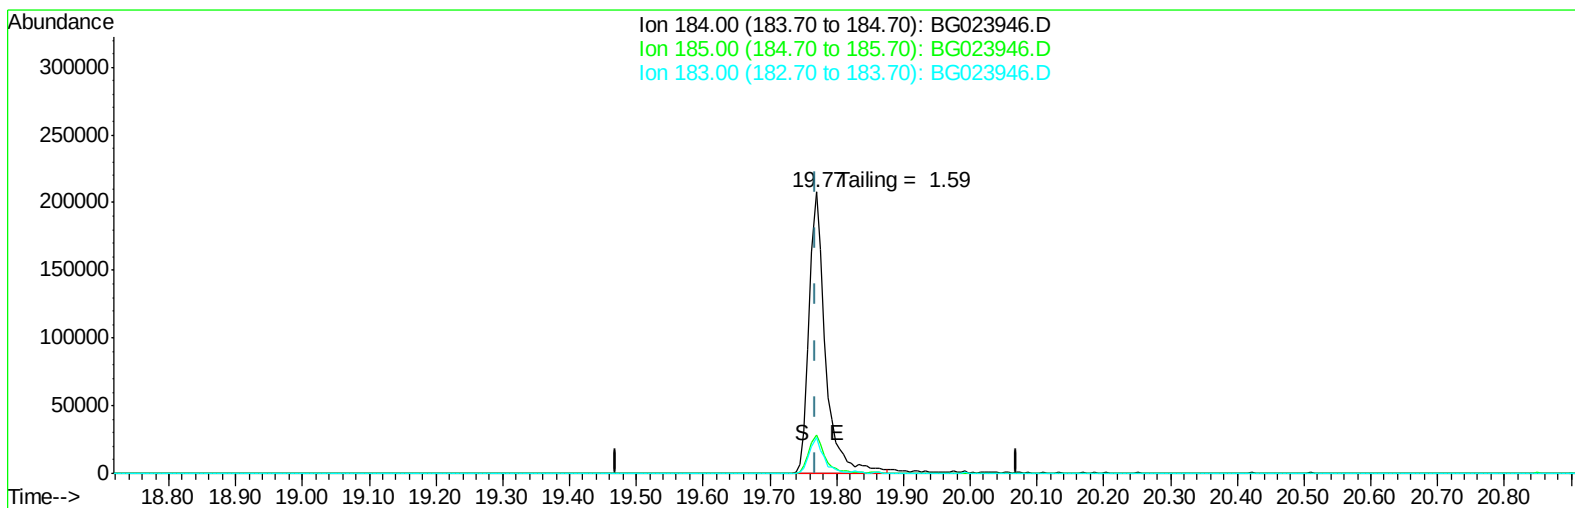

TIC: BG023946.D

(76) Benzidine

19.769min (-0.001) 196736.69ng

response 347250

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	13.57
183.00	13.40	12.53
0.00	0.00	0.00