


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090616\
Data File : BG023946.D
Acq On : 6 Sep 2016 13:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 31 20:05:47 2016

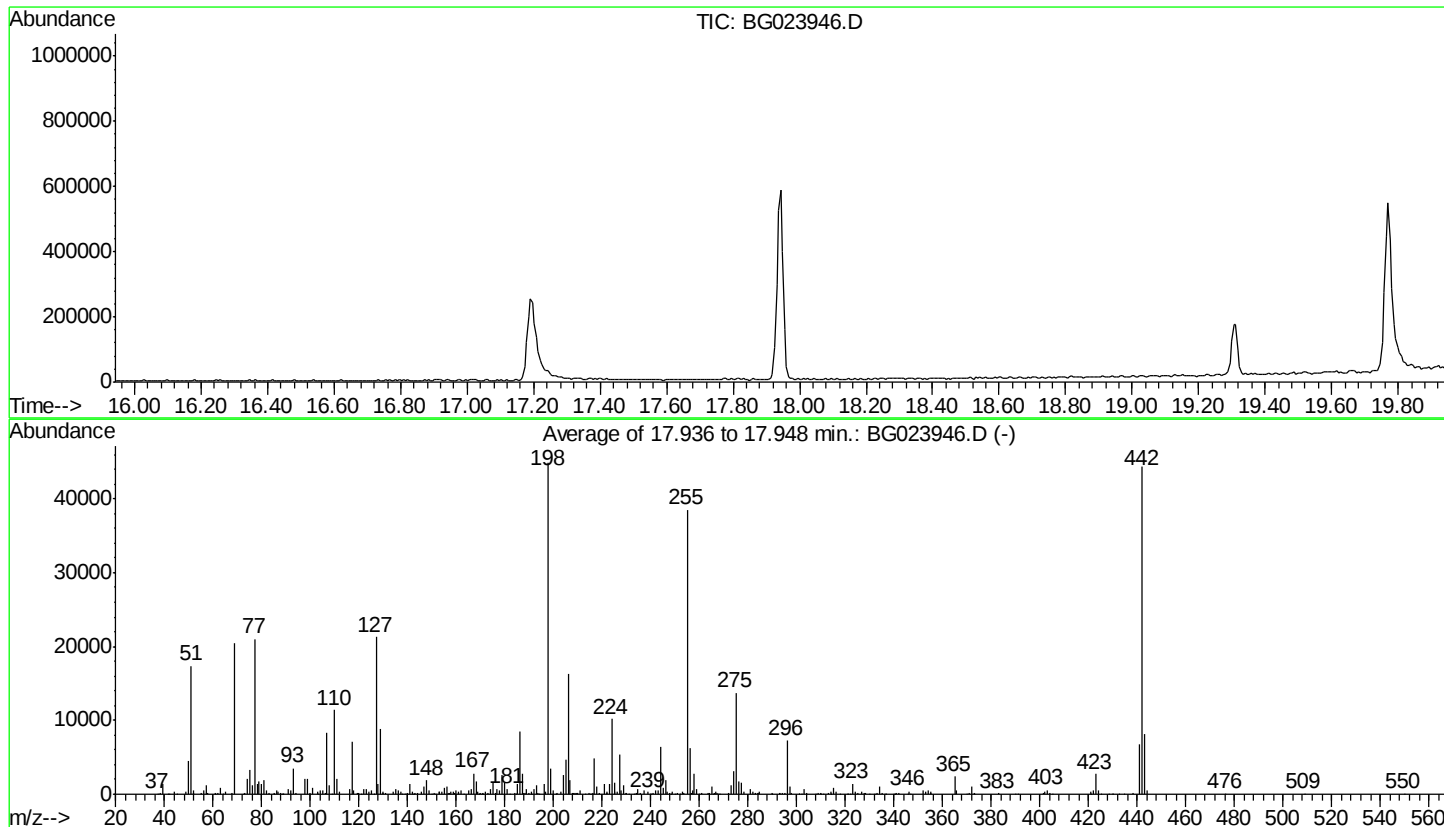

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	17336	PASS
68	69	0.00	2	0.6	132	PASS
69	198	0.00	100	45.7	20506	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	21294	PASS
197	198	0.00	2	0.8	379	PASS
198	198	100	100	100.0	44901	PASS
199	198	5	9	7.6	3399	PASS
275	198	10	60	30.6	13746	PASS
365	198	1	100	5.2	2351	PASS
441	442	0.01	24	15.4	6838	PASS
442	198	50	100	98.9	44416	PASS
443	442	15	24	18.3	8144	PASS