

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG090617\
 Data File : BG028586.D
 Acq On : 6 Sep 2017 17:26
 Operator : SJ/JU
 Sample : I5097-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDZT4

Manual Integrations
 APPROVED

Sohil
 9/7/2017 10:42:25 AM

Quant Time: Sep 07 03:50:34 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 07 02:23:39 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	41669	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	169587	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	117850	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.70	188	291377	20.00	ng/ul	0.00
75) Chrysene-d12	22.03	240	330164	20.00	ng/ul	0.00
83) Perylene-d12	25.55	264	332499	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.83	96	3634	4.06	ng/uL	0.00
5) Phenol-d5	7.50	99	87292	19.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.65	67	54377	18.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.88	132	64308	22.27	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	73171	19.13	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	32776	24.72	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	39065	26.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	75948	25.25	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	73140	21.84	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	251080	23.95	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	288712	24.43	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	30701	18.42	ng/ul	0.00
57) Fluorene-d10	15.94	176	217040	23.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	39131	20.67	ng/ul	0.00
70) Anthracene-d10	17.80	188	357671	25.60	ng/ul	0.00
76) Pyrene-d10	20.07	212	415133	24.52	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	384972	24.73	ng/ul	0.00

Target Compounds

					Ovalue	
6) Phenol	7.52	94	14298	3.144	ng/ul#	85
44) Dimethylphthalate	14.38	163	96369	9.985	ng/ul	97
69) Phenanthrene	17.74	178	34051	2.322	ng/ul	93
74) Fluoranthene	19.74	202	83839	4.705	ng/ul	98
77) Pyrene	20.10	202	80284	4.076	ng/ul	98
80) Benzo(a)anthracene	22.01	228	46680	2.447	ng/ul	96
82) Chrysene	22.08	228	41955	2.442	ng/ul	95
85) Benzo(b)fluoranthene	24.42	252	60025	3.017	ng/ul	99
88) Benzo(a)pyrene	25.38	252	40960	2.126	ng/ul	96
89) Indeno(1,2,3-cd)pyrene	29.58	276	26552m	1.177	ng/ul	
91) Benzo(g,h,i)perylene	30.83	276	21703	1.169	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG090617\
Data File : BG028586.D
Acq On : 6 Sep 2017 17:26
Operator : SJ/JU
Sample : I5097-18
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDZT4

Manual Integrations
APPROVED

Sohil
9/7/2017 10:42:25 AM

Quant Time: Sep 07 03:50:34 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 07 02:23:39 2017
Response via : Initial Calibration

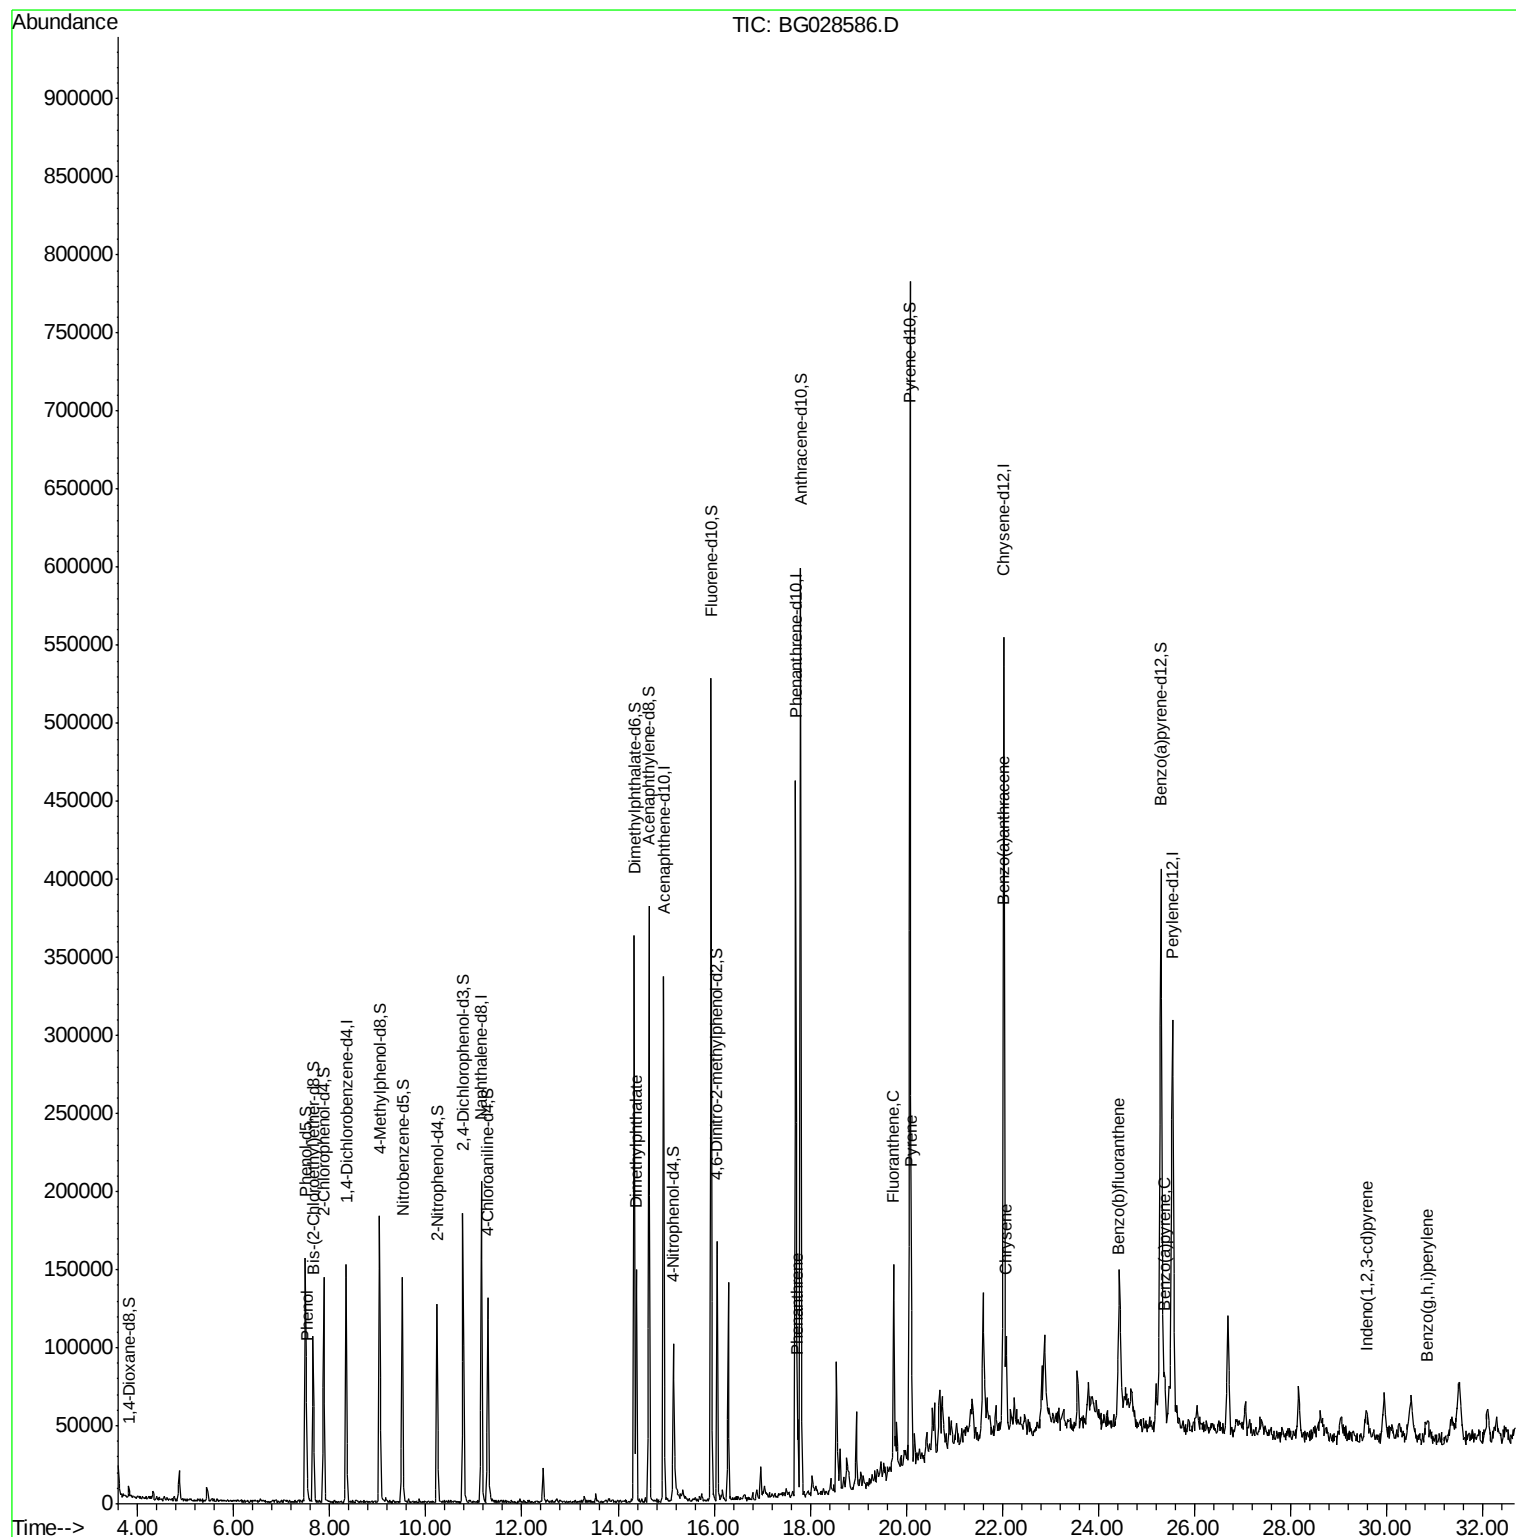

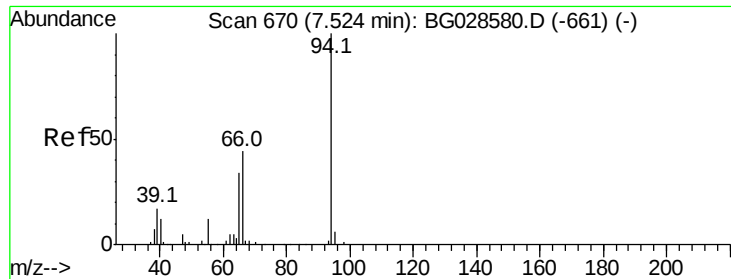

#6

Phenol

Concen: 3.144 ng/ul

RT: 7.52 min Scan# 669

Delta R.T. -0.00 min

Lab File: BG028586.D

Acq: 6 Sep 2017 17:26

Instrument :

BNA_G

ClientSampled :

BDZT4

Tot Ion: 94 Resp: 14298

Ion Ratio Lower Upper

94 100

65 52.3 26.8 40.2#





66 58.2 44.4 66.6

Manual Integrations

APPROVED

Sohil

9/7/2017 10:42:25 AM

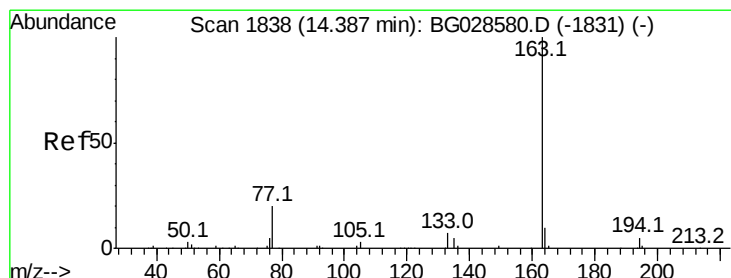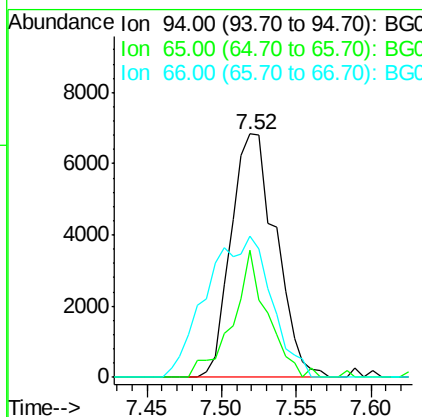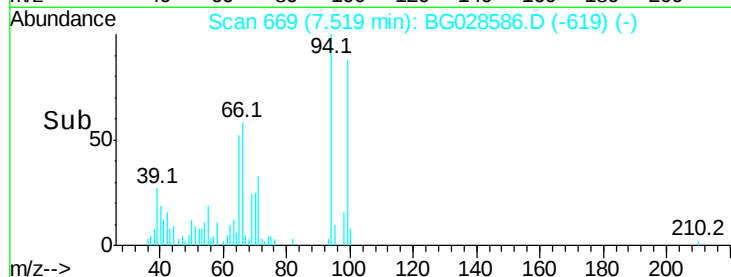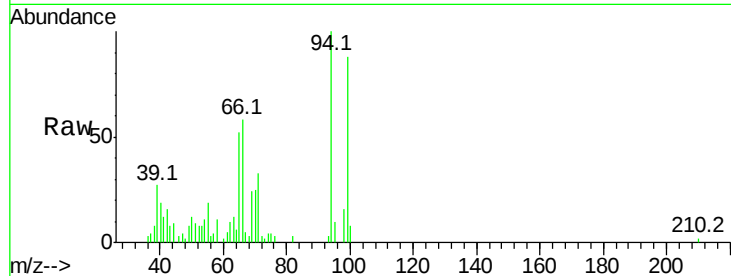

#44

Dimethylphthalate

Concen: 9.985 ng/ul

RT: 14.38 min Scan# 1837

Delta R.T. -0.00 min

Lab File: BG028586.D

Acq: 6 Sep 2017 17:26




Tgt Ion:163 Resp: 96369


Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 9.9 9.0 13.4

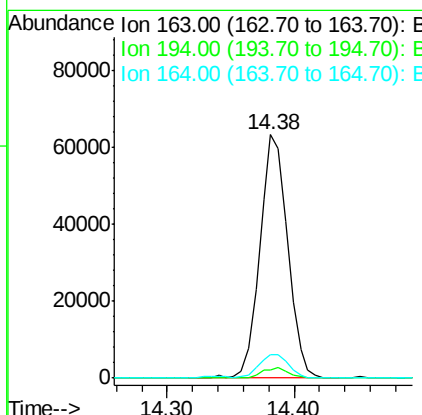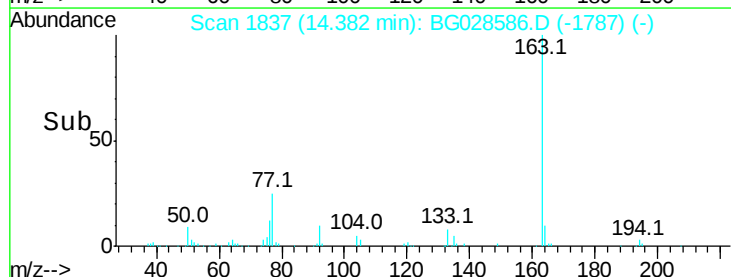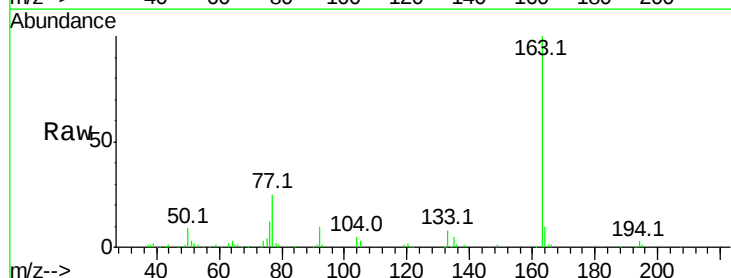

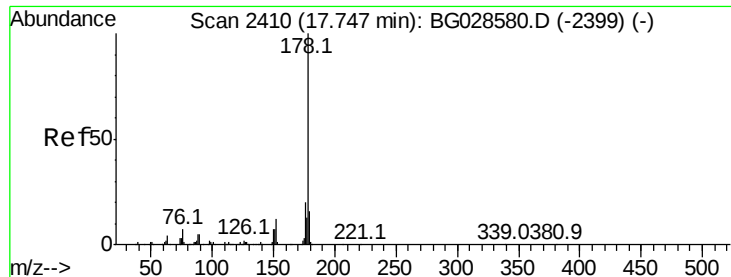

#69

Phenanthrene

Concen: 2.322 ng/ul

RT: 17.74 min Scan# 2409

Delta R.T. -0.00 min

Lab File: BG028586.D

Acq: 6 Sep 2017 17:26

Instrument :

BNA_G





ClientSampled :

BDZT4

Tot Ion:	178	Resp:	34051
Ion	Ratio	Lower	Upper
178	100		
179	12.5	12.4	18.6
176	17.7	16.5	24.7

Manual Integrations
APPROVED

Sohil
9/7/2017 10:42:25 AM

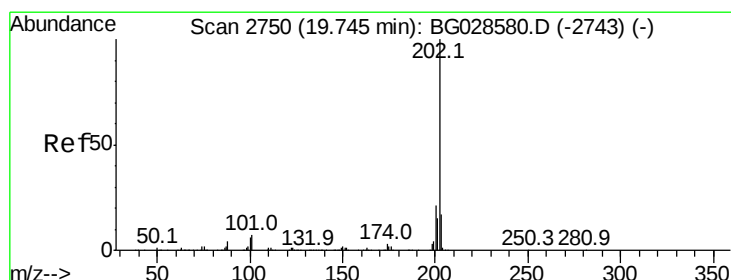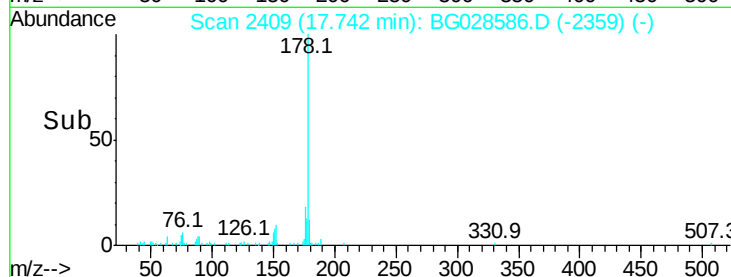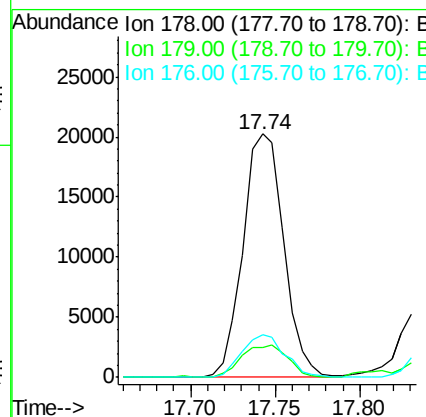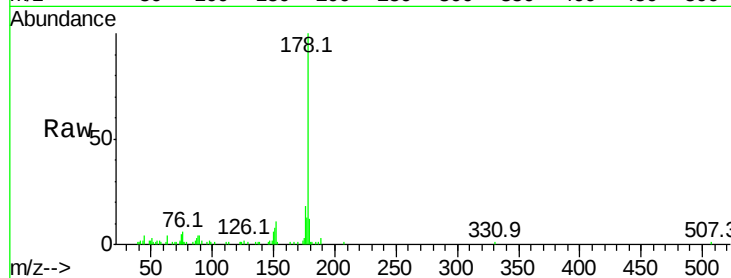

#74

Fluoranthene

Concen: 4.705 ng/ul




RT: 19.74 min Scan# 2749


Delta R.T. -0.00 min

Lab File: BG028586.D

Acq: 6 Sep 2017 17:26

Tgt Ion:	202	Resp:	83839
Ion	Ratio	Lower	Upper
202	100		
101	8.4	6.2	9.2
100	6.9	5.2	7.8

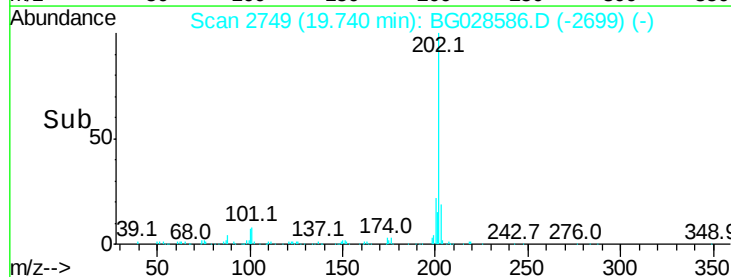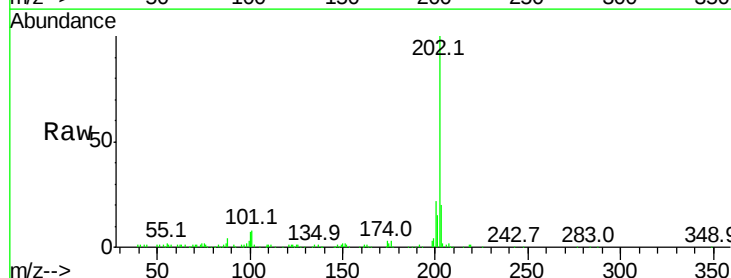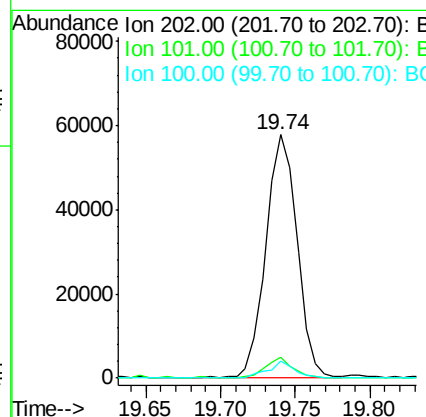

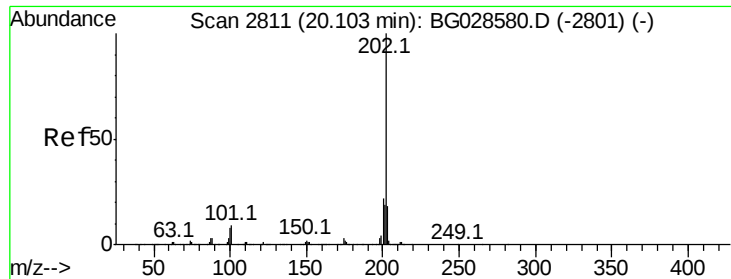

#77

Pvrene

Concen: 4.076 ng/ul

RT: 20.10 min Scan# 2811

Delta R.T. 0.00 min

Lab File: BG028586.D

Acq: 6 Sep 2017 17:26

Instrument :

BNA_G





ClientSampleId :

BDZT4

Tot Ion	Ratio	Resp	Lower	Upper
202	100	80284		
101	8.5	6.9	10.3	
100	6.8	6.6	10.0	

Manual Integrations
APPROVED

Sohil
9/7/2017 10:42:25 AM

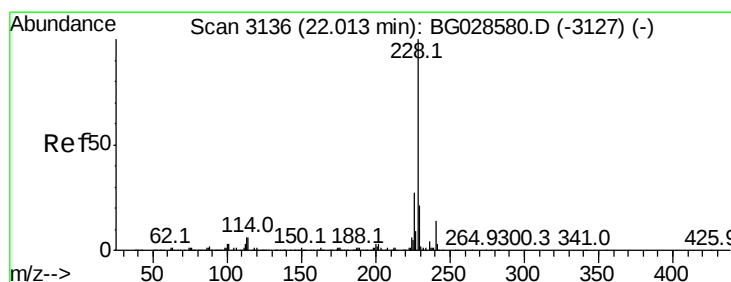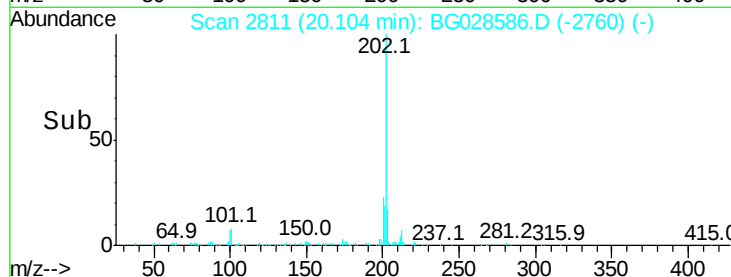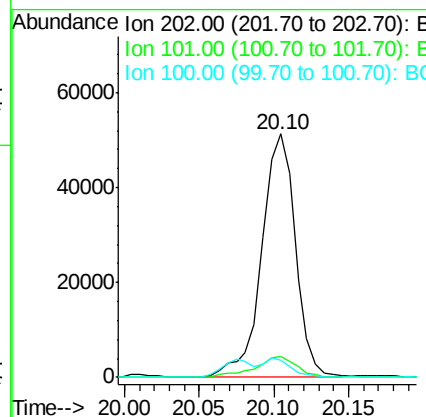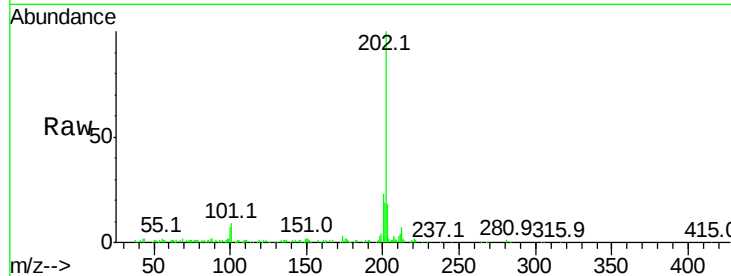

#80

Benzo(a)anthracene

Concen: 2.447 ng/ul




RT: 22.01 min Scan# 3136


Delta R.T. 0.00 min

Lab File: BG028586.D

Acq: 6 Sep 2017 17:26

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	46680		
229	21.0	16.3	24.5	
226	24.4	21.9	32.9	

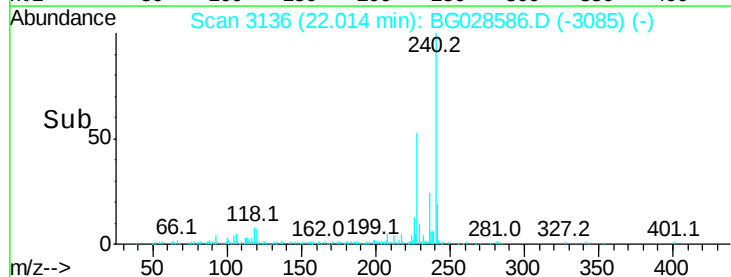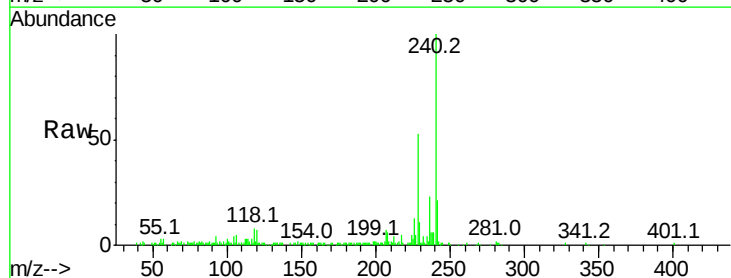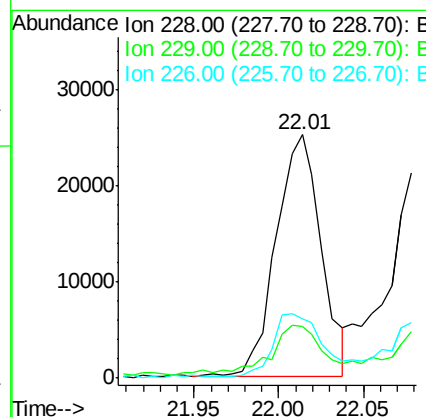

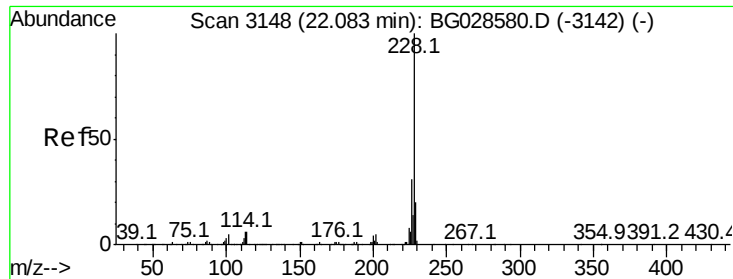

#82

Chrysene

Concen: 2.442 ng/ul

RT: 22.08 min Scan# 3147

Delta R.T. -0.00 min

Lab File: BG028586.D

Acq: 6 Sep 2017 17:26

Instrument :

BNA_G





ClientSampleId :

BDZT4

Tot Ion:	228	Resp:	41955
Ion Ratio	Lower	Upper	
228	100		
226	26.9	24.0	36.0
229	22.7	16.9	25.3

Manual Integrations
APPROVED

Sohil
9/7/2017 10:42:25 AM

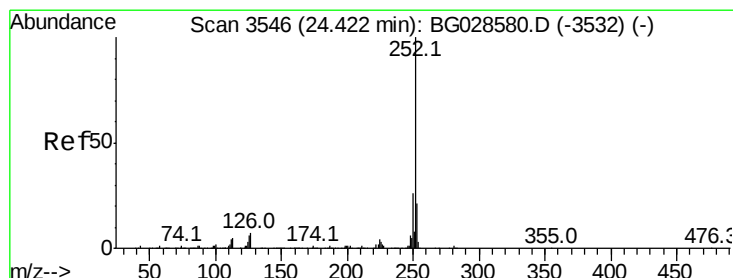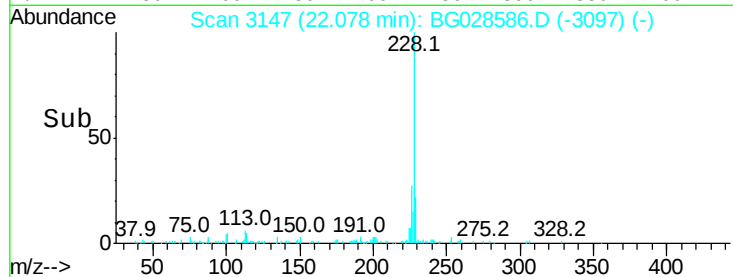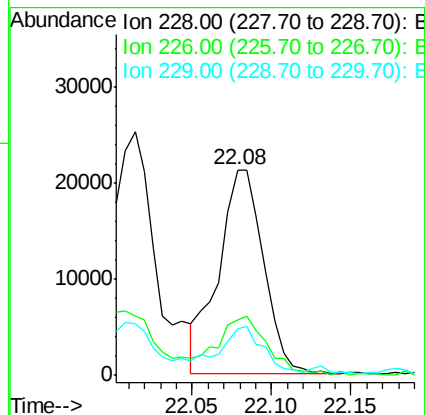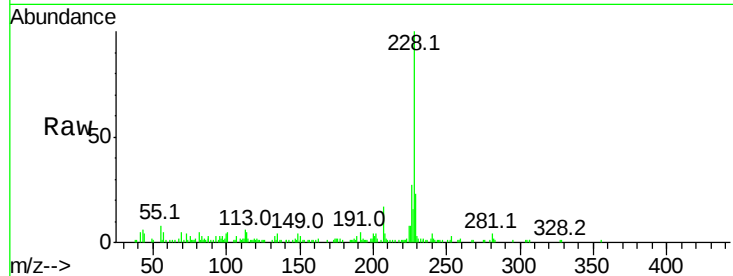

#85

Benzo(b)fluoranthene

Concen: 3.017 ng/ul




RT: 24.42 min Scan# 3545


Delta R.T. -0.00 min

Lab File: BG028586.D

Acq: 6 Sep 2017 17:26

Tgt Ion:	252	Resp:	60025
Ion Ratio	Lower	Upper	
252	100		
253	22.6	17.7	26.5
125	5.8	4.0	6.0

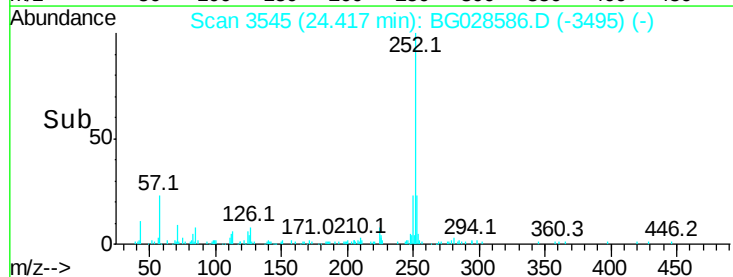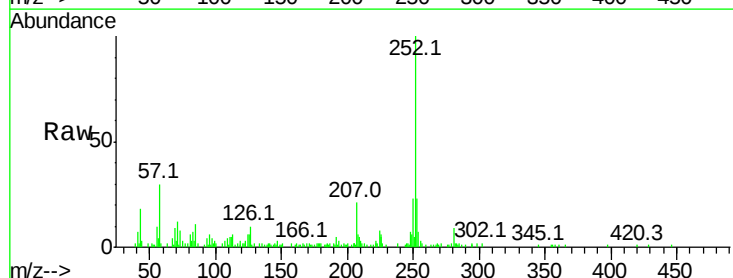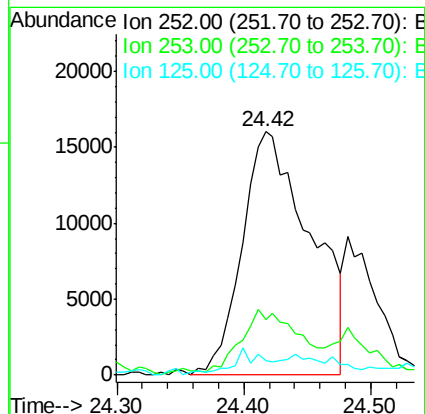

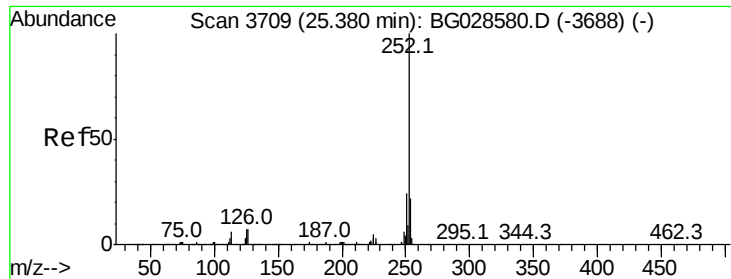





#88
Benzo(a)pyrene
Concen: 2.126 ng/ul
RT: 25.38 min Scan# 3709
Delta R.T. 0.00 min
Lab File: BG028586.D
Acq: 6 Sep 2017 17:26

Instrument :
BNA_G
ClientSampleId :
BDZT4

Tot Ion	Ratio	Lower	Upper
252	100		
253	20.0	17.8	26.6
125	5.8	5.4	8.0




Manual Integrations
APPROVED


Sohil
9/7/2017 10:42:25 AM

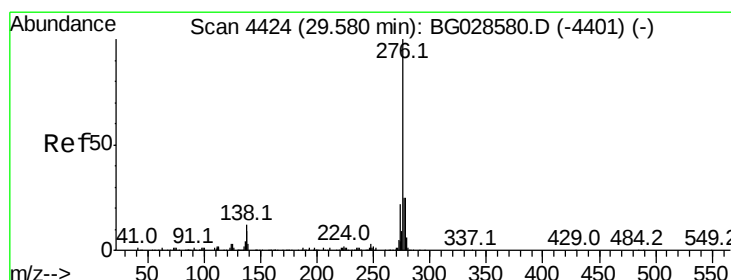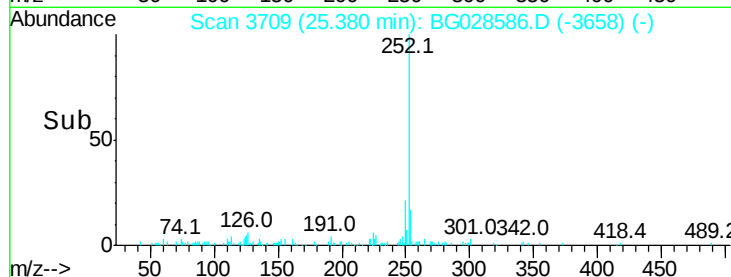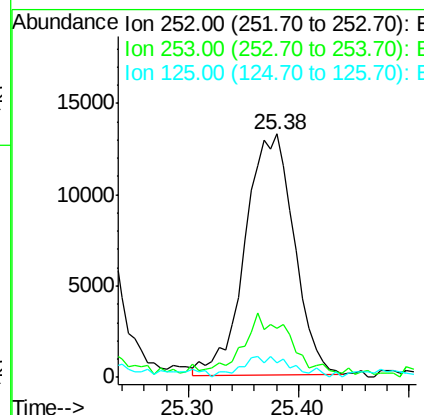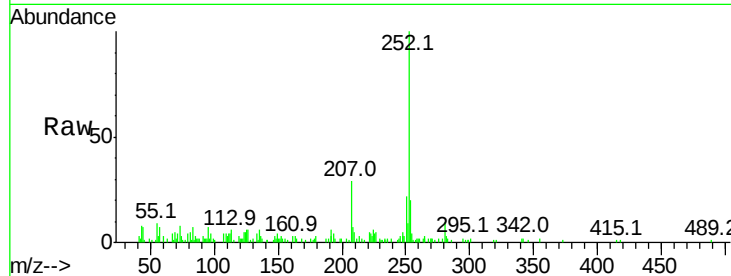

#89
Indeno(1,2,3-cd)pyrene
Concen: 1.177 ng/ul m
RT: 29.58 min Scan# 4424
Delta R.T. 0.00 min
Lab File: BG028586.D
Acq: 6 Sep 2017 17:26

Tgt Ion	Ratio	Lower	Upper
276	100		
138	11.7	8.2	12.4
277	19.4	18.6	28.0

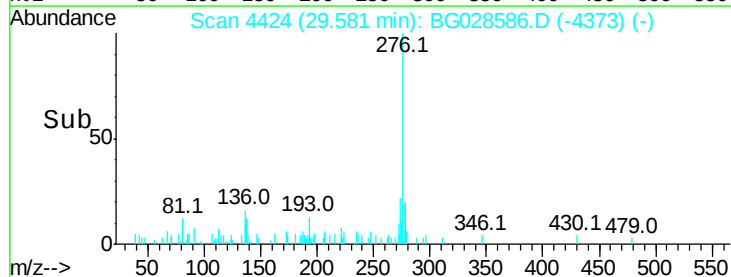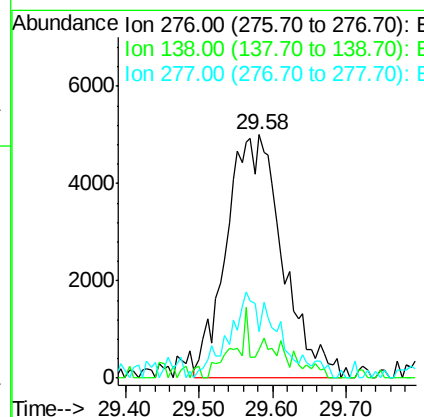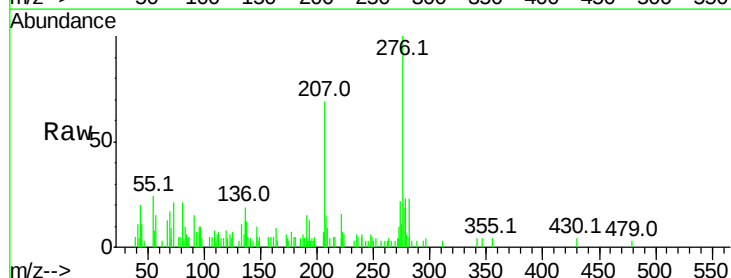

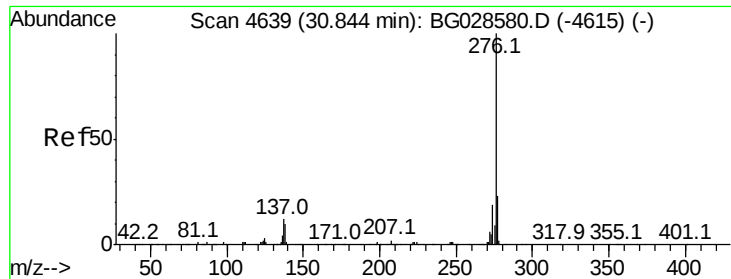

#91
 Benzo(a,h,i)perylene
 Concen: 1.169 ng/ul
 RT: 30.83 min Scan# 4637
 Delta R.T. -0.01 min
 Lab File: BG028586.D
 Acq: 6 Sep 2017 17:26

Instrument :
 BNA_G
 ClientSampleId :
 BDZT4

Tot Ion	Ratio	Lower	Upper
276	100		
138	10.1	8.6	12.8
277	20.9	17.6	26.4

Manual Integrations
 APPROVED

Sohil
 9/7/2017 10:42:25 AM

