
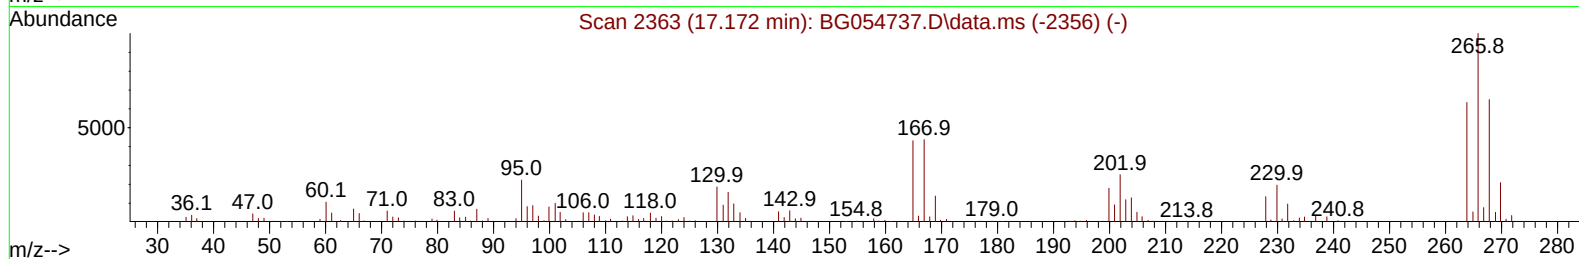
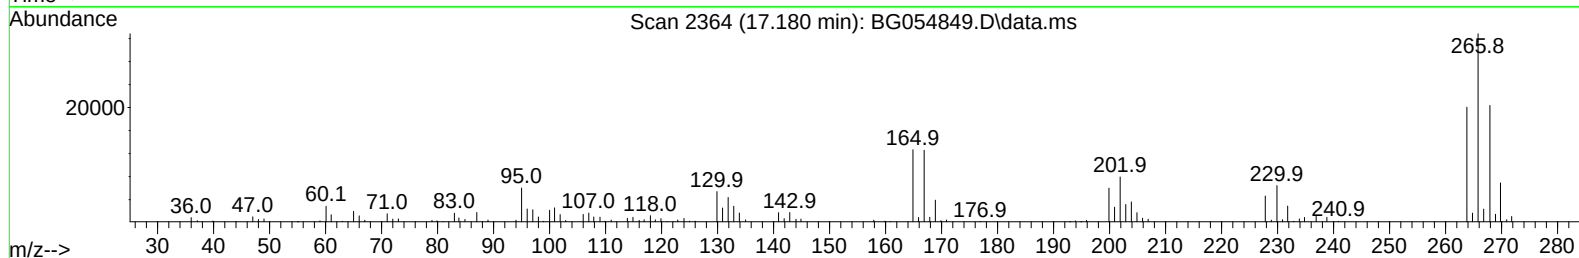


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090622\
Data File : BG054849.D
Acq On : 6 Sep 2022 12:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 07:05:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

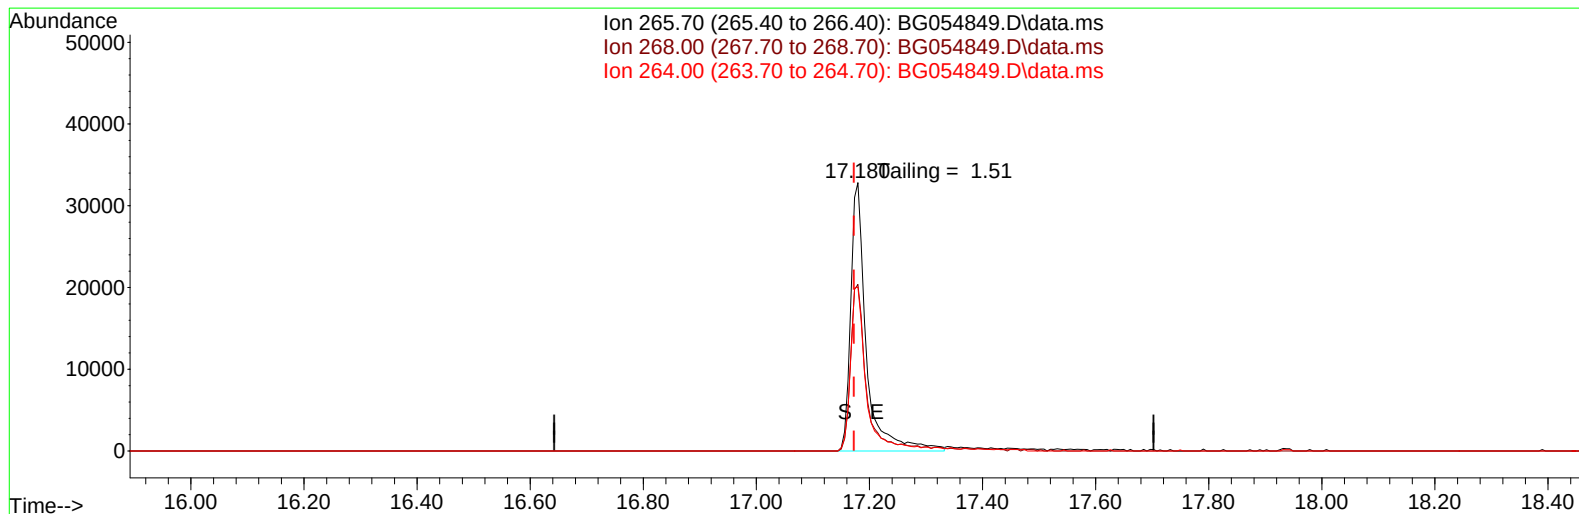

TIC: BG054849.D\data.ms

(70) Pentachlorophenol (C)




17.180min (+ 0.007) 21566.47 ng

response 63491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.06
264.00	61.70	61.11
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090622\  
Data File : BG054849.D  
Acq On    : 6 Sep 2022 12:51  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Sep 07 07:05:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

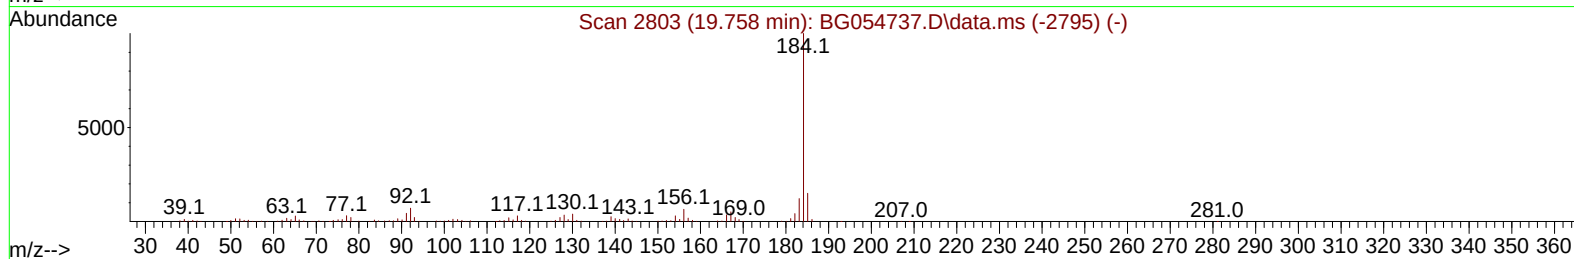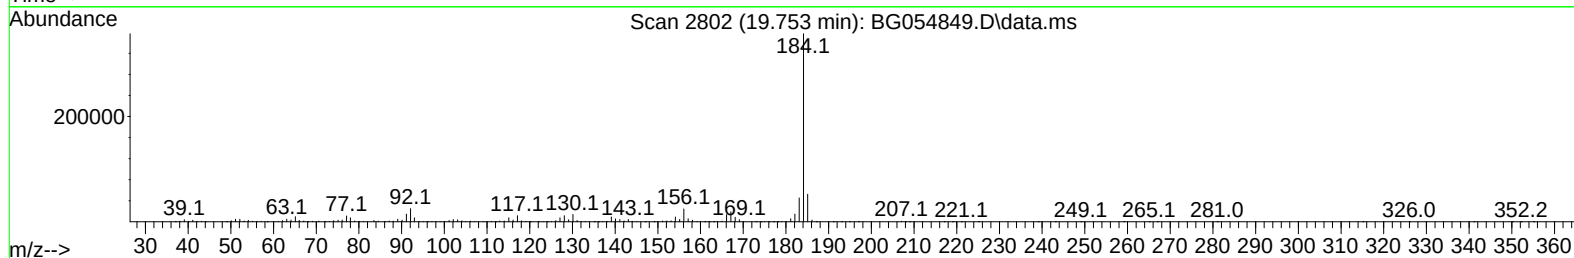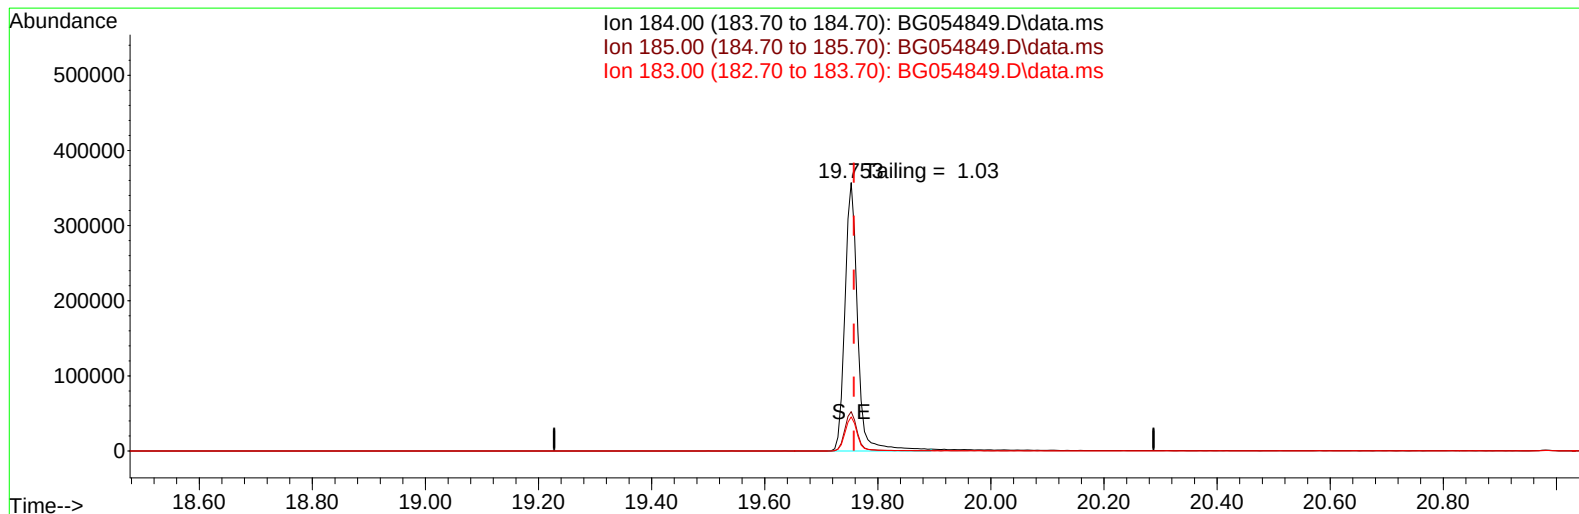

TIC: BG054849.D\data.ms

(77) Benzidine

19.753min (-0.005) 362145.72 ng

response **565104**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.20	14.71
--------	-------	-------

183.00	12.30	12.71
--------	-------	-------

0.00 0.00 0.00