


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090622\
 Data File : BG054849.D
 Acq On : 6 Sep 2022 12:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

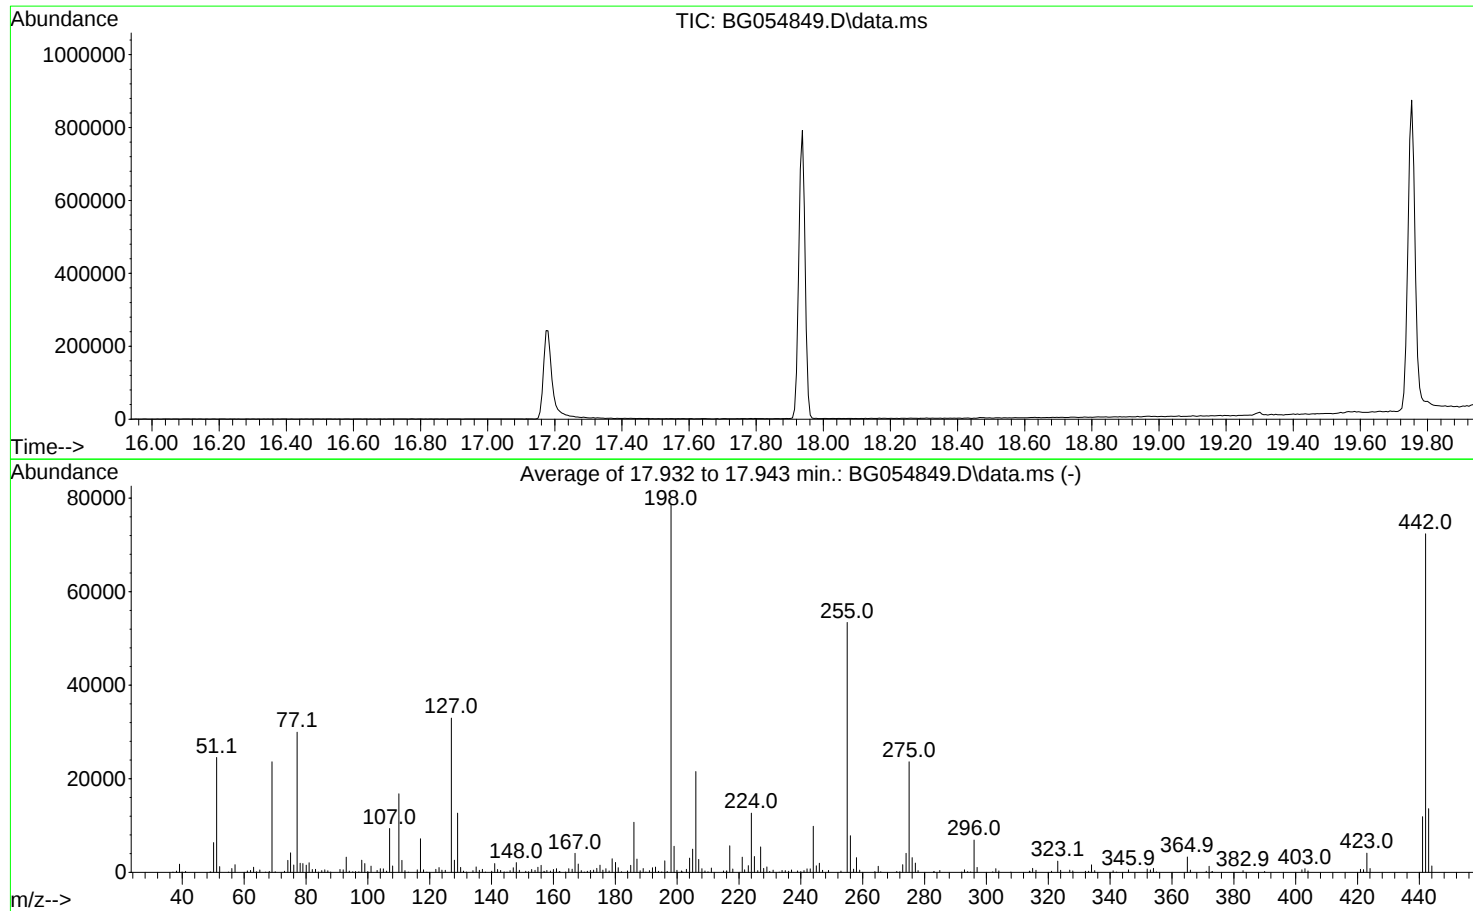




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	24536	PASS
68	69	0.00	2	0.8	180	PASS
69	198	0.00	100	30.0	23635	PASS
70	69	0.00	2	0.6	130	PASS
127	198	10	80	41.9	32968	PASS
197	198	0.00	2	0.3	207	PASS
198	198	100	100	100.0	78661	PASS
199	198	5	9	7.1	5556	PASS
275	198	10	60	30.1	23643	PASS
365	198	1	100	4.2	3272	PASS
441	198	0.01	100	15.1	11886	PASS
442	442	50	100	100.0	72389	PASS
443	442	15	24	18.8	13607	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090622\
Data File : BG054849.D
Acq On : 6 Sep 2022 12:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 07 07:05:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

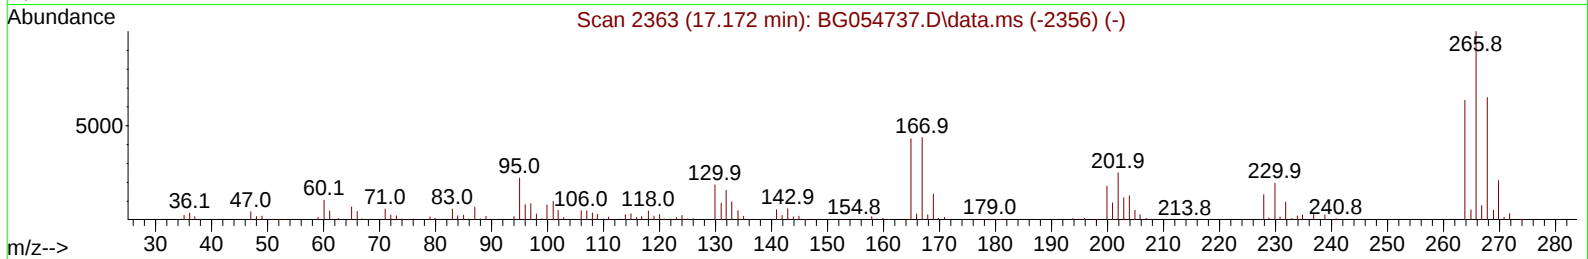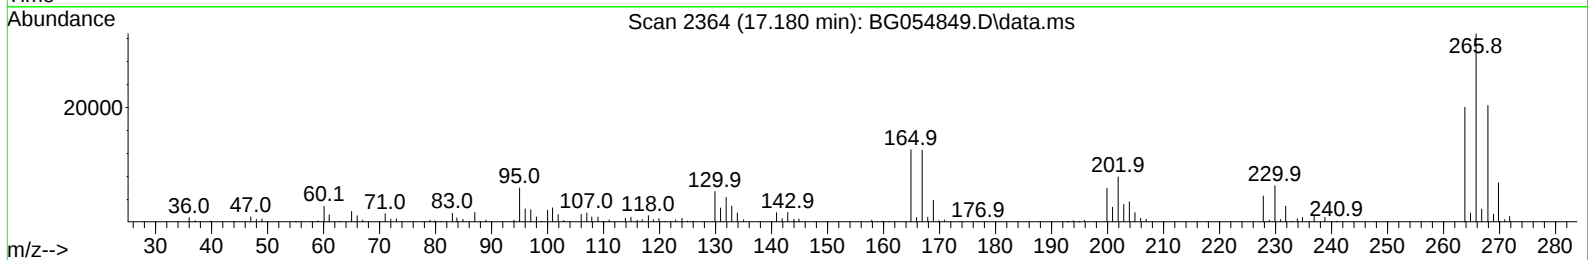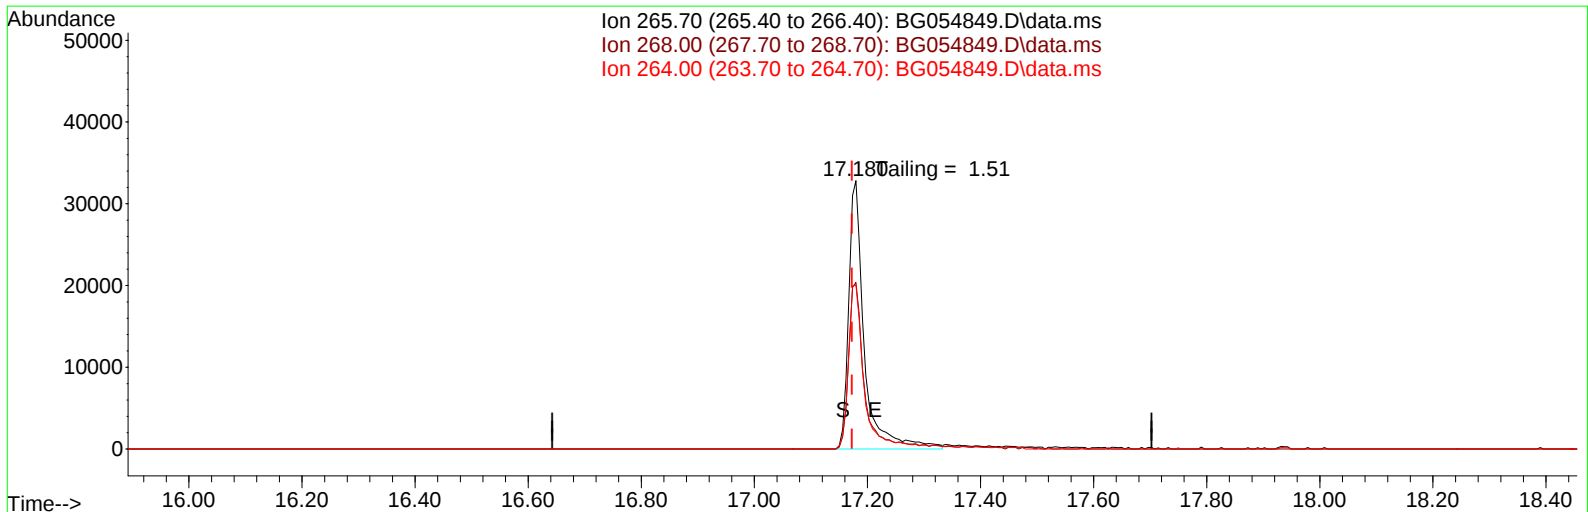

TIC: BG054849.D\data.ms

(70) Pentachlorophenol (C)

17.180min (+ 0.007) 21566.47 ng




response 63491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.06
264.00	61.70	61.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090622\
 Data File : BG054849.D
 Acq On : 6 Sep 2022 12:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Sep 07 07:05:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 17:50:55 2022
 Response via : Initial Calibration

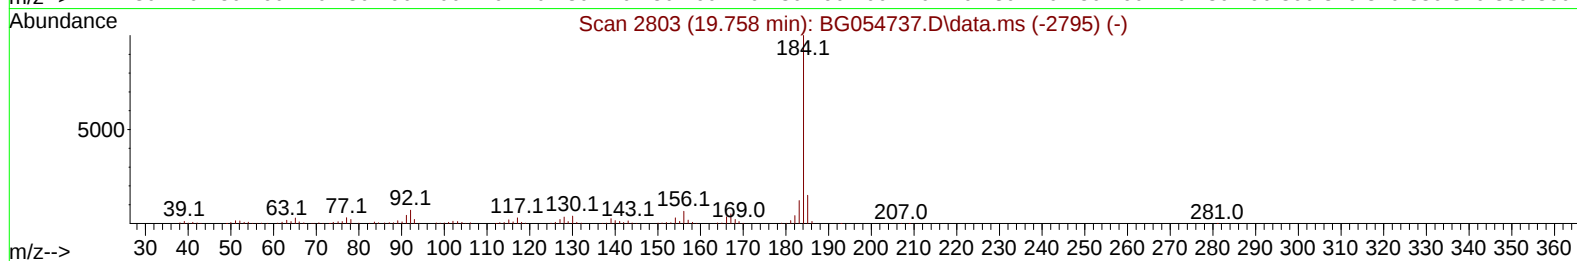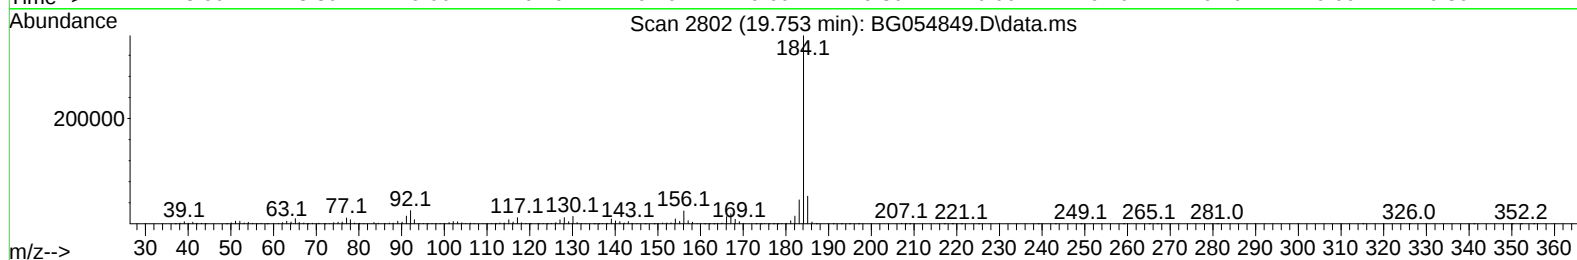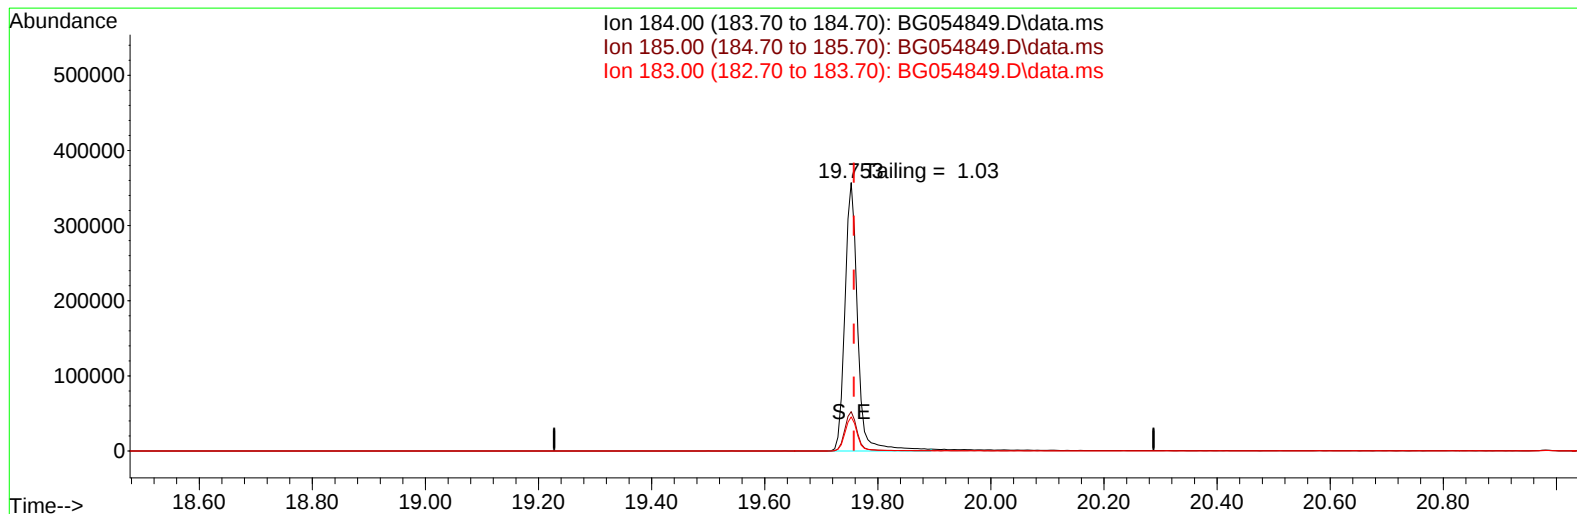

TIC: BG054849.D\data.ms

(77) Benzidine

19.753min (-0.005) 362145.72 ng

response 565104

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.71
183.00	12.30	12.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/6/2022	BNA_G	BG054849.D
Compound Name	Response	Retention Time
DDT	253002	20.981
DDD	10213	20.534
DDE	948	20.029
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11161	264163	4.23

Instrument :
BNA_G
ClientSampleId :
DFTPP