
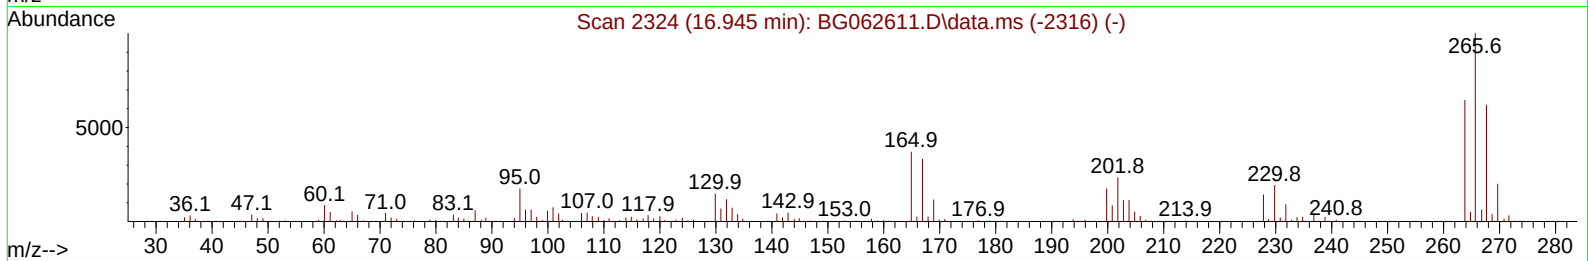
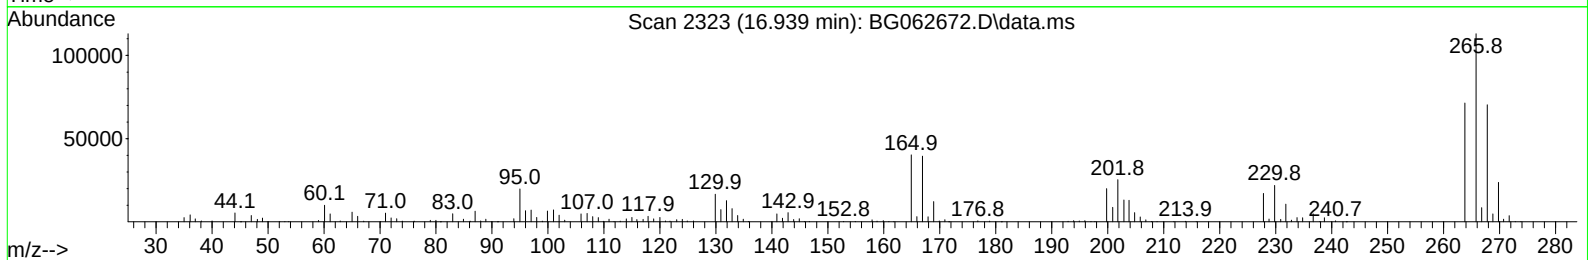


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090624\
Data File : BG062672.D
Acq On : 6 Sep 2024 8:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 11:00:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

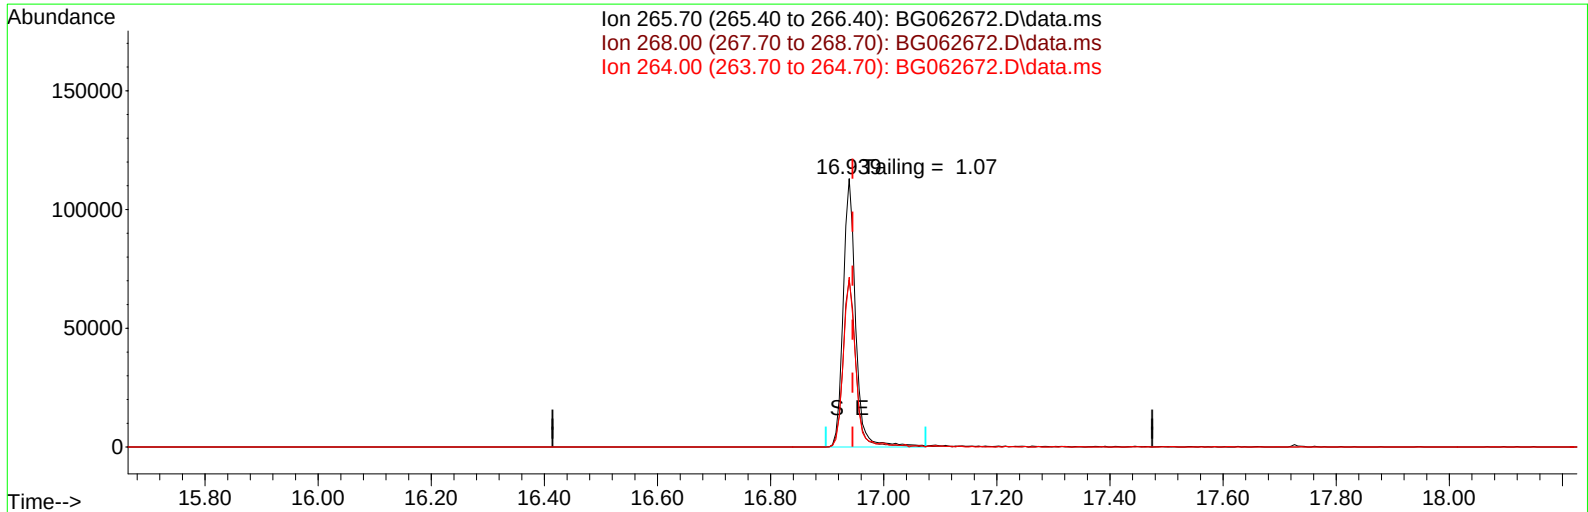

TIC: BG062672.D\data.ms

(70) Pentachlorophenol (C)




16.939min (-0.006) 142305.99 ng

response 173790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.26
264.00	64.50	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090624\
Data File : BG062672.D
Acq On : 6 Sep 2024 8:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 11:00:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

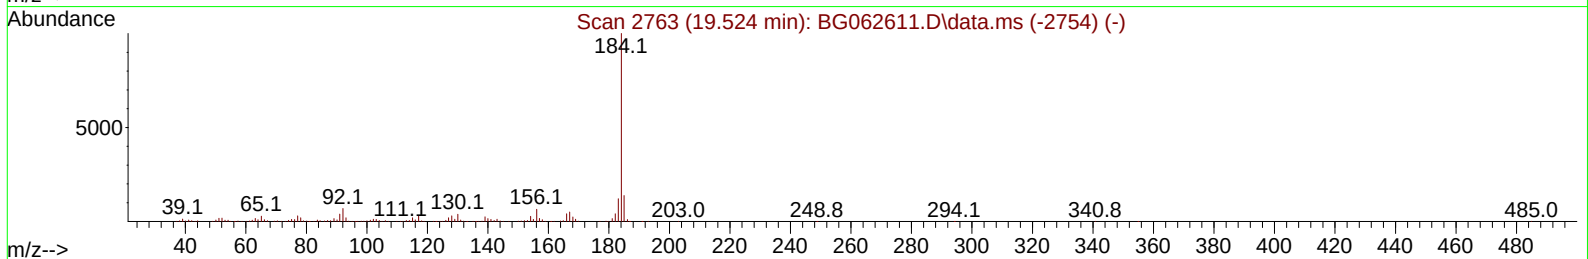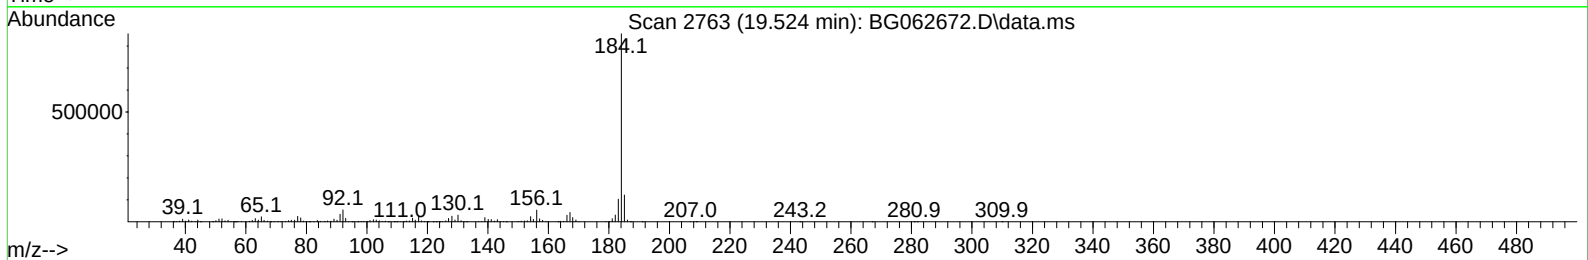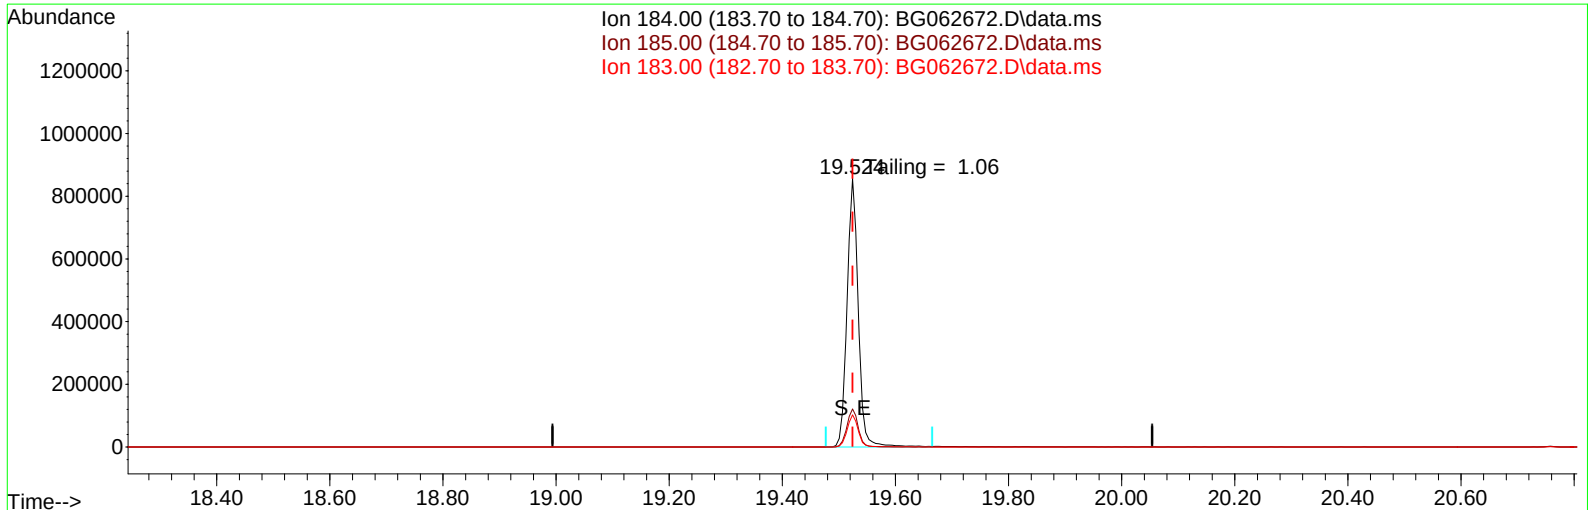

TIC: BG062672.D\data.ms

(77) Benzidine**19.524min (+ 0.000) 49296.56 ng****response 1181727**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.23
183.00	12.10	11.98
0.00	0.00	0.00