
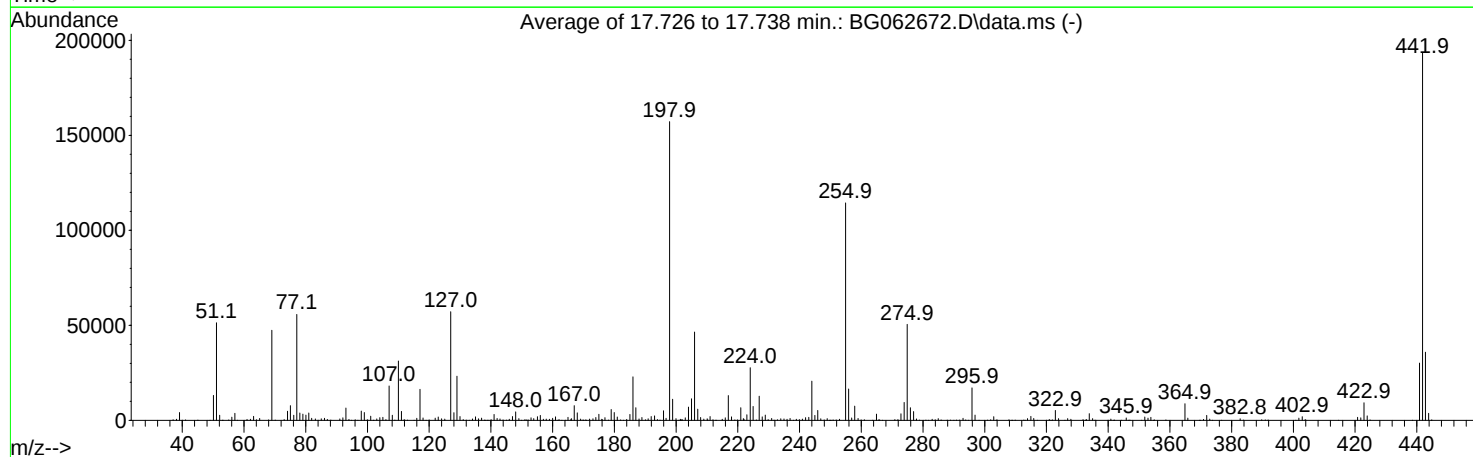


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090624\
Data File : BG062672.D
Acq On : 6 Sep 2024 8:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 31 02:36:01 2024

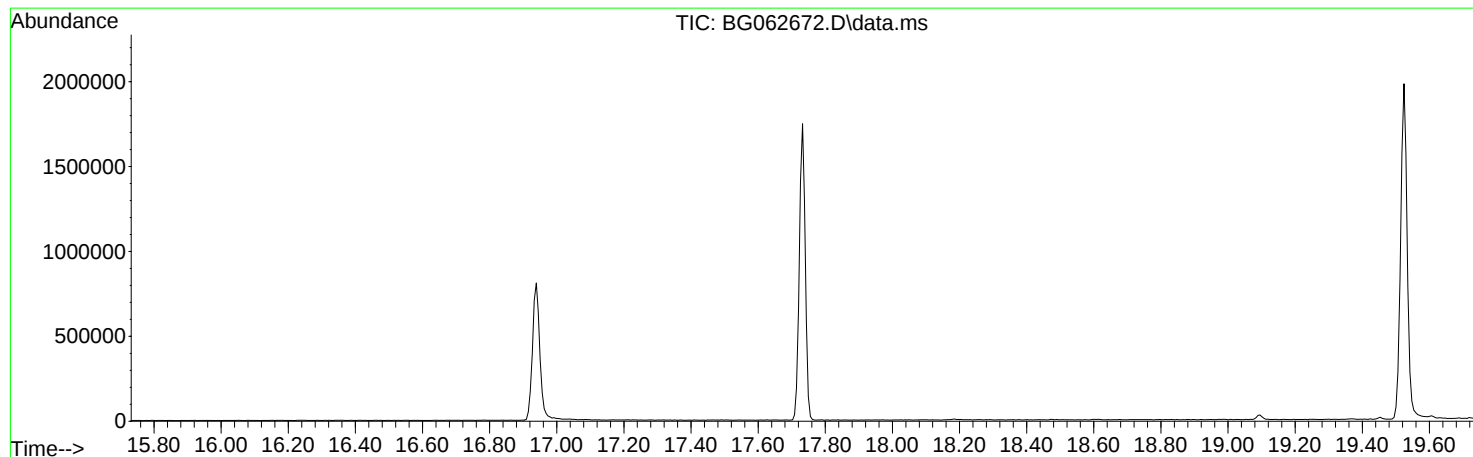

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	51368	PASS
68	69	0.00	2	0.5	250	PASS
69	198	0.00	100	30.2	47427	PASS
70	69	0.00	2	0.4	202	PASS
127	198	10	80	36.4	57208	PASS
197	198	0.00	2	0.7	1059	PASS
198	198	100	100	100.0	157227	PASS
199	198	5	9	7.1	11102	PASS
275	198	10	60	32.1	50504	PASS
365	198	1	100	5.6	8771	PASS
441	198	0.01	100	19.1	30104	PASS
442	442	50	100	100.0	193579	PASS
443	442	15	24	18.5	35856	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/6/2024	BNA_G	<u>BG062672.D</u>
Compound Name	Response	Retention Time
DDT	530506	20.758
DDD	12099	20.317
DDE	280	19.818
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12379	542885	2.28

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090624\
Data File : BG062672.D
Acq On : 6 Sep 2024 8:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 06 11:00:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

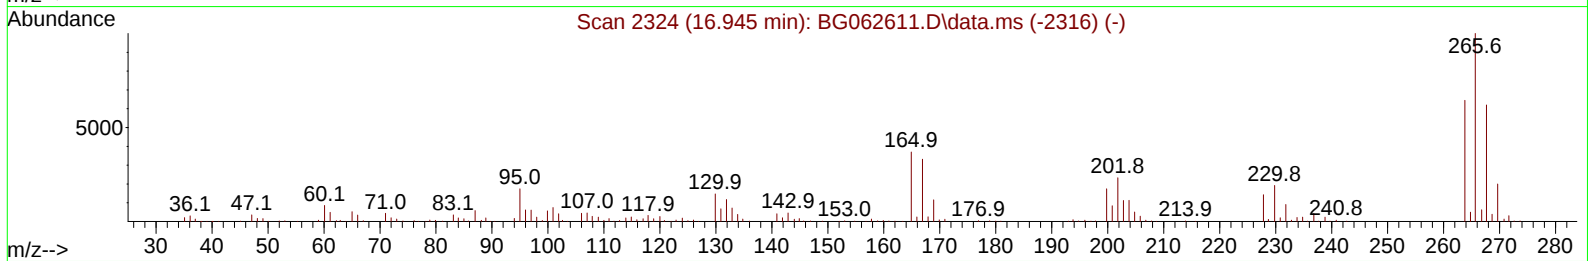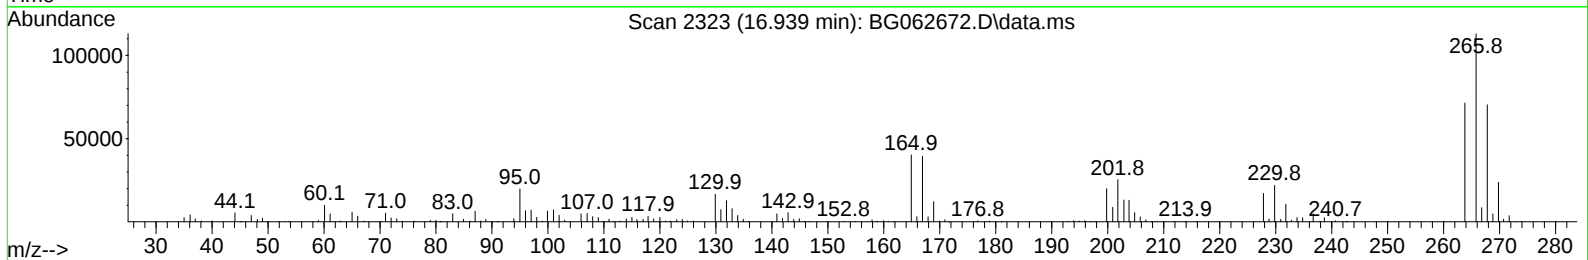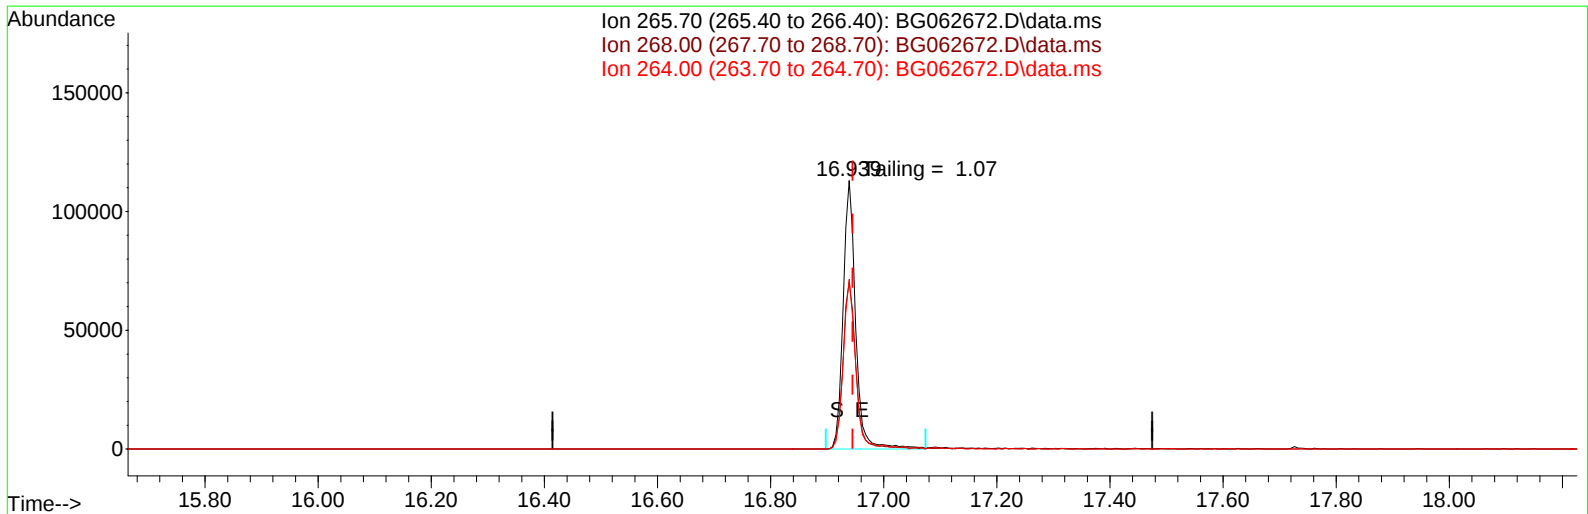

TIC: BG062672.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.006) 142305.99 ng




response 173790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.26
264.00	64.50	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090624\
Data File : BG062672.D
Acq On : 6 Sep 2024 8:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 06 11:00:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

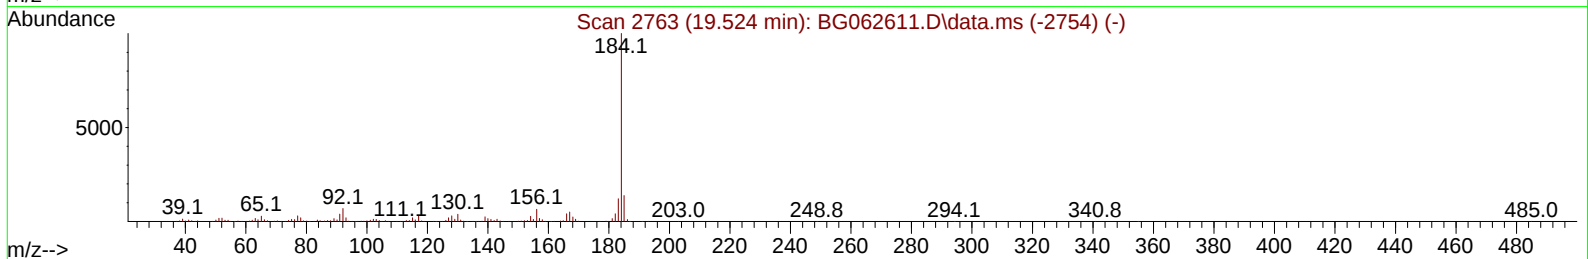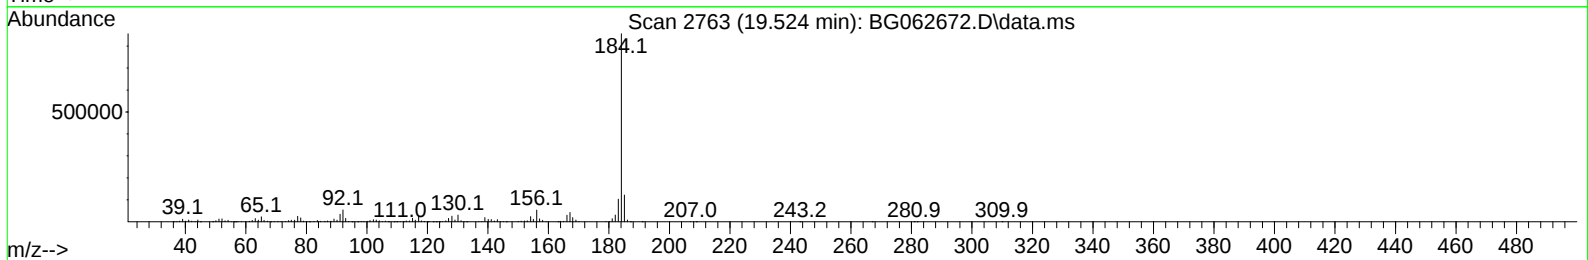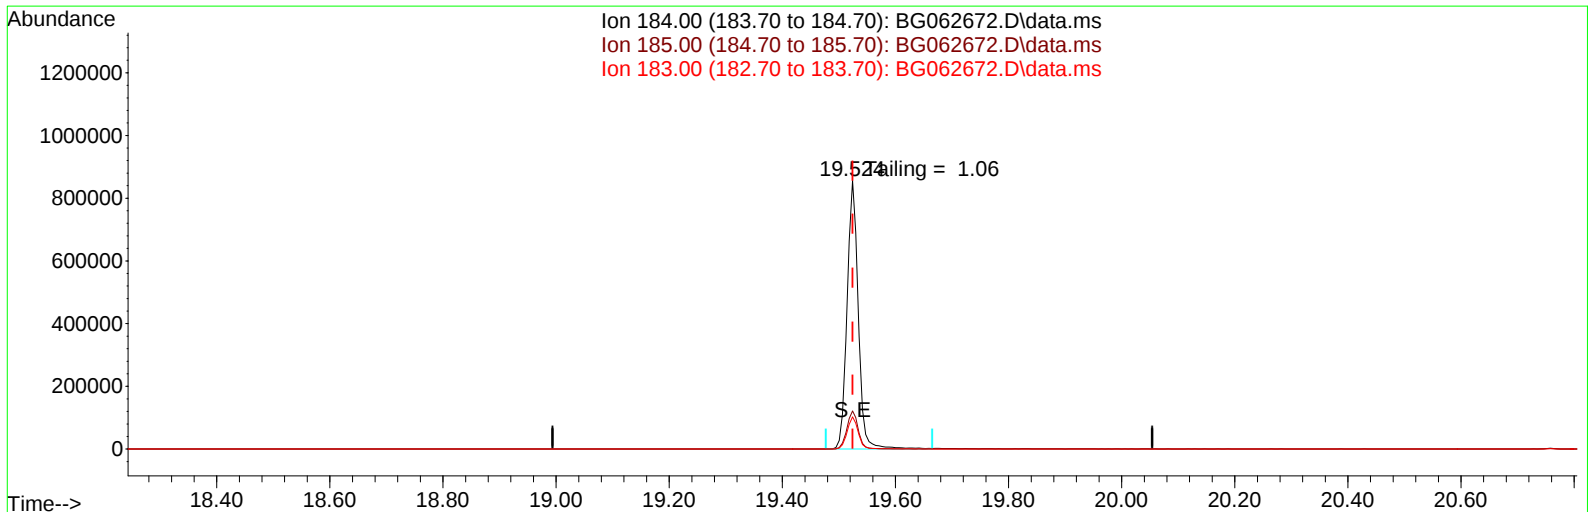

TIC: BG062672.D\data.ms

(77) Benzidine

19.524min (+ 0.000) 49296.56 ng

response 1181727

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.23
183.00	12.10	11.98
0.00	0.00	0.00