
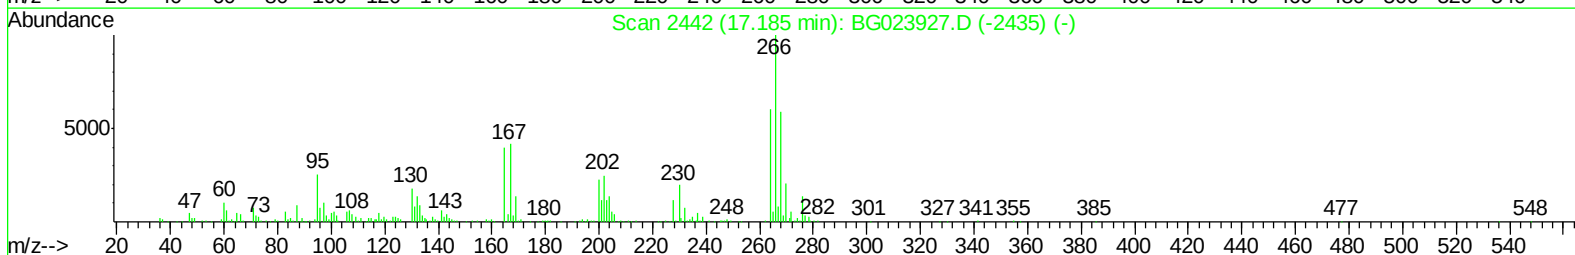
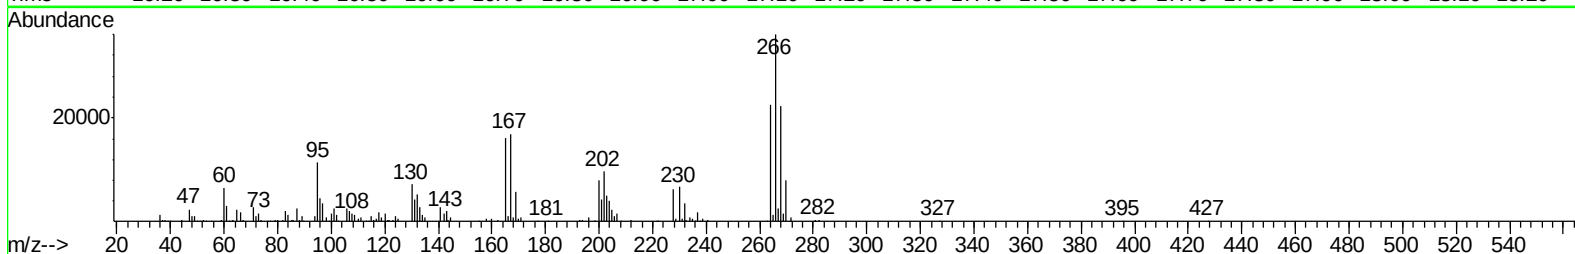


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090716\
Data File : BG023955.D
Acq On : 7 Sep 2016 13:55
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 09:52:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 20:05:47 2016
Response via : Initial Calibration

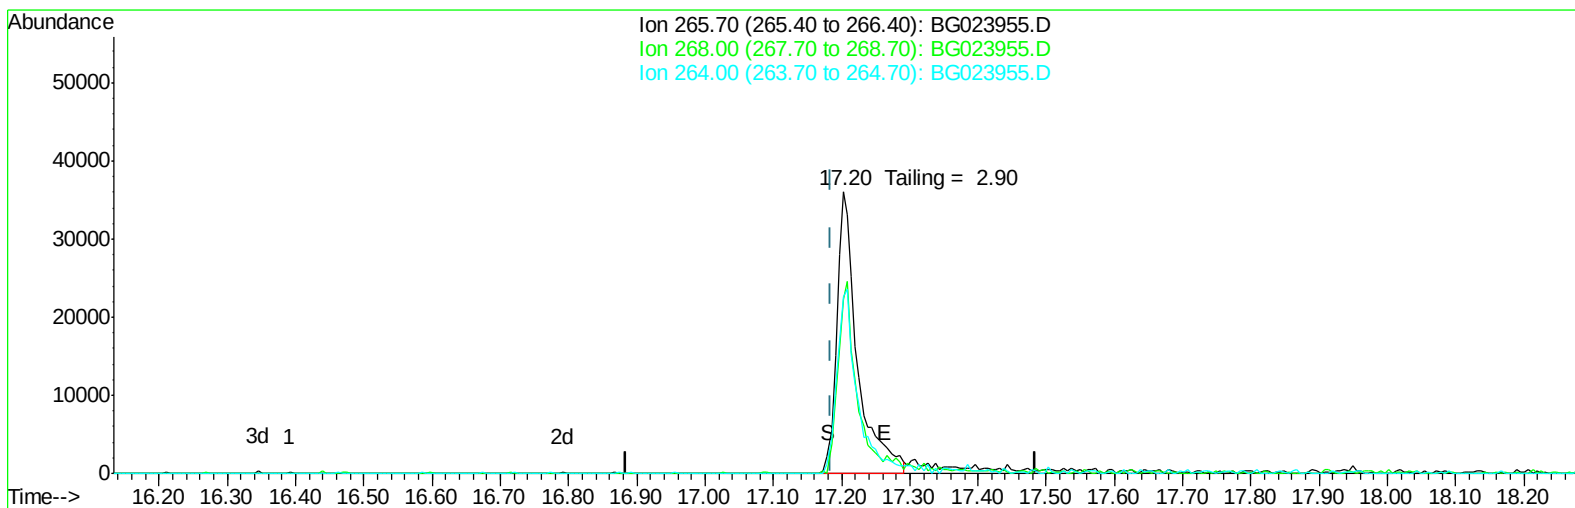

TIC: BG023955.D

(69) Pentachlorophenol (C)




17.203min (+0.017) 149214.73ng m

response 74634

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	61.92
264.00	63.20	62.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090716\
 Data File : BG023955.D
 Acq On : 7 Sep 2016 13:55
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 09:52:58 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 31 20:05:47 2016
 Response via : Initial Calibration

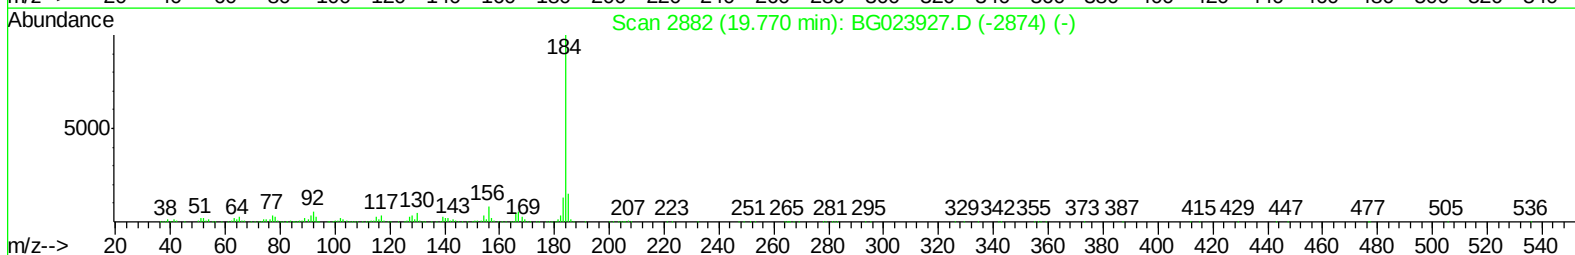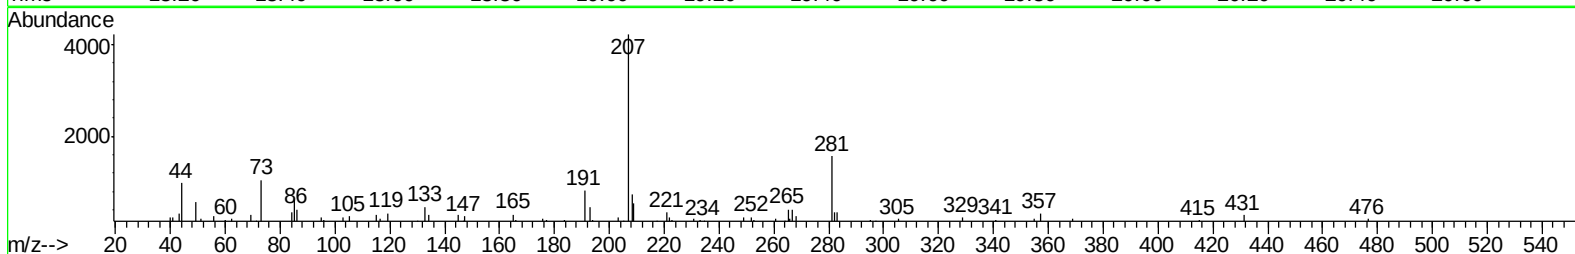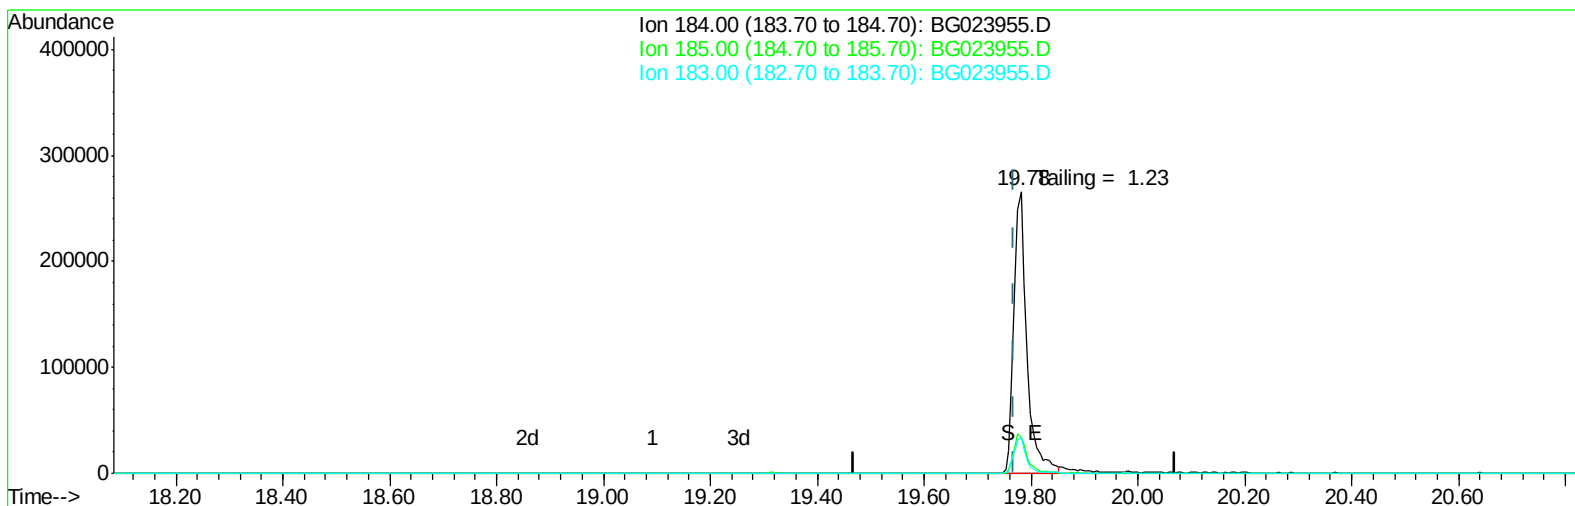

TIC: BG023955.D

(76) Benzidine

19.094min (-0.676) 0.43ng

response 68

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	0.00#
183.00	13.40	0.00#
0.00	0.00	0.00