


Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG090716\  
 Data File : BG023955.D  
 Acq On : 7 Sep 2016 13:55  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG083116.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Aug 31 20:05:47 2016

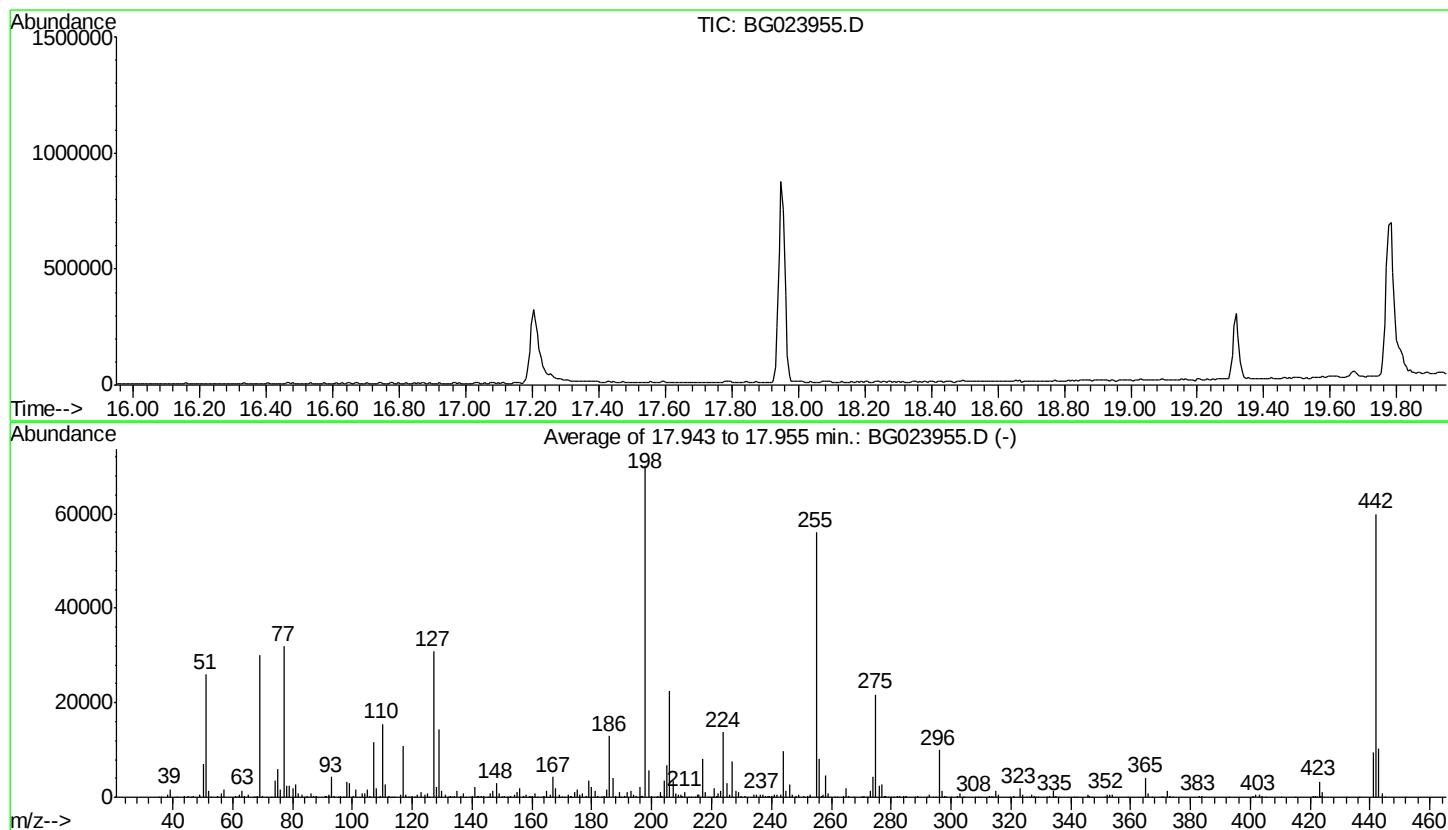

AutoFind: Scans 2571, 2572, 2573; Background Corrected with Scan 2565

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 37.0      | 25978   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.0       | 300     | PASS             |
| 69          | 198          | 0.00         | 100          | 42.8      | 30064   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 156     | PASS             |
| 127         | 198          | 10           | 80           | 43.9      | 30826   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 290     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 70208   | PASS             |
| 199         | 198          | 5            | 9            | 8.3       | 5818    | PASS             |
| 275         | 198          | 10           | 60           | 30.9      | 21706   | PASS             |
| 365         | 198          | 1            | 100          | 6.0       | 4208    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.9      | 9532    | PASS             |
| 442         | 198          | 50           | 100          | 85.4      | 59978   | PASS             |
| 443         | 442          | 15           | 24           | 17.1      | 10273   | PASS             |