


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG090717\
 Data File : BG028591.D
 Acq On : 7 Sep 2017 13:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG090717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 07 18:39:50 2017

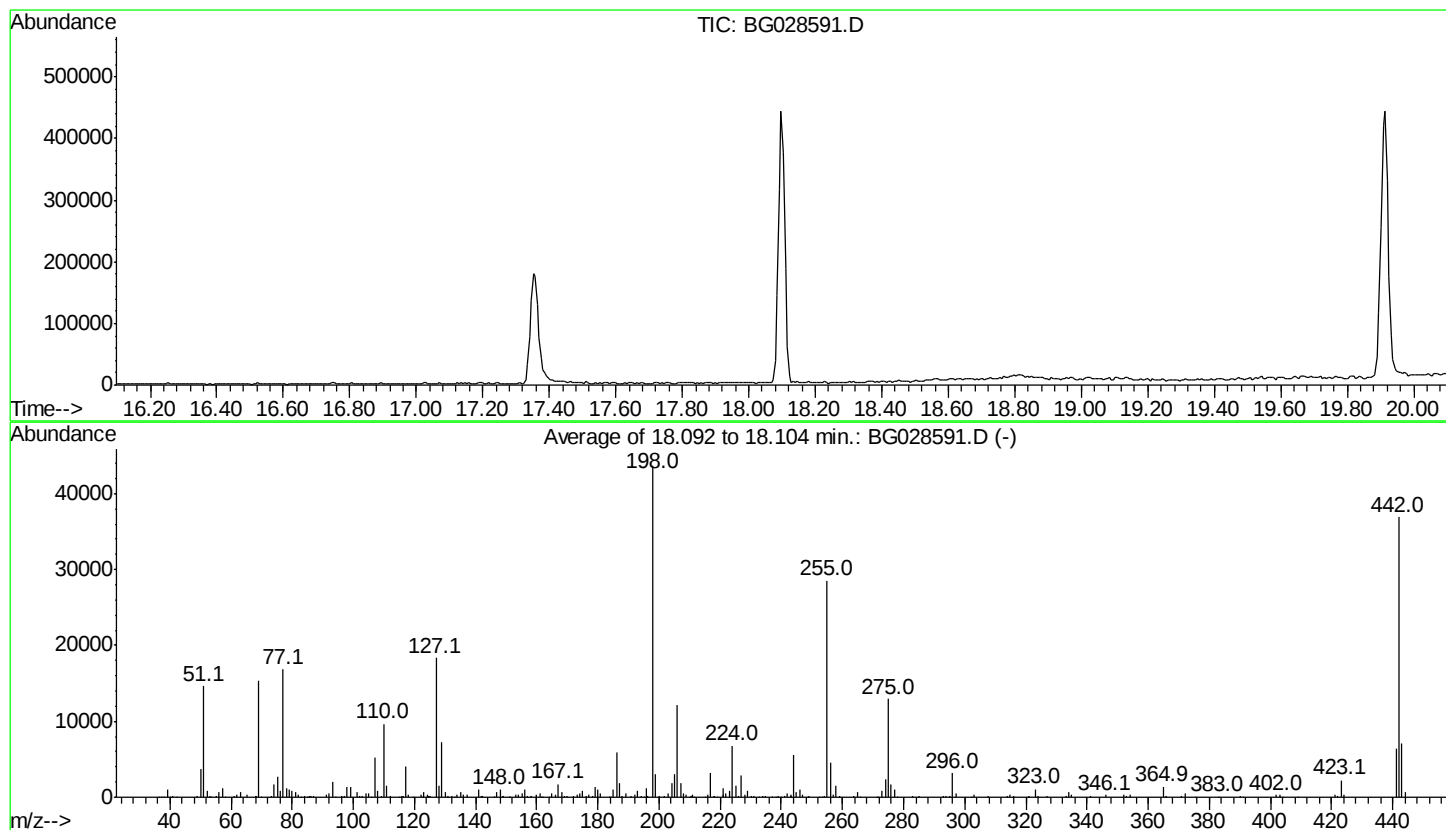

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	14637	PASS
68	69	0.00	2	1.1	168	PASS
69	198	0.00	100	35.2	15394	PASS
70	69	0.00	2	0.4	67	PASS
127	198	10	80	42.0	18367	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43690	PASS
199	198	5	9	7.0	3057	PASS
275	198	10	60	29.6	12944	PASS
365	198	1	100	3.2	1391	PASS
441	442	0.01	24	17.4	6434	PASS
442	198	50	100	84.4	36890	PASS
443	442	15	24	19.2	7100	PASS