

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050212.D
 Acq On : 9 Sep 2021 00:13
 Operator : CG/JU
 Sample : M3608-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKK0

Manual Integrations
 APPROVED

mohammad
 9/9/2021 11:47:01 AM

Quant Time: Sep 09 00:57:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 07 18:32:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	50149	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	275247	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.610	164	115891	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.365	188	256921	20.000	ng/ul	0.00
79) Chrysene-d12	21.636	240	268627	20.000	ng/ul	0.00
88) Perylene-d12	24.849	264	270904	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	2939	2.897	ng/uL	0.00
4) Pyridine-d5	3.749	84	29486m	8.189	ng/ul	0.00
7) Phenol-d5	7.126	99	27697	7.113	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.267	67	52588	23.126	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.479	132	60975	18.869	ng/ul	0.00
15) 4-Methylphenol-d8	8.671	113	72406	23.651	ng/ul	0.00
21) Nitrobenzene-d5	9.124	128	46312	24.513	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	78773	34.289	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.398	165	119482	27.250	ng/ul	0.00
31) 4-Chloroaniline-d4	10.909	131	112177	20.766	ng/ul	0.00
46) Dimethylphthalate-d6	14.011	166	255672	29.217	ng/ul	0.00
49) Acenaphthylene-d8	14.299	160	302554	29.037	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.863	143	6882m	6.518	ng/ul	0.00
60) Fluorene-d10	15.603	176	224898	30.953	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.744	200	40123	25.889	ng/ul	0.00
73) Anthracene-d10	17.459	188	384102	33.303	ng/ul	0.00
81) Pyrene-d10	19.756	212	461441	34.486	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.626	264	458594	31.978	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.501	149	10302	1.106	ng/ul#	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050212.D
Acq On : 9 Sep 2021 00:13
Operator : CG/JU
Sample : M3608-04
Misc :
ALS Vial : 40 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
DBKK0

Manual Integrations
APPROVED

mohammad
9/9/2021 11:47:01 AM

Quant Time: Sep 09 00:57:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 07 18:32:38 2021
Response via : Initial Calibration

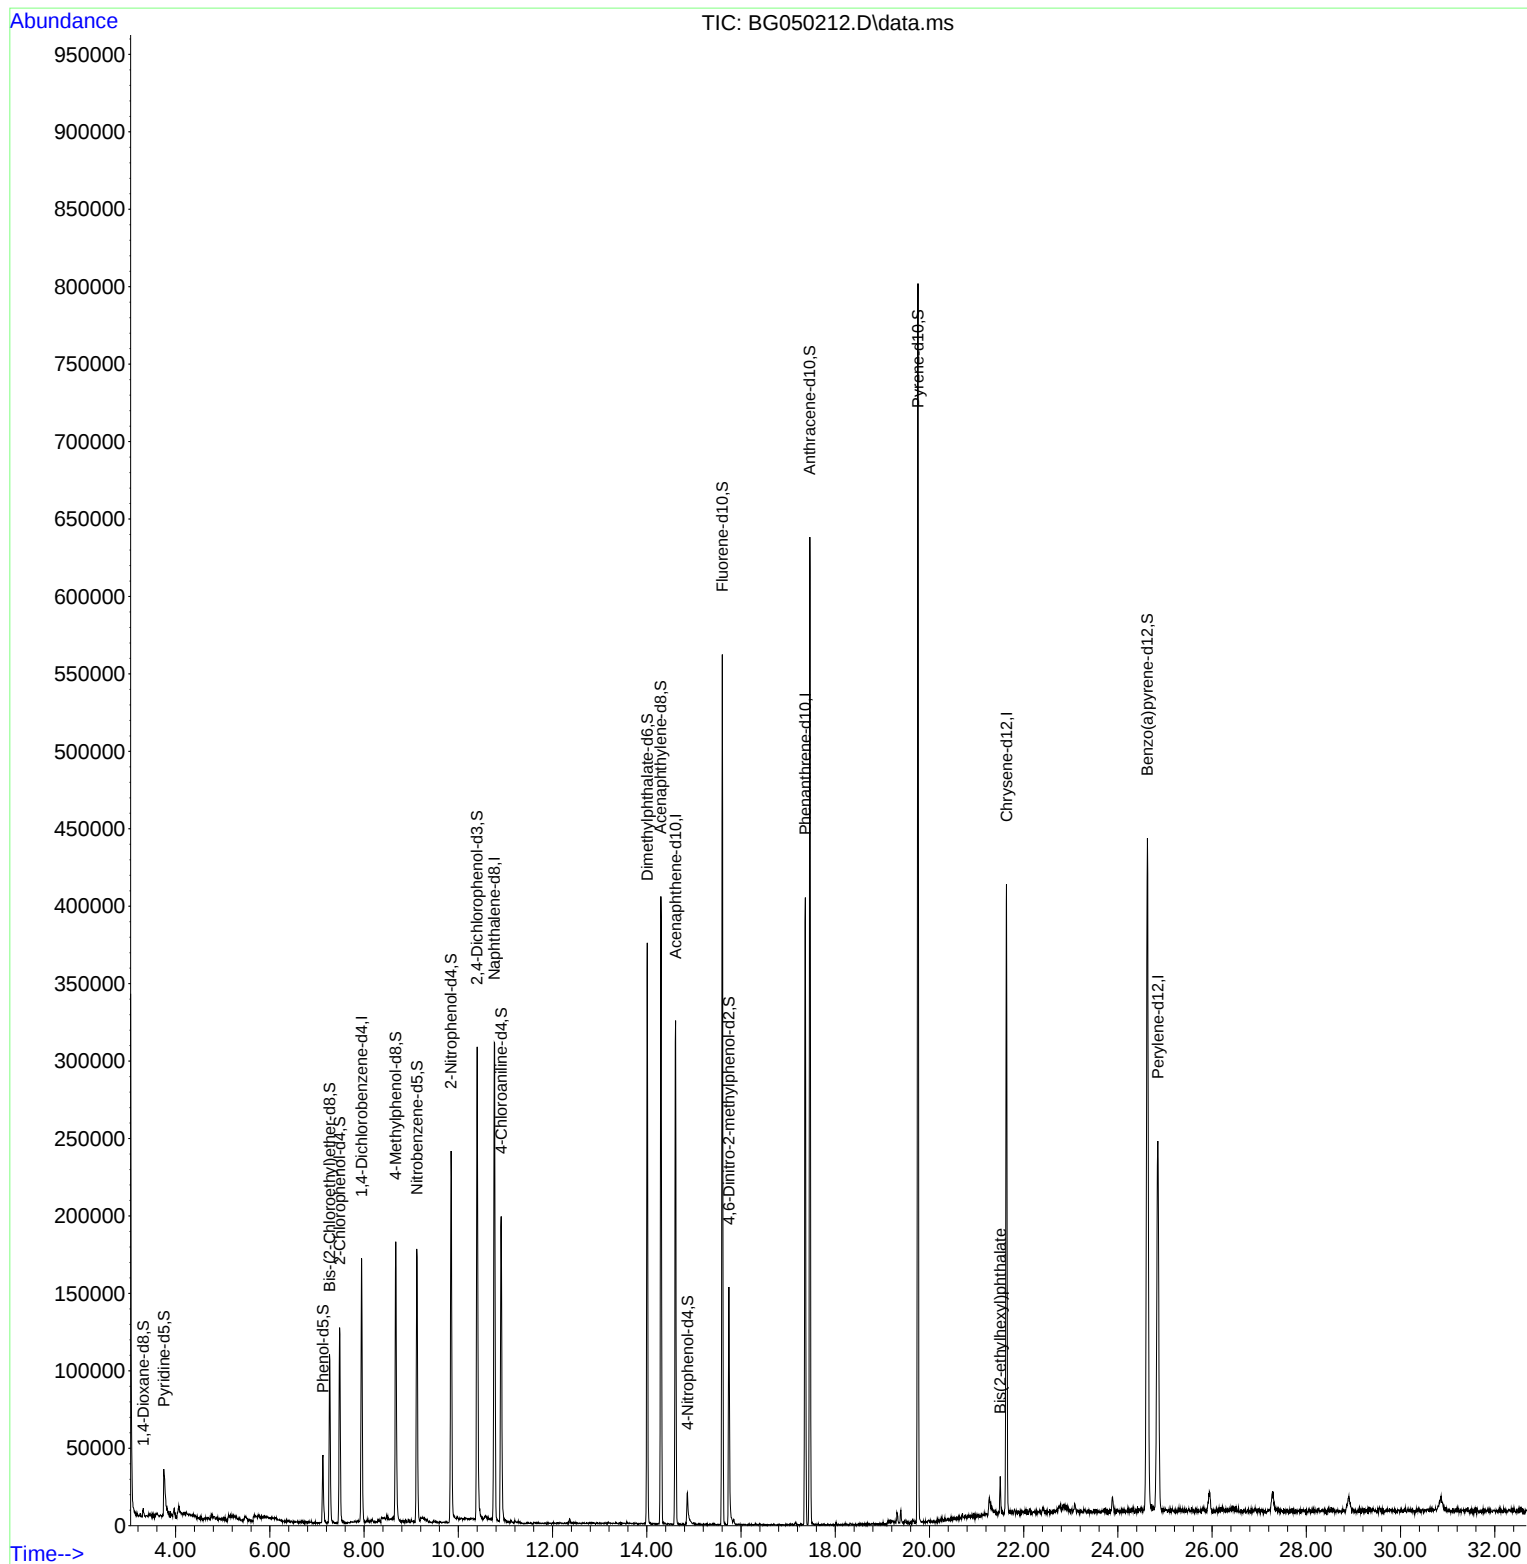

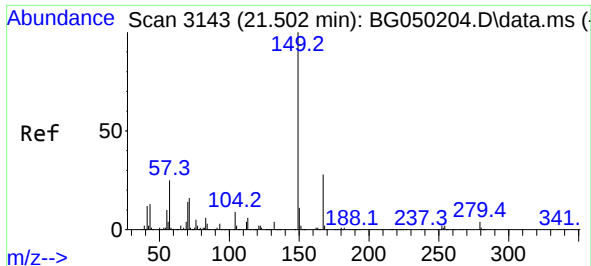

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.106 ng/ul
RT: 21.501 min Scan# 3143
Delta R.T. -0.008 min
Lab File: BG050212.D
Acq: 9 Sep 2021 00:13

Tgt Ion	Ratio	Lower	Upper
149	100		
167	21.2	20.4	30.6
279	3.1	3.7	5.5#

Instrument :
BNA_G
ClientSampleId :
DBKK0

Manual Integrations
APPROVED

mohammad
9/9/2021 11:47:01 AM

