

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050190.D
 Acq On : 8 Sep 2021 8:20
 Operator : CG/JU
 Sample : PB138845BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK845

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.304	42	45	50	rVB3	6799	10250	1.15%	0.105%
2	3.539	83	85	86	rBV2	3077	2279	0.26%	0.023%
3	3.733	116	118	129	rBV	118417	236686	26.63%	2.432%
4	3.968	155	158	159	rBV3	2705	2936	0.33%	0.030%
5	4.114	182	183	187	rBV2	3919	4861	0.55%	0.050%
6	4.173	191	193	194	rBV	2879	2062	0.23%	0.021%
7	4.490	245	247	252	rBV3	5210	7624	0.86%	0.078%
8	4.614	266	268	270	rVB2	2358	1623	0.18%	0.017%
9	4.673	276	278	281	rVB2	1987	1791	0.20%	0.018%
10	4.725	286	287	291	rBV	2973	2084	0.23%	0.021%
11	4.843	302	307	314	rBV4	5492	15587	1.75%	0.160%
12	5.078	345	347	349	rBV3	1236	1410	0.16%	0.014%
13	5.906	486	488	489	rBV	2061	1579	0.18%	0.016%
14	5.977	495	500	502	rBV3	4221	6715	0.76%	0.069%
15	6.323	555	559	561	rBV3	2778	3616	0.41%	0.037%
16	6.394	570	571	574	rVB2	2051	1502	0.17%	0.015%
17	6.558	597	599	602	rVB	2503	1966	0.22%	0.020%
18	7.052	680	683	685	rVB2	1306	1355	0.15%	0.014%
19	7.122	688	695	704	rVV	141165	247358	27.83%	2.542%
20	7.269	714	720	730	rVV	101277	166570	18.74%	1.712%
21	7.480	749	756	767	rBV	140612	246976	27.79%	2.538%
22	7.557	767	769	773	rBV3	2034	1731	0.19%	0.018%
23	7.945	829	835	843	rBV	113153	197089	22.17%	2.025%
24	8.279	890	892	893	rBV	1726	1423	0.16%	0.015%
25	8.362	904	906	911	rBV3	1809	2485	0.28%	0.026%
26	8.450	918	921	924	rBV3	1746	1817	0.20%	0.019%
27	8.544	936	937	939	rBV2	2323	2001	0.23%	0.021%
28	8.673	952	959	970	rBV	237805	394934	44.43%	4.058%
29	8.890	995	996	997	rBV	2707	1894	0.21%	0.019%
30	9.119	1028	1035	1047	rVB2	175667	311571	35.05%	3.202%
31	9.231	1052	1054	1061	rBV4	2965	6237	0.70%	0.064%
32	9.378	1077	1079	1082	rBV	2068	1866	0.21%	0.019%
33	9.401	1082	1083	1088	rVB	2396	2411	0.27%	0.025%
34	9.437	1088	1089	1092	rBV2	1550	1688	0.19%	0.017%
35	9.848	1152	1159	1168	rBV	127234	218698	24.61%	2.247%
36	10.059	1190	1195	1197	rBV2	1203	1877	0.21%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050190.D
 Acq On : 8 Sep 2021 8:20
 Operator : CG/JU
 Sample : PB138845BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK845

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

37	10.083	1197	1199	1202	rVB2	1806	1768	0.20%	0.018%
38	10.400	1247	1253	1264	rBV	167279	314445	35.38%	3.231%
39	10.770	1308	1316	1325	rVB	155308	282328	31.76%	2.901%
40	10.905	1332	1339	1351	rBV	154755	300313	33.79%	3.086%
41	11.475	1434	1436	1439	rVB	1841	1361	0.15%	0.014%
42	12.033	1529	1531	1538	rBV2	1120	2045	0.23%	0.021%
43	12.380	1584	1590	1593	rVB4	2381	3979	0.45%	0.041%
44	12.744	1648	1652	1655	rVB2	1433	1982	0.22%	0.020%
45	12.773	1655	1657	1661	rBV2	1973	3147	0.35%	0.032%
46	12.873	1673	1674	1679	rBV	1882	2863	0.32%	0.029%
47	12.944	1684	1686	1690	rBV2	1288	1546	0.17%	0.016%
48	12.991	1693	1694	1698	rBV2	2755	3343	0.38%	0.034%
49	13.226	1732	1734	1735	rBV	2344	1925	0.22%	0.020%
50	13.437	1769	1770	1776	rBV	2554	3794	0.43%	0.039%
51	14.013	1861	1868	1879	rVB	316916	481724	54.20%	4.950%
52	14.154	1889	1892	1894	rBV	1102	1422	0.16%	0.015%
53	14.301	1909	1917	1930	rBV	343280	557253	62.69%	5.726%
54	14.500	1948	1951	1955	rBV2	1417	1844	0.21%	0.019%
55	14.606	1963	1969	1976	rBV	246143	387157	43.56%	3.978%
56	14.847	2000	2010	2024	rBV2	76304	173988	19.57%	1.788%
57	15.605	2132	2139	2149	rVB	461118	690462	77.68%	7.095%
58	15.746	2157	2163	2177	rBV2	102942	185246	20.84%	1.903%
59	15.840	2177	2179	2180	rBV	2476	1648	0.19%	0.017%
60	17.150	2398	2402	2405	rBV2	1055	1464	0.16%	0.015%
61	17.361	2431	2438	2445	rBV	319871	484646	54.53%	4.980%
62	17.461	2449	2455	2464	rBV2	494358	753502	84.77%	7.743%
63	17.579	2474	2475	2479	rBV	1549	1513	0.17%	0.016%
64	17.761	2503	2506	2509	rBV3	1147	1641	0.18%	0.017%
65	19.188	2747	2749	2752	rBV2	1478	2103	0.24%	0.022%
66	19.317	2768	2771	2778	rVB4	5190	7530	0.85%	0.077%
67	19.394	2778	2784	2790	rVB2	7761	13716	1.54%	0.141%
68	19.464	2793	2796	2797	rBV2	1813	1928	0.22%	0.020%
69	19.505	2802	2803	2808	rVB3	2489	2581	0.29%	0.027%
70	19.646	2822	2827	2829	rBV4	2293	3075	0.35%	0.032%
71	19.758	2839	2846	2854	rBV	616496	888832	100.00%	9.133%
72	19.987	2882	2885	2888	rVB4	1352	1804	0.20%	0.019%
73	20.081	2897	2901	2902	rVB2	2016	1972	0.22%	0.020%
74	20.105	2902	2905	2908	rBV2	1630	2163	0.24%	0.022%
75	20.269	2932	2933	2936	rVB2	2382	1539	0.17%	0.016%
76	20.404	2954	2956	2957	rBV2	1509	1387	0.16%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050190.D
 Acq On : 8 Sep 2021 8:20
 Operator : CG/JU
 Sample : PB138845BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK845

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

77	20.475	2967	2968	2970	rBV2	2646	1681	0.19%	0.017%
78	20.504	2970	2973	2977	rVV3	2513	3685	0.41%	0.038%
79	20.921	3039	3044	3046	rBV4	2645	4329	0.49%	0.044%
80	21.068	3066	3069	3071	rBV3	2760	3455	0.39%	0.036%
81	21.221	3093	3095	3096	rBV2	2849	1640	0.18%	0.017%
82	21.285	3105	3106	3107	rBV	3868	1722	0.19%	0.018%
83	21.326	3112	3113	3115	rBV2	2819	1743	0.20%	0.018%
84	21.638	3160	3166	3173	rBV	331560	537404	60.46%	5.522%
85	21.967	3220	3222	3223	rBV2	3727	2115	0.24%	0.022%
86	23.089	3409	3413	3422	rVB7	8840	19184	2.16%	0.197%
87	23.559	3491	3493	3496	rBV4	2823	2878	0.32%	0.030%
88	23.894	3544	3550	3554	rBV7	12067	23304	2.62%	0.239%
89	24.634	3666	3676	3689	rVB2	309755	850543	95.69%	8.740%
90	24.851	3703	3713	3725	rVB2	194022	552255	62.13%	5.675%
91	25.427	3810	3811	3813	rBV2	4793	3654	0.41%	0.038%
92	26.079	3921	3922	3923	rBV	6183	3734	0.42%	0.038%
93	26.320	3961	3963	3966	rBV3	6920	6290	0.71%	0.065%
94	27.236	4117	4119	4120	rBV2	3745	3079	0.35%	0.032%
95	28.393	4314	4316	4318	rBV3	3301	2689	0.30%	0.028%
96	28.440	4322	4324	4325	rVB2	3147	2072	0.23%	0.021%
97	30.209	4623	4625	4628	rBV3	3025	2758	0.31%	0.028%
98	30.555	4683	4684	4685	rBV	3953	1750	0.20%	0.018%
99	31.736	4884	4885	4887	rBV2	3243	1558	0.18%	0.016%
100	32.018	4931	4933	4937	rVB5	6234	6912	0.78%	0.071%




Sum of corrected areas: 9731965

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050190.D
Acq On : 8 Sep 2021 8:20
Operator : CG/JU
Sample : PB138845BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK845

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

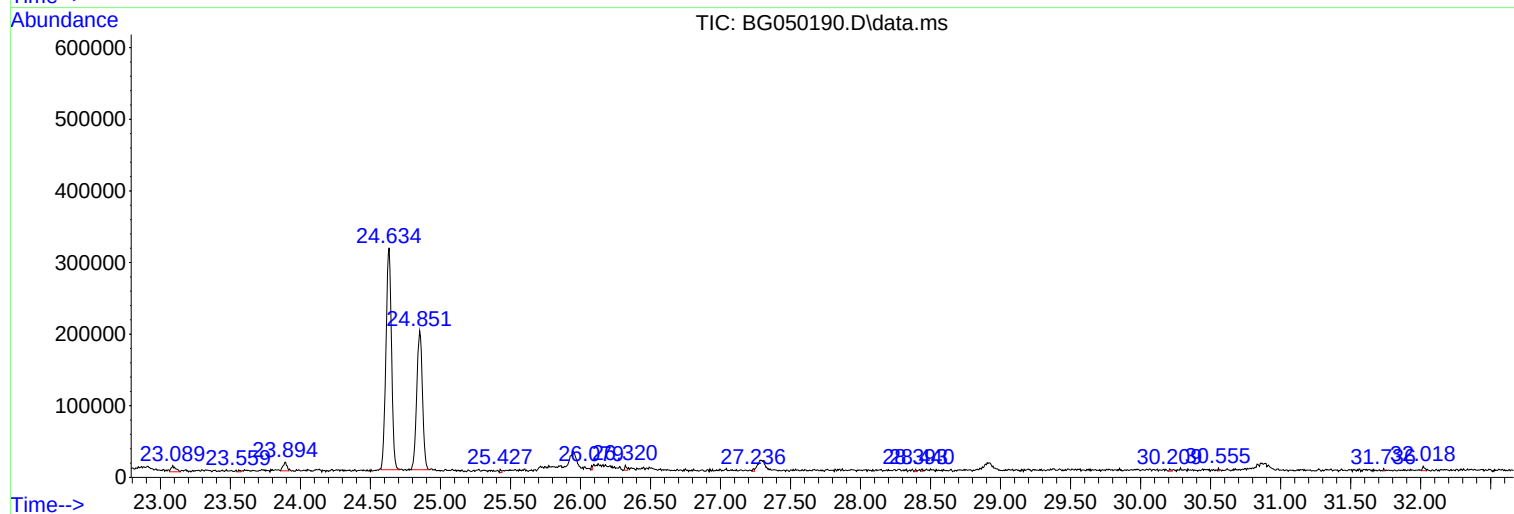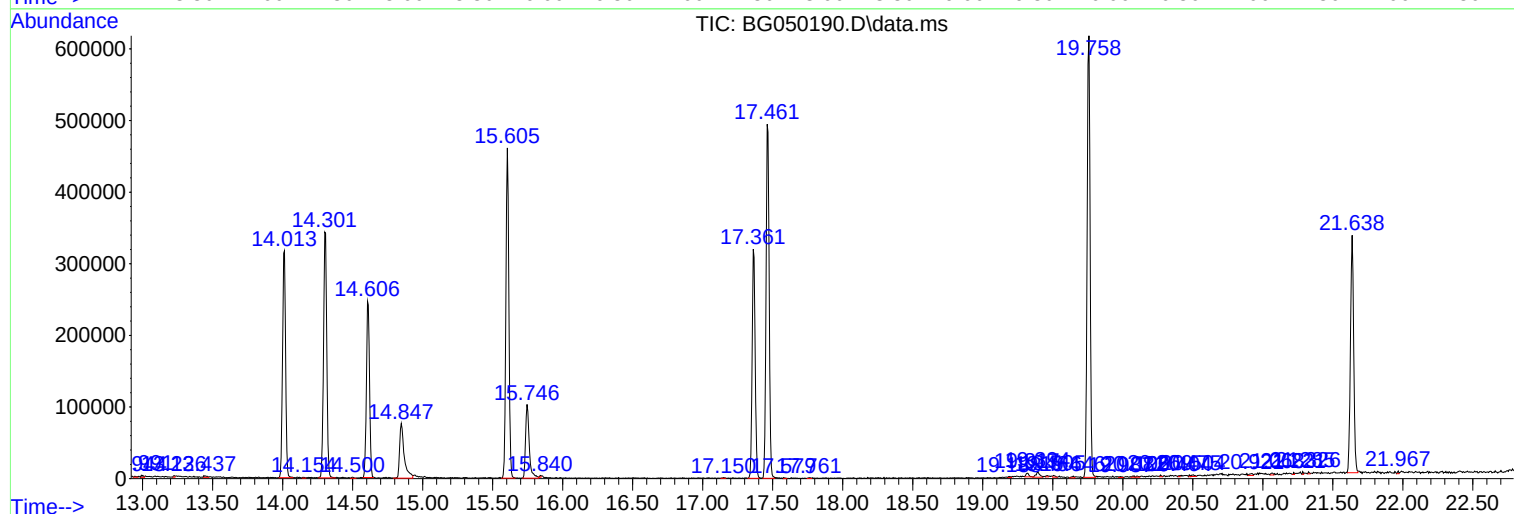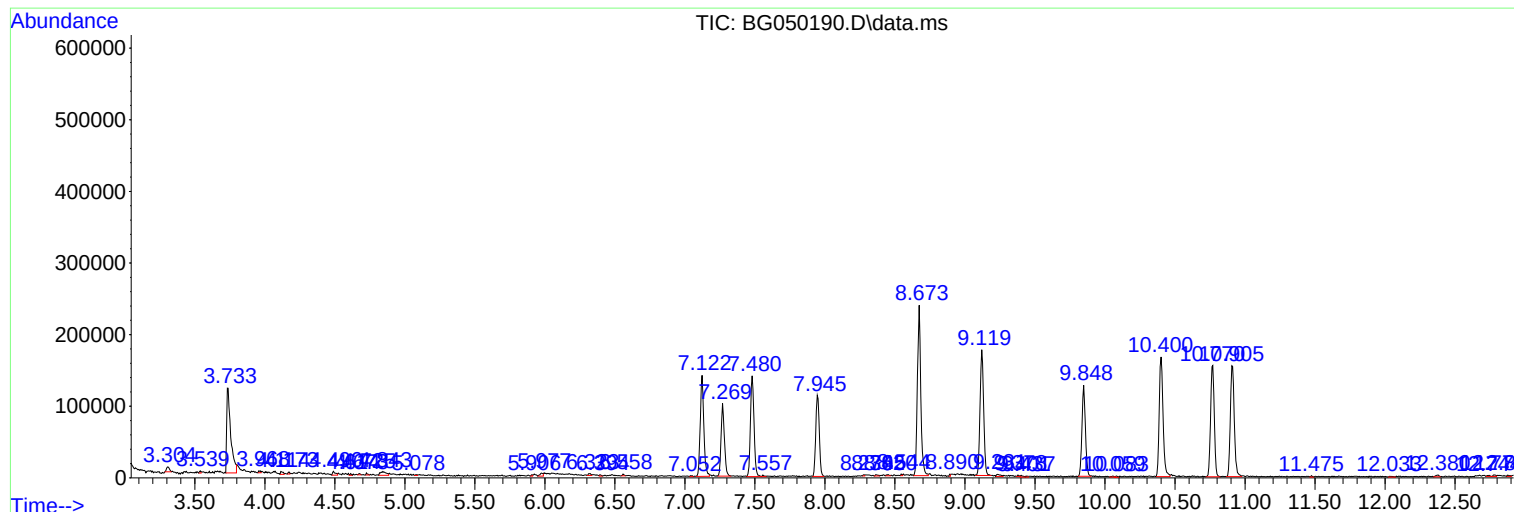

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050190.D
Acq On : 8 Sep 2021 8:20
Operator : CG/JU
Sample : PB138845BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK845

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050190.D
Acq On : 8 Sep 2021 8:20
Operator : CG/JU
Sample : PB138845BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK845

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
