

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050197.D
 Acq On : 8 Sep 2021 13:08
 Operator : CG/JU
 Sample : M3566-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKH0

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.309	44	46	48	rBV3	2943	3048	0.28%	0.029%
2	3.391	58	60	63	rVB3	3198	2374	0.21%	0.023%
3	3.744	117	120	135	rBV	32976	86167	7.80%	0.832%
4	5.101	348	351	354	rBV3	3292	4801	0.43%	0.046%
5	5.594	431	435	436	rVB3	2051	1996	0.18%	0.019%
6	6.129	524	526	529	rBV	2840	3352	0.30%	0.032%
7	6.493	586	588	591	rVB2	1465	1488	0.13%	0.014%
8	6.951	663	666	668	rBV2	2118	2636	0.24%	0.025%
9	7.086	686	689	690	rBV	1520	1666	0.15%	0.016%
10	7.128	690	696	703	rVV	41575	76150	6.89%	0.735%
11	7.274	713	721	731	rBV	117016	212664	19.25%	2.054%
12	7.415	743	745	746	rBV2	2676	2407	0.22%	0.023%
13	7.480	750	756	768	rVB	139721	252566	22.87%	2.439%
14	7.627	777	781	783	rBV2	3613	4009	0.36%	0.039%
15	7.950	829	836	843	rBV	156105	274422	24.84%	2.650%
16	8.672	953	959	971	rBV	127466	244260	22.11%	2.359%
17	9.119	1029	1035	1045	rVB	170521	313705	28.40%	3.030%
18	9.759	1142	1144	1147	rVB2	1273	1510	0.14%	0.015%
19	9.847	1152	1159	1169	rVB	119854	211271	19.13%	2.040%
20	10.400	1247	1253	1265	rBV	156943	293793	26.60%	2.837%
21	10.546	1275	1278	1279	rBV2	3822	3693	0.33%	0.036%
22	10.770	1308	1316	1327	rBV	160239	289849	26.24%	2.799%
23	10.911	1333	1340	1348	rBV2	111897	217206	19.66%	2.098%
24	11.104	1369	1373	1374	rBV2	1693	2482	0.22%	0.024%
25	11.334	1410	1412	1414	rBV2	1679	1513	0.14%	0.015%
26	11.510	1438	1442	1445	rBV	1837	2136	0.19%	0.021%
27	11.557	1449	1450	1454	rVB3	1820	1665	0.15%	0.016%
28	11.651	1464	1466	1469	rBV2	1419	1603	0.15%	0.015%
29	11.739	1477	1481	1484	rBV4	1421	1579	0.14%	0.015%
30	11.815	1492	1494	1499	rBV3	1591	2329	0.21%	0.022%
31	11.945	1515	1516	1522	rBV3	1811	2942	0.27%	0.028%
32	12.367	1584	1588	1594	rVB4	3046	4730	0.43%	0.046%
33	13.202	1726	1730	1735	rVB5	2357	3307	0.30%	0.032%
34	13.490	1777	1779	1783	rVB	2266	1569	0.14%	0.015%
35	13.701	1812	1815	1817	rBV	1548	1698	0.15%	0.016%
36	13.842	1837	1839	1841	rBV2	2360	1927	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050197.D
 Acq On : 8 Sep 2021 13:08
 Operator : CG/JU
 Sample : M3566-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

37	14.006	1861	1867	1879	rVB	422376	637660	57.73%	6.158%
38	14.095	1879	1882	1884	rVB2	1420	1506	0.14%	0.015%
39	14.124	1884	1887	1888	rBV2	1339	1463	0.13%	0.014%
40	14.306	1911	1918	1925	rVB	364026	600346	54.35%	5.798%
41	14.606	1963	1969	1977	rBV	281015	455131	41.21%	4.395%
42	14.870	2007	2014	2021	rBV3	20343	50424	4.57%	0.487%
43	15.346	2090	2095	2103	rBV	22254	34074	3.08%	0.329%
44	15.604	2132	2139	2146	rBV	543156	799156	72.35%	7.718%
45	15.657	2146	2148	2152	rVB3	3133	2926	0.26%	0.028%
46	15.739	2157	2162	2175	rBV	188631	305690	27.68%	2.952%
47	15.851	2175	2181	2184	rVB5	4585	7948	0.72%	0.077%
48	16.109	2224	2225	2231	rVB	1036	1547	0.14%	0.015%
49	16.174	2231	2236	2240	rBV2	1886	2654	0.24%	0.026%
50	16.362	2266	2268	2269	rBV	1787	1655	0.15%	0.016%
51	16.497	2286	2291	2292	rVB2	1451	1643	0.15%	0.016%
52	16.867	2350	2354	2362	rBV3	889	2136	0.19%	0.021%
53	17.002	2373	2377	2380	rVB2	951	1496	0.14%	0.014%
54	17.032	2380	2382	2387	rBV	1139	1884	0.17%	0.018%
55	17.155	2398	2403	2405	rBV2	1713	2497	0.23%	0.024%
56	17.361	2431	2438	2449	rBV	332271	496683	44.97%	4.797%
57	17.461	2449	2455	2465	rVB	615104	927897	84.01%	8.961%
58	17.942	2535	2537	2541	rBV	1019	1481	0.13%	0.014%
59	18.007	2546	2548	2550	rBV	2847	2154	0.20%	0.021%
60	18.318	2598	2601	2605	rVB2	2525	3495	0.32%	0.034%
61	18.530	2634	2637	2638	rBV2	2307	1556	0.14%	0.015%
62	18.647	2651	2657	2659	rBV3	1618	2097	0.19%	0.020%
63	18.729	2669	2671	2674	rBV	1817	1932	0.17%	0.019%
64	19.223	2753	2755	2756	rBV2	1979	1714	0.16%	0.017%
65	19.241	2756	2758	2761	rVB2	2093	1999	0.18%	0.019%
66	19.317	2768	2771	2777	rVB4	8145	11376	1.03%	0.110%
67	19.364	2777	2779	2780	rBV	2553	1735	0.16%	0.017%
68	19.387	2780	2783	2789	rVB3	8057	11796	1.07%	0.114%
69	19.640	2819	2826	2827	rBV3	1708	3104	0.28%	0.030%
70	19.752	2839	2845	2852	rBV	748330	1104545	100.00%	10.667%
71	20.086	2898	2902	2903	rBV3	2503	2094	0.19%	0.020%
72	20.263	2930	2932	2936	rVB4	1869	1715	0.16%	0.017%
73	20.498	2970	2972	2974	rBV3	3133	2364	0.21%	0.023%
74	20.556	2980	2982	2986	rBV4	3005	4190	0.38%	0.040%
75	20.650	2996	2998	3000	rBV2	2061	1509	0.14%	0.015%
76	20.762	3013	3017	3018	rBV4	3822	4354	0.39%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050197.D
 Acq On : 8 Sep 2021 13:08
 Operator : CG/JU
 Sample : M3566-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKH0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

77	20.868	3034	3035	3036	rBV	3184	1944	0.18%	0.019%
78	21.273	3099	3104	3108	rBV8	11648	25948	2.35%	0.251%
79	21.573	3154	3155	3157	rBV2	3665	1683	0.15%	0.016%
80	21.631	3159	3165	3173	rVV	326837	550160	49.81%	5.313%
81	22.401	3294	3296	3297	rBV2	4029	3107	0.28%	0.030%
82	22.859	3372	3374	3375	rBV2	3809	2149	0.19%	0.021%
83	23.870	3544	3546	3547	rBV2	6403	5020	0.45%	0.048%
84	24.627	3664	3675	3686	rBV	398309	1090877	98.76%	10.535%
85	24.845	3703	3712	3725	rVB2	198657	574558	52.02%	5.549%
86	25.902	3890	3892	3893	rBV2	4164	3322	0.30%	0.032%
87	26.307	3959	3961	3962	rBV2	3758	3107	0.28%	0.030%
88	26.789	4041	4043	4046	rBV3	4298	2951	0.27%	0.028%
89	28.205	4282	4284	4285	rBV2	3481	3028	0.27%	0.029%
90	28.775	4379	4381	4384	rBV3	3841	3135	0.28%	0.030%
91	29.720	4540	4542	4544	rBV3	5980	4370	0.40%	0.042%
92	29.762	4548	4549	4551	rBV2	6243	5033	0.46%	0.049%
93	29.844	4560	4563	4565	rBV3	6073	6563	0.59%	0.063%
94	29.961	4581	4583	4585	rBV3	6744	6475	0.59%	0.063%
95	30.261	4631	4634	4635	rBV3	4750	3934	0.36%	0.038%
96	30.455	4665	4667	4670	rBV3	9459	13161	1.19%	0.127%
97	31.060	4768	4770	4774	rBV4	4529	3894	0.35%	0.038%
98	31.589	4858	4860	4862	rBV3	4459	4106	0.37%	0.040%




Sum of corrected areas: 10354664

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050197.D
Acq On : 8 Sep 2021 13:08
Operator : CG/JU
Sample : M3566-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKH0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

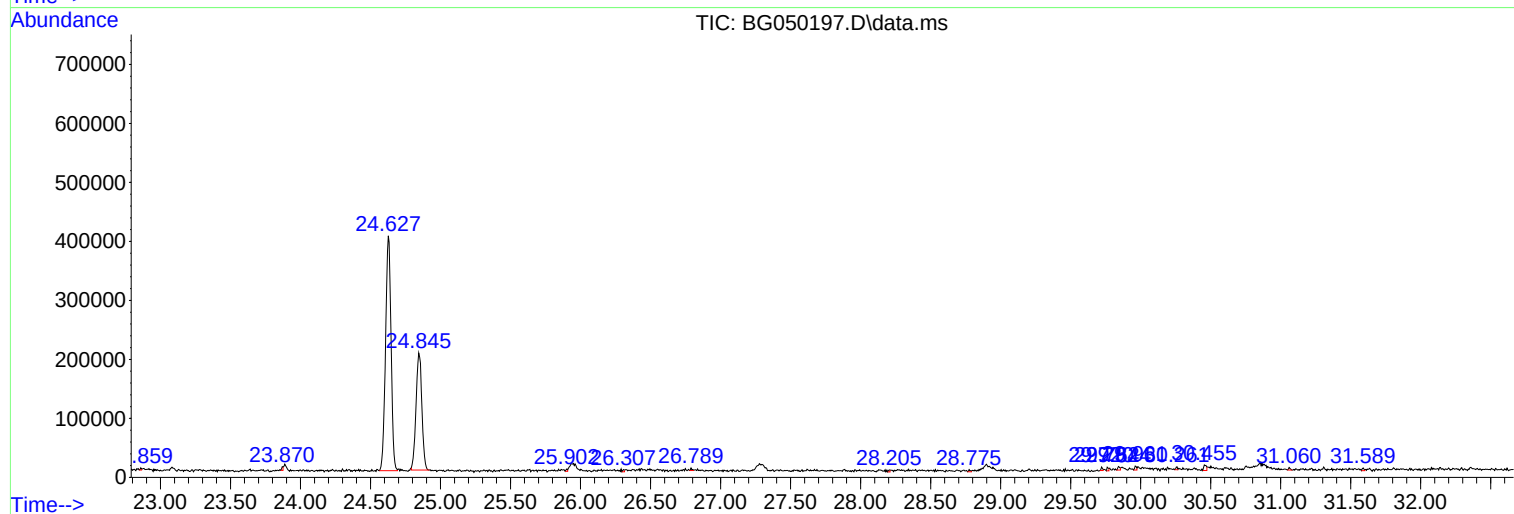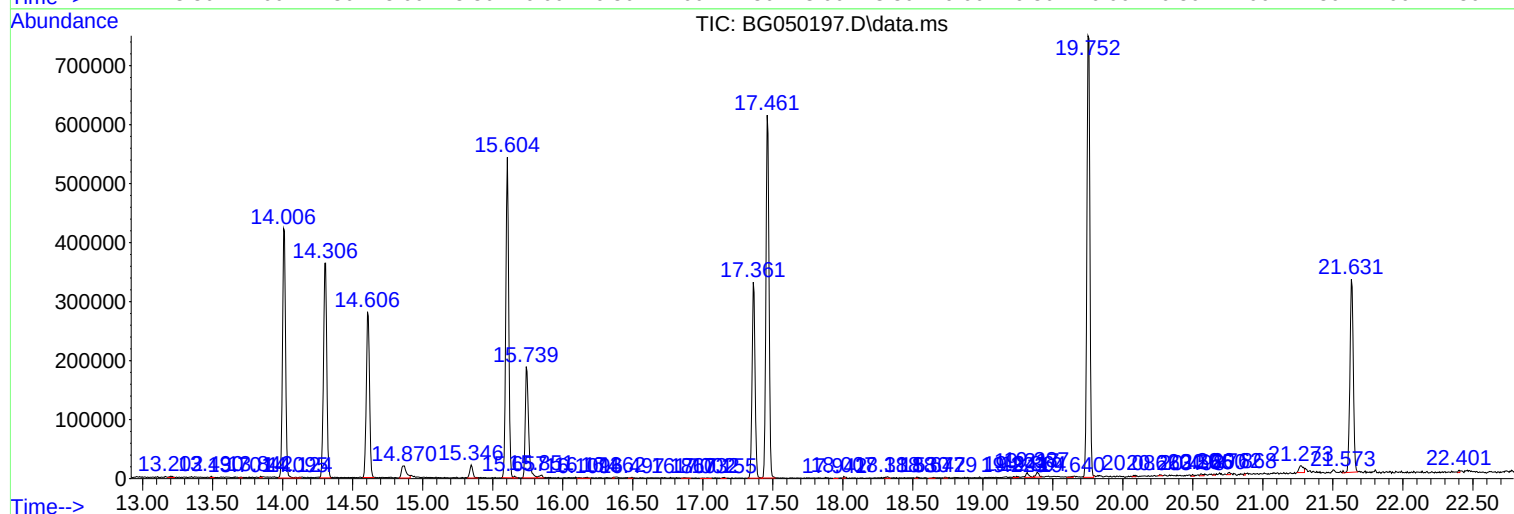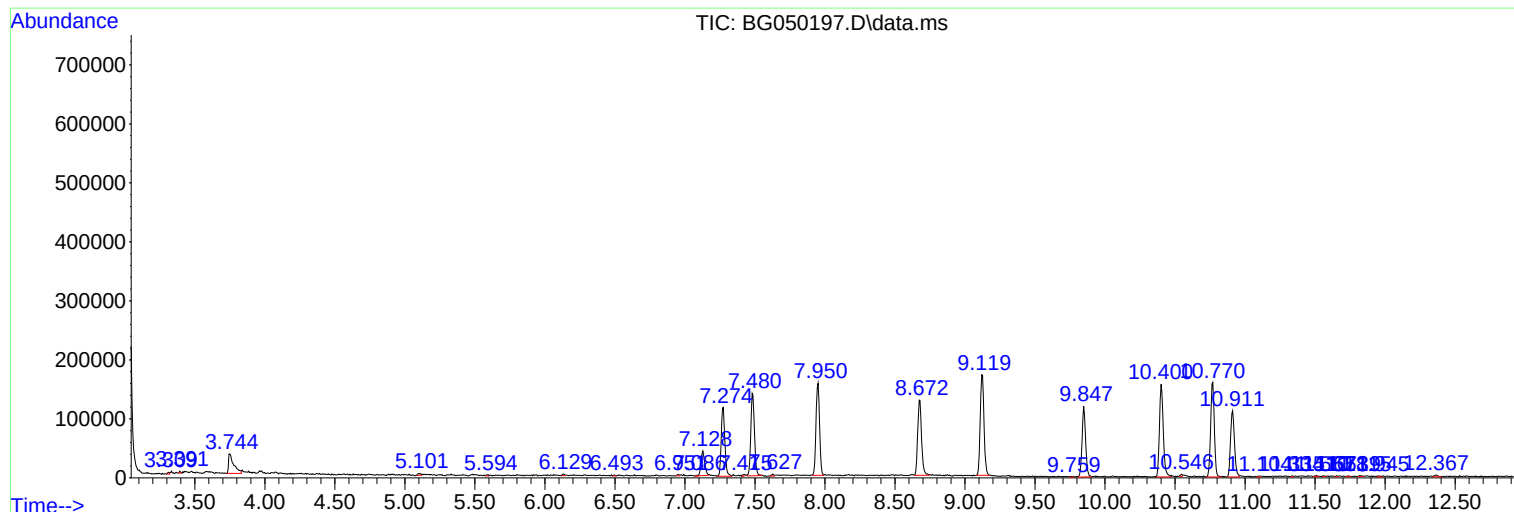

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050197.D
Acq On : 8 Sep 2021 13:08
Operator : CG/JU
Sample : M3566-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKH0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050197.D
Acq On : 8 Sep 2021 13:08
Operator : CG/JU
Sample : M3566-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKH0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
