

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050212.D
 Acq On : 9 Sep 2021 00:13
 Operator : CG/JU
 Sample : M3608-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.249	34	36	40	rVB4	2628	2016	0.17%	0.017%
2	3.314	43	47	52	rBV4	5538	7911	0.68%	0.066%
3	3.525	81	83	88	rVB2	2471	2545	0.22%	0.021%
4	3.749	118	121	130	rBV	30314	69109	5.93%	0.579%
5	3.890	144	145	150	rBV2	4344	5108	0.44%	0.043%
6	4.066	168	175	179	rBV5	7797	18965	1.63%	0.159%
7	4.753	289	292	293	rBV2	3109	2756	0.24%	0.023%
8	5.017	334	337	340	rVV2	2207	2173	0.19%	0.018%
9	5.047	340	342	345	rVB	2529	2319	0.20%	0.019%
10	5.123	351	355	357	rBV3	4497	6227	0.53%	0.052%
11	5.470	411	414	415	rBV	2515	2532	0.22%	0.021%
12	5.652	443	445	446	rBV	3387	3404	0.29%	0.029%
13	7.085	684	689	690	rBV	1103	1945	0.17%	0.016%
14	7.126	690	696	707	rVB	44188	80707	6.92%	0.676%
15	7.267	714	720	728	rBV	108960	188306	16.15%	1.578%
16	7.479	750	756	764	rBV	126227	229391	19.68%	1.922%
17	7.943	828	835	845	rVB	170546	302670	25.96%	2.536%
18	8.172	870	874	877	rBV2	2074	2932	0.25%	0.025%
19	8.213	879	881	887	rVB	1278	1739	0.15%	0.015%
20	8.301	894	896	900	rBV2	1668	1884	0.16%	0.016%
21	8.372	905	908	909	rBV2	3689	4381	0.38%	0.037%
22	8.671	953	959	972	rVB2	179993	326930	28.05%	2.739%
23	8.801	979	981	983	rBV2	1411	1637	0.14%	0.014%
24	8.871	990	993	994	rBV	1656	1786	0.15%	0.015%
25	8.936	1002	1004	1008	rVB	2093	1877	0.16%	0.016%
26	9.000	1013	1015	1019	rBV	1830	1840	0.16%	0.015%
27	9.118	1029	1035	1047	rBV	176458	329127	28.23%	2.758%
28	9.206	1047	1050	1051	rBV2	2300	2711	0.23%	0.023%
29	9.470	1092	1095	1098	rBV2	1500	1939	0.17%	0.016%
30	9.611	1116	1119	1121	rBV	1069	1614	0.14%	0.014%
31	9.846	1151	1159	1171	rBV	240090	449251	38.54%	3.764%
32	10.398	1246	1253	1265	rBV	305356	565266	48.49%	4.736%
33	10.763	1308	1315	1323	rBV	308137	576301	49.44%	4.829%
34	10.909	1333	1340	1350	rBV	196888	384194	32.96%	3.219%
35	11.115	1373	1375	1378	rBV	1757	1649	0.14%	0.014%
36	11.197	1387	1389	1392	rBV2	1859	1889	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050212.D
 Acq On : 9 Sep 2021 00:13
 Operator : CG/JU
 Sample : M3608-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

37	12.360	1583	1587	1593	rBV2	3403	6408	0.55%	0.054%
38	14.011	1861	1868	1876	rBV	374937	559482	48.00%	4.688%
39	14.299	1910	1917	1924	rBV	405372	637669	54.70%	5.343%
40	14.610	1963	1970	1980	rVB	325369	496910	42.63%	4.164%

41	14.863	2008	2013	2030	rBV3	20098	44995	3.86%	0.377%
42	15.603	2133	2139	2147	rBV	561697	821199	70.45%	6.881%
43	15.744	2157	2163	2176	rBV	153450	254386	21.82%	2.131%
44	15.844	2176	2180	2188	rVB5	3780	7392	0.63%	0.062%
45	17.154	2398	2403	2407	rBV2	1852	3002	0.26%	0.025%

46	17.266	2419	2422	2425	rBV2	1367	1912	0.16%	0.016%
47	17.365	2432	2439	2448	rBV	404993	620304	53.21%	5.197%
48	17.459	2448	2455	2463	rBV2	637704	967621	83.01%	8.108%
49	18.017	2547	2550	2555	rVB5	2204	2565	0.22%	0.021%
50	18.317	2597	2601	2606	rBV2	1613	3103	0.27%	0.026%

51	19.110	2732	2736	2737	rBV2	1978	2619	0.22%	0.022%
52	19.310	2766	2770	2776	rBV4	6981	10758	0.92%	0.090%
53	19.392	2780	2784	2790	rBV2	8423	12037	1.03%	0.101%
54	19.480	2796	2799	2800	rBV3	2300	2133	0.18%	0.018%
55	19.515	2803	2805	2810	rVB	1727	1960	0.17%	0.016%

56	19.609	2818	2821	2824	rVB3	1677	1705	0.15%	0.014%
57	19.639	2824	2826	2827	rBV	2561	2257	0.19%	0.019%
58	19.692	2833	2835	2839	rBV2	1865	1800	0.15%	0.015%
59	19.756	2839	2846	2858	rVV	800468	1165696	100.00%	9.767%
60	19.980	2880	2884	2889	rBV2	1608	3044	0.26%	0.026%

61	20.220	2923	2925	2928	rBV3	1340	1828	0.16%	0.015%
62	20.496	2970	2972	2973	rBV	2206	1681	0.14%	0.014%
63	20.702	3004	3007	3010	rBV3	4051	4455	0.38%	0.037%
64	20.761	3014	3017	3019	rBV3	2265	2461	0.21%	0.021%
65	20.937	3045	3047	3051	rVB3	4096	4436	0.38%	0.037%

66	20.978	3051	3054	3056	rBV3	2968	3205	0.27%	0.027%
67	21.272	3098	3104	3109	rBV8	11858	27310	2.34%	0.229%
68	21.501	3139	3143	3148	rVB	24140	32608	2.80%	0.273%
69	21.636	3159	3166	3174	rVB	405519	684730	58.74%	5.737%
70	21.924	3213	3215	3218	rBV3	2431	2451	0.21%	0.021%

71	22.071	3238	3240	3241	rVB2	3549	1760	0.15%	0.015%
72	22.112	3245	3247	3248	rBV2	2893	2490	0.21%	0.021%
73	23.886	3544	3549	3555	rVB7	10201	20773	1.78%	0.174%
74	23.933	3555	3557	3558	rBV2	2886	1588	0.14%	0.013%
75	24.626	3664	3675	3688	rBV2	433026	1148567	98.53%	9.624%

76	24.849	3702	3713	3726	rVB3	238761	722696	62.00%	6.055%
----	--------	------	------	------	------	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050212.D
 Acq On : 9 Sep 2021 00:13
 Operator : CG/JU
 Sample : M3608-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKK0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

77	25.942	3895	3899	3905	rVB5	11496	25396	2.18%	0.213%
78	26.559	4002	4004	4006	rVB3	3434	2337	0.20%	0.020%
79	28.445	4323	4325	4326	rBV2	3518	3223	0.28%	0.027%
80	28.562	4343	4345	4346	rBV2	3003	1556	0.13%	0.013%
81	28.973	4413	4415	4417	rBV3	3551	3948	0.34%	0.033%
82	29.226	4456	4458	4460	rBV2	2861	1865	0.16%	0.016%
83	29.614	4522	4524	4526	rBV3	3159	2495	0.21%	0.021%
84	31.628	4865	4867	4871	rBV5	3575	5198	0.45%	0.044%
85	32.380	4993	4995	4997	rBV3	3332	2098	0.18%	0.018%
86	32.521	5017	5019	5023	rBV5	3315	3777	0.32%	0.032%
87	32.551	5023	5024	5027	rVV2	3271	1840	0.16%	0.015%




Sum of corrected areas: 11934760

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050212.D
Acq On : 9 Sep 2021 00:13
Operator : CG/JU
Sample : M3608-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKK0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

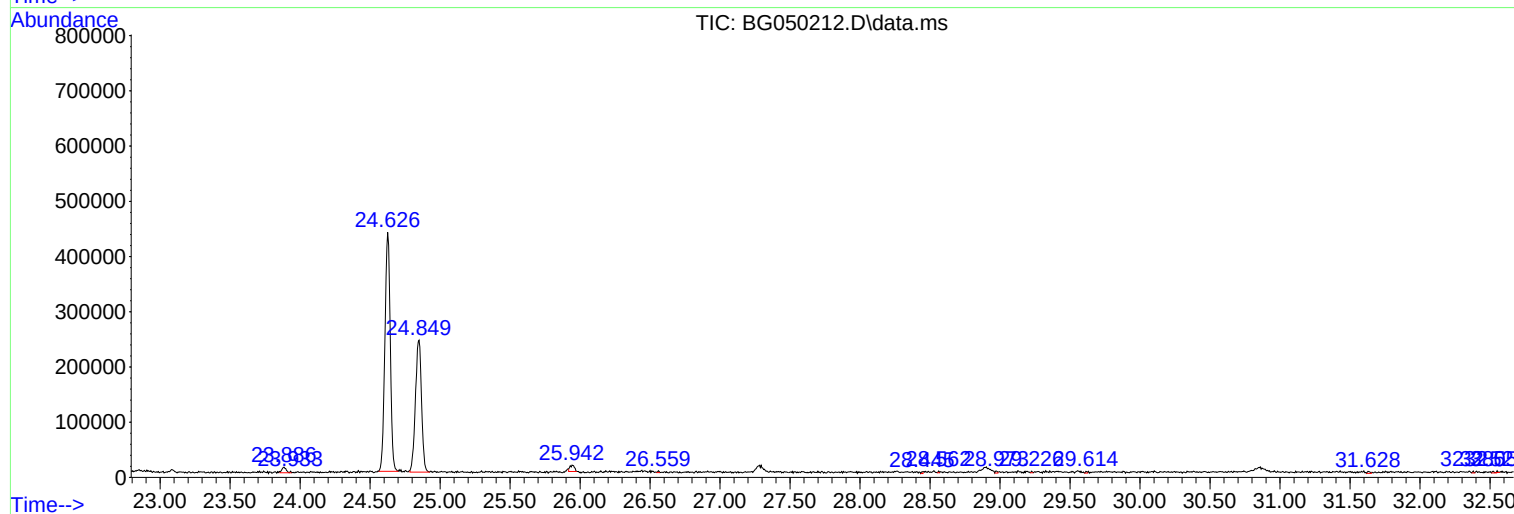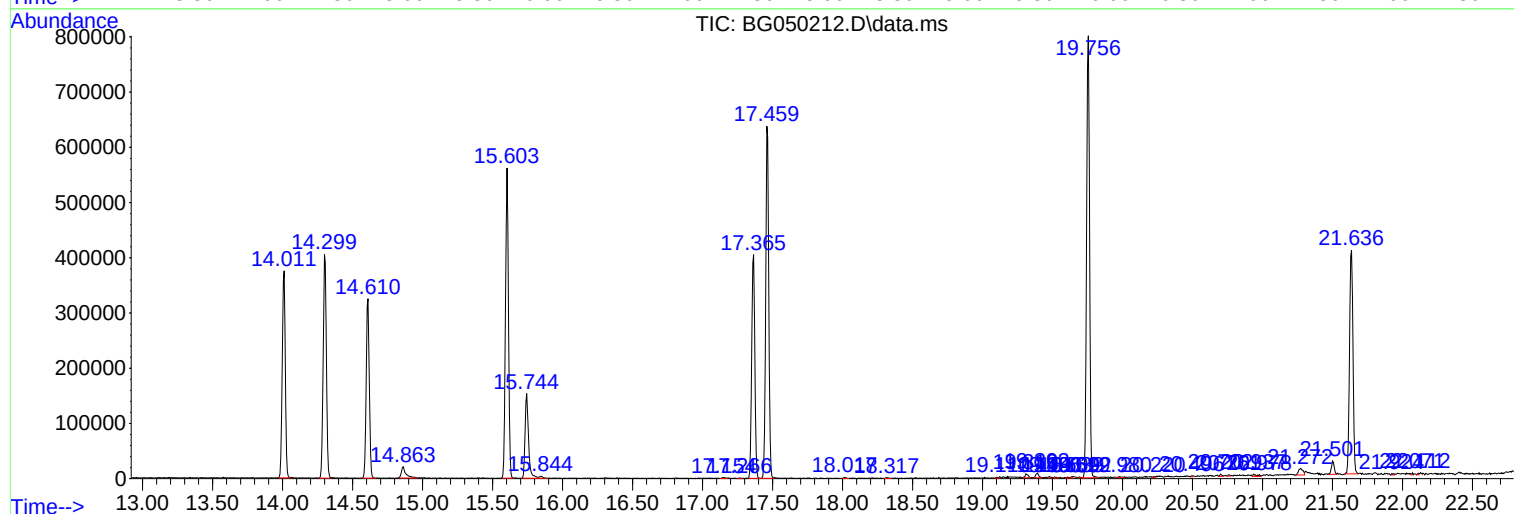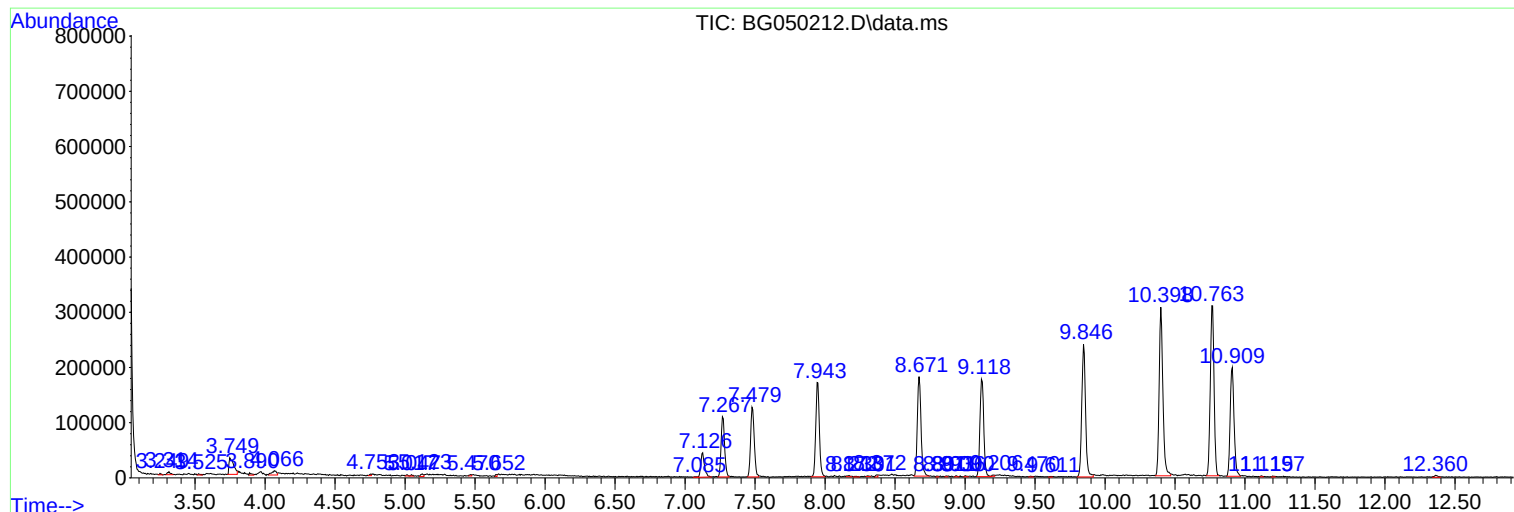

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050212.D
Acq On : 9 Sep 2021 00:13
Operator : CG/JU
Sample : M3608-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKK0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050212.D
Acq On : 9 Sep 2021 00:13
Operator : CG/JU
Sample : M3608-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKK0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
