

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050223.D
 Acq On : 9 Sep 2021 8:30
 Operator : CG/JU
 Sample : M3608-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.304	41	45	47	rBV3	4400	5501	0.43%	0.051%
2	3.474	72	74	75	rBV	2687	1828	0.14%	0.017%
3	3.745	117	120	134	rBV	34738	78052	6.07%	0.720%
4	4.068	172	175	178	rBV3	3631	3915	0.30%	0.036%
5	4.197	195	197	199	rBV2	1996	1933	0.15%	0.018%
6	4.438	236	238	240	rBV2	3078	2732	0.21%	0.025%
7	4.843	305	307	308	rBV2	2076	2065	0.16%	0.019%
8	5.037	336	340	342	rBV3	4256	5704	0.44%	0.053%
9	5.501	418	419	423	rBV2	2169	2478	0.19%	0.023%
10	5.566	428	430	435	rBV2	2389	2705	0.21%	0.025%
11	5.642	440	443	444	rBV2	2111	2077	0.16%	0.019%
12	5.842	475	477	482	rVB3	2203	2450	0.19%	0.023%
13	5.883	482	484	485	rBV	3119	2073	0.16%	0.019%
14	7.122	690	695	704	rBV	37000	70983	5.52%	0.655%
15	7.269	712	720	730	rBV	102766	175959	13.68%	1.624%
16	7.481	749	756	766	rBV	117512	208235	16.19%	1.922%
17	7.945	829	835	843	rVB	130112	224843	17.49%	2.075%
18	8.033	847	850	851	rBV	1846	1718	0.13%	0.016%
19	8.673	952	959	969	rBV	174517	315225	24.52%	2.909%
20	9.120	1028	1035	1044	rBV	185180	336053	26.14%	3.101%
21	9.255	1054	1058	1062	rVB3	2142	3678	0.29%	0.034%
22	9.372	1075	1078	1081	rBV3	2453	3772	0.29%	0.035%
23	9.566	1109	1111	1113	rBV	1955	2024	0.16%	0.019%
24	9.701	1131	1134	1135	rBV2	2229	2233	0.17%	0.021%
25	9.848	1152	1159	1171	rBV	196846	350854	27.29%	3.238%
26	10.400	1246	1253	1263	rBV	165737	322941	25.12%	2.980%
27	10.535	1273	1276	1281	rBV5	4611	8463	0.66%	0.078%
28	10.765	1307	1315	1322	rBV	185481	329513	25.63%	3.041%
29	10.906	1331	1339	1352	rBV	136042	265646	20.66%	2.452%
30	11.217	1389	1392	1396	rVB2	1282	1727	0.13%	0.016%
31	12.362	1583	1587	1592	rVB5	2811	4993	0.39%	0.046%
32	12.439	1596	1600	1603	rVB2	3026	4428	0.34%	0.041%
33	12.879	1672	1675	1680	rBV2	917	1783	0.14%	0.016%
34	14.007	1860	1867	1874	rBV	349056	511033	39.74%	4.716%
35	14.301	1910	1917	1927	rVB	376228	585059	45.50%	5.399%
36	14.606	1962	1969	1978	rBV	288667	453994	35.31%	4.190%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050223.D
 Acq On : 9 Sep 2021 8:30
 Operator : CG/JU
 Sample : M3608-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKL4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

37	14.683	1978	1982	1985	rBV2	1226	1575	0.12%	0.015%
38	14.859	2008	2012	2020	rBV3	17409	38586	3.00%	0.356%
39	15.605	2132	2139	2146	rBV	503515	770847	59.95%	7.114%
40	15.740	2157	2162	2172	rBV	141378	236111	18.36%	2.179%
41	15.846	2177	2180	2183	rVB	3999	5865	0.46%	0.054%
42	16.386	2270	2272	2277	rVB2	1613	2042	0.16%	0.019%
43	17.033	2376	2382	2385	rBV	1153	1546	0.12%	0.014%
44	17.091	2389	2392	2395	rBV2	1529	1850	0.14%	0.017%
45	17.156	2398	2403	2405	rBV2	2190	2911	0.23%	0.027%
46	17.362	2428	2438	2445	rBV	366379	565275	43.96%	5.217%
47	17.461	2449	2455	2464	rVB	632212	939472	73.06%	8.670%
48	17.714	2495	2498	2500	rBV2	1543	1787	0.14%	0.016%
49	17.890	2525	2528	2530	rBV2	1829	2099	0.16%	0.019%
50	17.949	2536	2538	2545	rVB3	1800	2922	0.23%	0.027%
51	18.014	2545	2549	2556	rBV5	3964	7559	0.59%	0.070%
52	18.284	2592	2595	2596	rBV5	1780	1669	0.13%	0.015%
53	18.824	2684	2687	2690	rBV3	1586	2534	0.20%	0.023%
54	19.047	2723	2725	2731	rVB	952	1592	0.12%	0.015%
55	19.318	2767	2771	2775	rVB5	7024	10728	0.83%	0.099%
56	19.347	2775	2776	2779	rBV	1426	1618	0.13%	0.015%
57	19.394	2779	2784	2789	rVB2	8592	13973	1.09%	0.129%
58	19.641	2824	2826	2827	rBV	2983	2172	0.17%	0.020%
59	19.700	2833	2836	2838	rBV2	1903	1542	0.12%	0.014%
60	19.752	2839	2845	2852	rVV	806707	1118944	87.02%	10.326%
61	20.111	2904	2906	2909	rBV3	1605	1843	0.14%	0.017%
62	20.152	2909	2913	2919	rVB8	1581	3658	0.28%	0.034%
63	20.217	2922	2924	2926	rBV2	1573	1572	0.12%	0.015%
64	20.322	2940	2942	2944	rBV3	1491	1574	0.12%	0.015%
65	20.346	2944	2946	2949	rVB3	2856	2160	0.17%	0.020%
66	20.522	2974	2976	2979	rBV3	2045	3088	0.24%	0.028%
67	20.698	3003	3006	3011	rVB6	3407	5510	0.43%	0.051%
68	20.933	3044	3046	3050	rBV4	2239	2802	0.22%	0.026%
69	21.268	3099	3103	3104	rBV3	8802	11410	0.89%	0.105%
70	21.632	3159	3165	3177	rVB	406535	641896	49.92%	5.924%
71	21.867	3203	3205	3206	rBV2	2678	1557	0.12%	0.014%
72	21.897	3208	3210	3211	rBV2	2939	2405	0.19%	0.022%
73	22.267	3271	3273	3276	rVB2	3423	2632	0.20%	0.024%
74	22.760	3355	3357	3358	rBV2	4046	2664	0.21%	0.025%
75	22.807	3361	3365	3367	rBV5	6122	8863	0.69%	0.082%
76	22.919	3382	3384	3385	rBV2	5750	2700	0.21%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050223.D
 Acq On : 9 Sep 2021 8:30
 Operator : CG/JU
 Sample : M3608-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKL4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

77	22.995	3396	3397	3398	rBV	5754	3527	0.27%	0.033%
78	23.271	3442	3444	3450	rVB5	9320	14772	1.15%	0.136%
79	23.353	3456	3458	3461	rBV3	8476	12324	0.96%	0.114%
80	23.624	3503	3504	3505	rBV	4558	2800	0.22%	0.026%
81	23.706	3516	3518	3519	rBV	6534	4170	0.32%	0.038%
82	23.882	3542	3548	3550	rBV6	11306	24218	1.88%	0.223%
83	24.076	3579	3581	3583	rBV3	5136	5320	0.41%	0.049%
84	24.176	3595	3598	3601	rBV5	9727	15568	1.21%	0.144%
85	24.628	3665	3675	3688	rVB	478091	1285810	100.00%	11.866%
86	24.734	3691	3693	3697	rBV4	7308	8373	0.65%	0.077%
87	24.846	3702	3712	3727	rVB	244228	704993	54.83%	6.506%
88	26.549	4000	4002	4008	rBV7	3009	4256	0.33%	0.039%
89	28.323	4303	4304	4306	rBV2	2867	1884	0.15%	0.017%
90	28.464	4326	4328	4329	rVB2	3309	1617	0.13%	0.015%
91	28.781	4380	4382	4383	rBV2	2690	2537	0.20%	0.023%
92	29.269	4463	4465	4466	rBV2	3340	1841	0.14%	0.017%
93	29.992	4586	4588	4590	rBV2	3312	2690	0.21%	0.025%
94	31.014	4760	4762	4763	rBV2	2691	1752	0.14%	0.016%
95	31.695	4876	4878	4880	rBV3	3297	2915	0.23%	0.027%
96	32.283	4976	4978	4979	rVB2	3920	2107	0.16%	0.019%
97	32.600	5031	5032	5035	rBV2	3945	2244	0.17%	0.021%




Sum of corrected areas: 10835941

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050223.D
Acq On : 9 Sep 2021 8:30
Operator : CG/JU
Sample : M3608-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKL4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

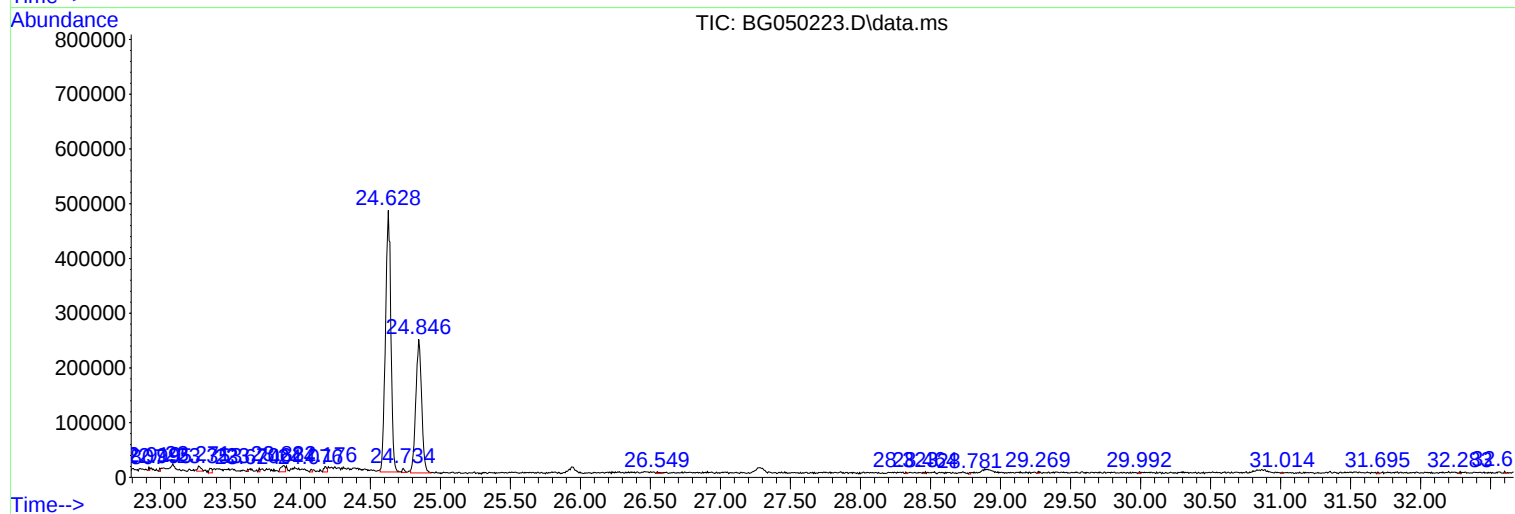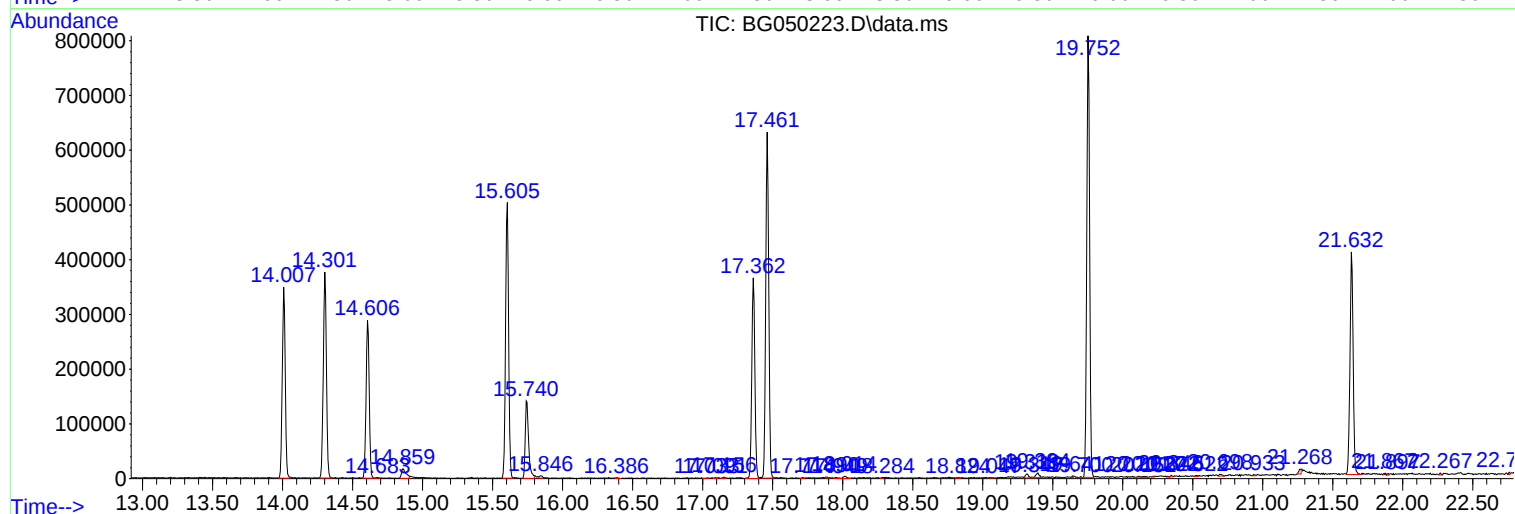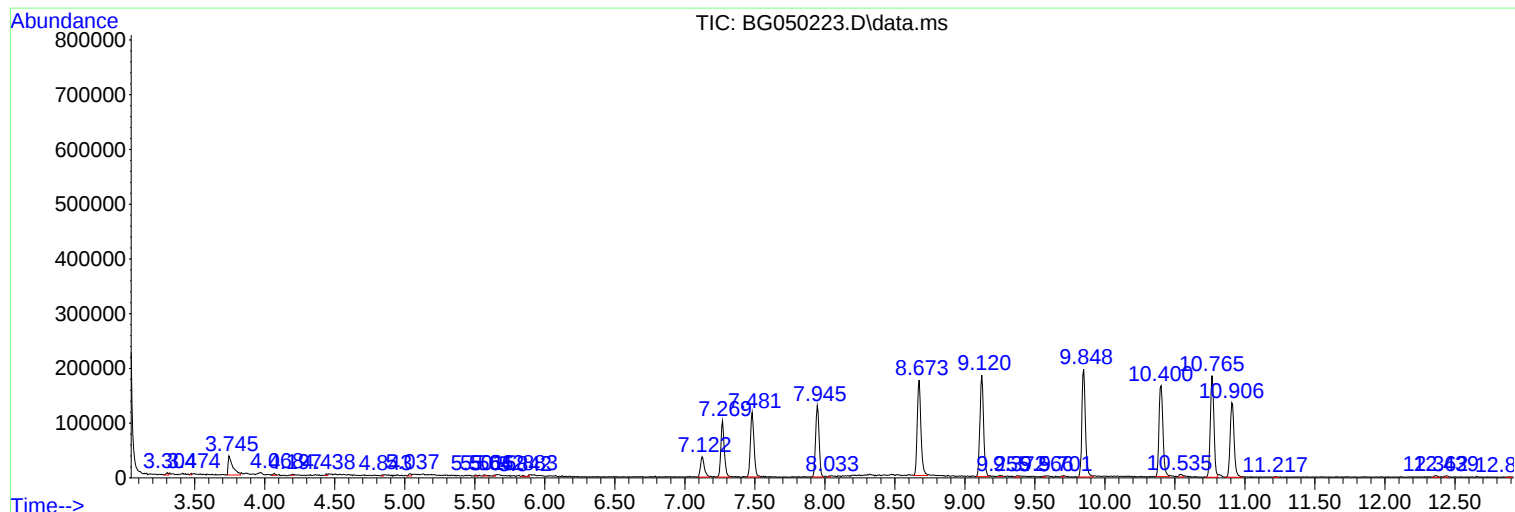

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050223.D
Acq On : 9 Sep 2021 8:30
Operator : CG/JU
Sample : M3608-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKL4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050223.D
Acq On : 9 Sep 2021 8:30
Operator : CG/JU
Sample : M3608-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKL4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
