

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050232.D
 Acq On : 9 Sep 2021 16:37
 Operator : CG/JU
 Sample : PB138900BL
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK900

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.313	42	47	50	rBV3	12113	21865	1.72%	0.153%
2	3.736	115	119	138	rBV	178145	340731	26.73%	2.392%
3	3.989	159	162	163	rBV2	4968	5334	0.42%	0.037%
4	4.981	330	331	333	rBV2	2559	2204	0.17%	0.015%
5	5.199	365	368	372	rBV5	3400	7269	0.57%	0.051%
6	6.444	578	580	587	rBV3	2601	5948	0.47%	0.042%
7	6.585	601	604	607	rBV2	2627	3526	0.28%	0.025%
8	6.614	607	609	611	rVB2	2411	1809	0.14%	0.013%
9	6.679	618	620	624	rBV3	3397	5403	0.42%	0.038%
10	6.867	650	652	653	rBV2	2447	1899	0.15%	0.013%
11	6.926	659	662	663	rBV	2644	2475	0.19%	0.017%
12	7.008	674	676	679	rBV2	2258	2582	0.20%	0.018%
13	7.067	683	686	689	rBV3	3957	6890	0.54%	0.048%
14	7.120	689	695	708	rVV	272571	499600	39.20%	3.507%
15	7.272	714	721	730	rVB	162311	278868	21.88%	1.958%
16	7.343	730	733	739	rVB2	2564	4117	0.32%	0.029%
17	7.437	746	749	750	rBV2	2415	2290	0.18%	0.016%
18	7.478	750	756	767	rVB	182716	324644	25.47%	2.279%
19	7.948	828	836	845	rVB	131012	231809	18.19%	1.627%
20	8.665	953	958	973	rBV	218743	397916	31.22%	2.793%
21	9.117	1029	1035	1047	rVB	156702	286363	22.47%	2.010%
22	9.569	1108	1112	1113	rBV	4190	3954	0.31%	0.028%
23	9.845	1152	1159	1171	rBV	185187	334067	26.21%	2.345%
24	9.928	1171	1173	1175	rBV	1692	1799	0.14%	0.013%
25	10.139	1205	1209	1212	rBV3	2764	4703	0.37%	0.033%
26	10.397	1247	1253	1268	rVB	282189	506671	39.75%	3.557%
27	10.585	1284	1285	1287	rBV	1974	1612	0.13%	0.011%
28	10.685	1298	1302	1303	rBV	3806	3464	0.27%	0.024%
29	10.768	1307	1316	1324	rVB	285017	535495	42.01%	3.759%
30	10.903	1333	1339	1353	rVB	196373	395863	31.06%	2.779%
31	11.026	1358	1360	1363	rVB	1714	1757	0.14%	0.012%
32	12.371	1585	1589	1593	rVB3	2136	3225	0.25%	0.023%
33	13.200	1727	1730	1734	rBV2	2197	2395	0.19%	0.017%
34	13.276	1741	1743	1747	rVB	2176	2527	0.20%	0.018%
35	13.393	1760	1763	1764	rBV	2274	2375	0.19%	0.017%
36	13.487	1777	1779	1782	rBV3	1571	1867	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050232.D
 Acq On : 9 Sep 2021 16:37
 Operator : CG/JU
 Sample : PB138900BL
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK900

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

37	14.010	1861	1868	1875	rBV	660301	979631	76.86%	6.877%
38	14.304	1910	1918	1926	rBV	701560	1141561	89.56%	8.014%
39	14.609	1961	1970	1980	rBV	516947	811177	63.64%	5.694%
40	14.844	2004	2010	2027	rBV2	151864	347913	27.30%	2.442%
41	15.226	2072	2075	2077	rBV3	1800	1810	0.14%	0.013%
42	15.602	2131	2139	2147	rBV	826891	1274621	100.00%	8.948%
43	15.743	2157	2163	2177	rBV	224692	380926	29.89%	2.674%
44	15.843	2178	2180	2185	rVB4	7256	9216	0.72%	0.065%
45	16.289	2254	2256	2261	rVB2	1061	1695	0.13%	0.012%
46	17.241	2414	2418	2423	rVB	1007	1938	0.15%	0.014%
47	17.359	2432	2438	2447	rVB	367390	565014	44.33%	3.966%
48	17.459	2449	2455	2465	rVB2	571061	870431	68.29%	6.110%
49	17.911	2529	2532	2536	rBV2	1091	1632	0.13%	0.011%
50	19.227	2753	2756	2757	rBV	2019	2305	0.18%	0.016%
51	19.315	2767	2771	2775	rVB3	5413	7336	0.58%	0.051%
52	19.391	2780	2784	2788	rBV3	8014	11038	0.87%	0.077%
53	19.538	2808	2809	2815	rVB5	3045	3354	0.26%	0.024%
54	19.644	2823	2827	2830	rBV3	2856	3621	0.28%	0.025%
55	19.755	2839	2846	2854	rBV	739942	1065406	83.59%	7.479%
56	20.026	2890	2892	2895	rBV2	1727	2229	0.17%	0.016%
57	20.055	2895	2897	2902	rVB2	2184	3341	0.26%	0.023%
58	20.695	3004	3006	3009	rVB3	3168	2635	0.21%	0.018%
59	21.629	3159	3165	3176	rVB	407537	668409	52.44%	4.692%
60	22.475	3306	3309	3310	rBV3	4767	4614	0.36%	0.032%
61	23.074	3409	3411	3413	rBV3	5134	5069	0.40%	0.036%
62	23.374	3460	3462	3463	rBV2	3743	2416	0.19%	0.017%
63	23.879	3543	3548	3554	rBV7	12764	25536	2.00%	0.179%
64	24.625	3665	3675	3686	rVB	399308	1063250	83.42%	7.464%
65	24.843	3702	3712	3723	rVB2	228503	678736	53.25%	4.765%
66	25.941	3889	3899	3906	rBV4	17727	59301	4.65%	0.416%
67	26.523	3996	3998	4000	rBV2	6869	7021	0.55%	0.049%
68	26.928	4065	4067	4068	rBV2	4075	2679	0.21%	0.019%
69	31.422	4830	4832	4833	rBV2	3280	2201	0.17%	0.015%
70	32.321	4983	4985	4986	rBV	3262	1874	0.15%	0.013%


Sum of corrected areas: 14245252

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050232.D
Acq On : 9 Sep 2021 16:37
Operator : CG/JU
Sample : PB138900BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK900

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

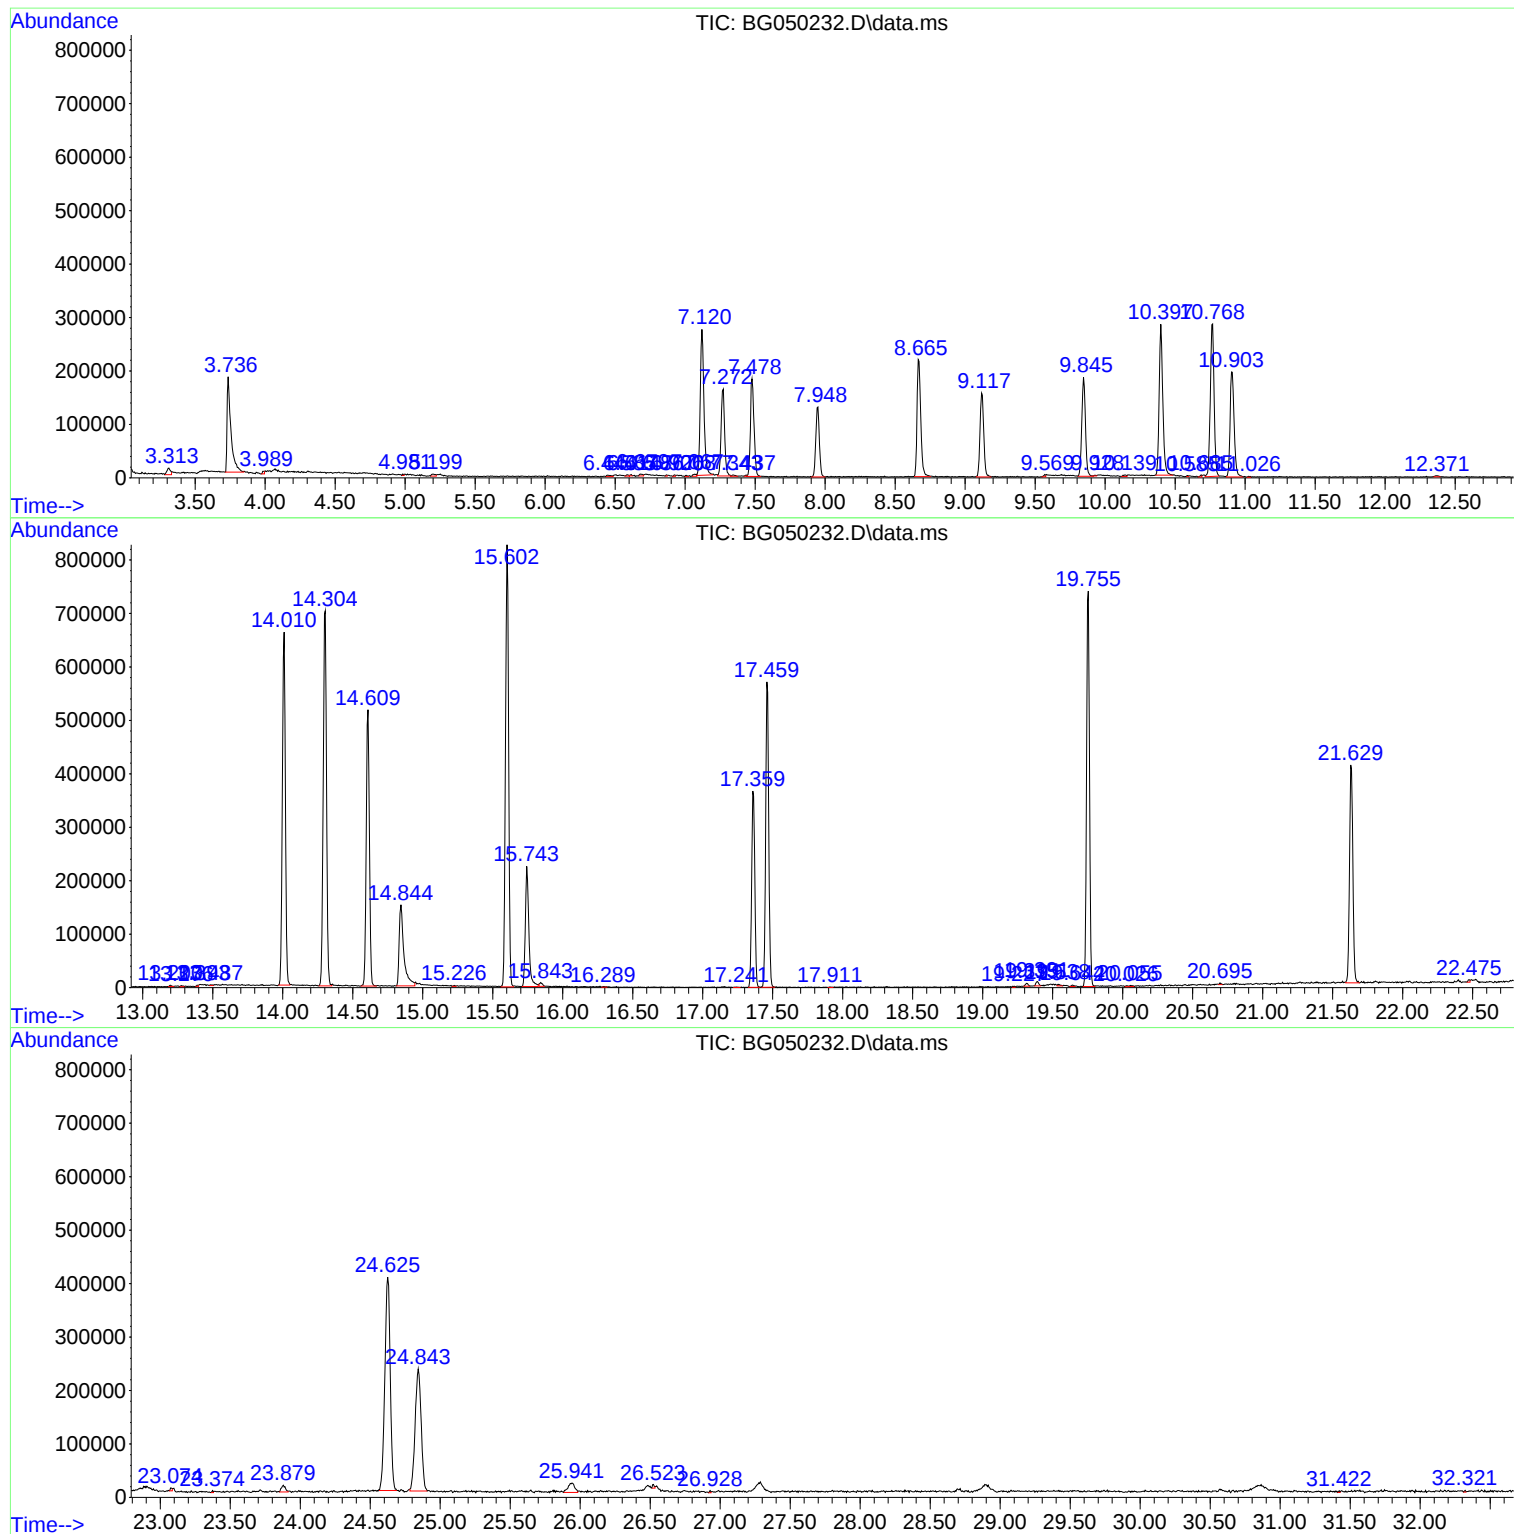

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050232.D
Acq On : 9 Sep 2021 16:37
Operator : CG/JU
Sample : PB138900BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK900

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050232.D
Acq On : 9 Sep 2021 16:37
Operator : CG/JU
Sample : PB138900BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK900

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
