

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050233.D
 Acq On : 9 Sep 2021 17:19
 Operator : CG/JU
 Sample : PB138901BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.307	42	46	50	rBV3	8643	13865	1.24%	0.113%
2	3.736	115	119	140	rBV	151309	353793	31.66%	2.887%
3	4.071	172	176	180	rBV5	8844	17067	1.53%	0.139%
4	4.347	221	223	228	rVB4	2476	3433	0.31%	0.028%
5	4.435	236	238	240	rBV2	3637	3658	0.33%	0.030%
6	4.494	246	248	250	rVB	4058	2161	0.19%	0.018%
7	4.541	253	256	258	rBV2	5219	6408	0.57%	0.052%
8	4.723	286	287	290	rVB2	2723	2548	0.23%	0.021%
9	4.746	290	291	294	rVV2	3881	3670	0.33%	0.030%
10	4.781	296	297	300	rVB2	3588	2660	0.24%	0.022%
11	4.864	310	311	318	rBV3	4991	6869	0.61%	0.056%
12	6.115	522	524	528	rBV4	2409	3404	0.30%	0.028%
13	6.174	531	534	538	rBV3	2674	5319	0.48%	0.043%
14	6.221	540	542	544	rBV2	4474	4635	0.41%	0.038%
15	6.550	595	598	599	rBV	2605	2035	0.18%	0.017%
16	6.661	613	617	618	rBV	4584	4796	0.43%	0.039%
17	7.119	689	695	706	rVB	230140	403085	36.07%	3.289%
18	7.208	709	710	713	rBV3	2302	1618	0.14%	0.013%
19	7.266	715	720	730	rVB	117920	202915	18.16%	1.656%
20	7.478	750	756	766	rVB2	160913	284151	25.42%	2.319%
21	7.948	829	836	847	rVB	139191	238125	21.31%	1.943%
22	8.059	852	855	860	rVB4	1095	1816	0.16%	0.015%
23	8.670	952	959	970	rBV	196641	353263	31.61%	2.882%
24	9.117	1028	1035	1045	rBV	166315	290842	26.02%	2.373%
25	9.845	1152	1159	1172	rBV2	147515	261677	23.41%	2.135%
26	10.033	1187	1191	1193	rBV3	2570	4193	0.38%	0.034%
27	10.127	1205	1207	1210	rBV2	1420	1886	0.17%	0.015%
28	10.209	1217	1221	1222	rBV2	2974	3348	0.30%	0.027%
29	10.397	1246	1253	1263	rBV	302559	574236	51.38%	4.685%
30	10.621	1288	1291	1295	rBV3	3041	4965	0.44%	0.041%
31	10.703	1303	1305	1308	rVB2	1661	1410	0.13%	0.012%
32	10.762	1308	1315	1323	rBV	307310	560865	50.18%	4.576%
33	10.903	1332	1339	1352	rBV	201459	406354	36.36%	3.316%
34	11.179	1382	1386	1387	rBV	1307	1530	0.14%	0.012%
35	11.983	1519	1523	1525	rVB3	1267	1540	0.14%	0.013%
36	12.371	1584	1589	1595	rVB6	3215	6036	0.54%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050233.D
 Acq On : 9 Sep 2021 17:19
 Operator : CG/JU
 Sample : PB138901BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

37	12.906	1678	1680	1685	rVB3	1217	1391	0.12%	0.011%
38	13.481	1775	1778	1781	rVB	979	1403	0.13%	0.011%
39	13.523	1781	1785	1789	rBV2	1289	2239	0.20%	0.018%
40	14.010	1861	1868	1878	rVB	403637	577376	51.66%	4.711%
41	14.304	1911	1918	1927	rVB	408579	652861	58.41%	5.327%
42	14.609	1963	1970	1977	rBV	289785	462260	41.36%	3.772%
43	14.844	2004	2010	2029	rBV	95868	210388	18.82%	1.717%
44	15.073	2046	2049	2052	rVB3	1181	1547	0.14%	0.013%
45	15.602	2132	2139	2147	rBV	535512	803422	71.89%	6.556%
46	15.743	2155	2163	2173	rBV2	145344	247184	22.12%	2.017%
47	17.153	2399	2403	2406	rBV	1570	2381	0.21%	0.019%
48	17.364	2431	2439	2446	rBV	389501	564366	50.50%	4.605%
49	17.458	2449	2455	2465	rBV	563764	868309	77.69%	7.085%
50	18.475	2624	2628	2631	rBV3	1468	2124	0.19%	0.017%
51	18.833	2686	2689	2693	rVB3	1300	1580	0.14%	0.013%
52	19.121	2736	2738	2741	rBV2	1532	1406	0.13%	0.011%
53	19.191	2749	2750	2753	rBV3	1351	1396	0.12%	0.011%
54	19.315	2768	2771	2776	rVB4	6250	9060	0.81%	0.074%
55	19.391	2779	2784	2789	rVV2	7082	11007	0.98%	0.090%
56	19.485	2797	2800	2803	rBV2	1560	2135	0.19%	0.017%
57	19.514	2803	2805	2810	rVB3	1937	1974	0.18%	0.016%
58	19.614	2817	2822	2823	rBV3	1535	2110	0.19%	0.017%
59	19.650	2823	2828	2830	rBV2	2928	4245	0.38%	0.035%
60	19.755	2839	2846	2856	rVB	727112	1077641	96.42%	8.793%
61	19.855	2861	2863	2865	rBV2	2422	1802	0.16%	0.015%
62	19.943	2875	2878	2881	rBV3	1550	2031	0.18%	0.017%
63	20.172	2915	2917	2919	rBV	2043	1983	0.18%	0.016%
64	20.266	2931	2933	2934	rBV2	2162	1394	0.12%	0.011%
65	20.390	2952	2954	2957	rBV3	1548	1468	0.13%	0.012%
66	20.454	2963	2965	2967	rBV3	2130	1533	0.14%	0.013%
67	20.631	2994	2995	2997	rBV2	2028	1609	0.14%	0.013%
68	20.695	3004	3006	3010	rVB5	3930	3777	0.34%	0.031%
69	20.877	3035	3037	3039	rBV3	2756	2817	0.25%	0.023%
70	21.206	3091	3093	3096	rBV2	2413	2832	0.25%	0.023%
71	21.635	3159	3166	3175	rBV	419605	680446	60.88%	5.552%
72	21.711	3178	3179	3181	rBV2	3401	2411	0.22%	0.020%
73	22.035	3232	3234	3236	rBV2	3039	3575	0.32%	0.029%
74	22.070	3239	3240	3242	rBV2	3784	1746	0.16%	0.014%
75	22.651	3337	3339	3340	rBV2	5186	2365	0.21%	0.019%
76	22.693	3342	3346	3347	rBV4	8441	11473	1.03%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050233.D
 Acq On : 9 Sep 2021 17:19
 Operator : CG/JU
 Sample : PB138901BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

77	23.027	3401	3403	3407	rBV5	6542	10121	0.91%	0.083%
78	23.086	3409	3413	3417	rBV4	21344	38203	3.42%	0.312%
79	23.462	3476	3477	3478	rBV	3883	2425	0.22%	0.020%
80	23.550	3491	3492	3494	rBV2	5370	4699	0.42%	0.038%
81	24.120	3585	3589	3591	rVB5	3719	4419	0.40%	0.036%
82	24.625	3665	3675	3686	rVB2	398036	1117630	100.00%	9.119%
83	24.843	3701	3712	3723	rBV2	239671	735517	65.81%	6.001%
84	25.324	3792	3794	3795	rVB2	4062	1586	0.14%	0.013%
85	26.335	3964	3966	3967	rBV2	3733	2271	0.20%	0.019%
86	27.280	4118	4127	4135	rBV9	18622	58723	5.25%	0.479%
87	27.615	4182	4184	4190	rVB6	3500	4222	0.38%	0.034%
88	30.364	4650	4652	4653	rBV2	3509	2559	0.23%	0.021%




Sum of corrected areas: 12255618

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050233.D
Acq On : 9 Sep 2021 17:19
Operator : CG/JU
Sample : PB138901BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

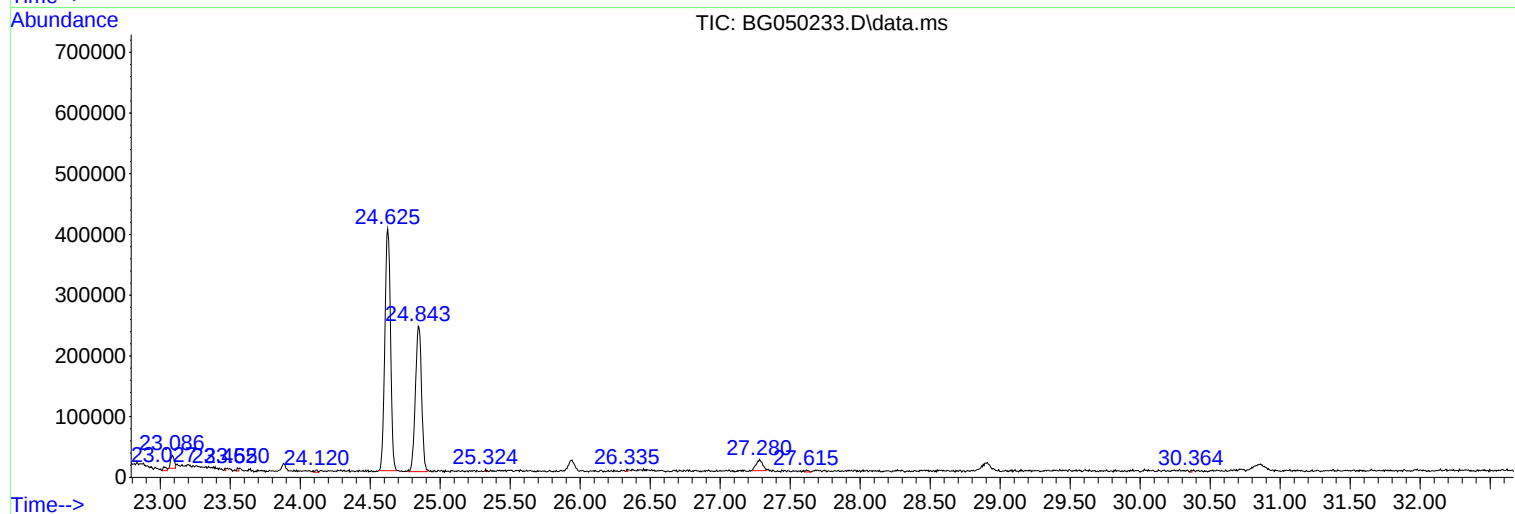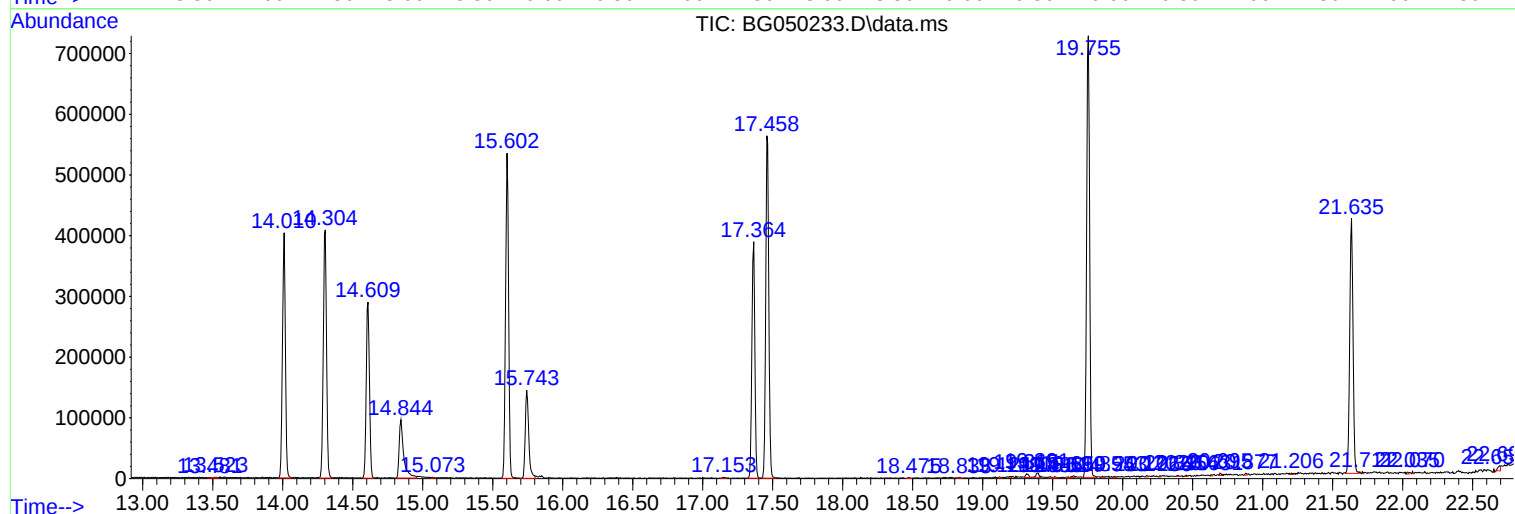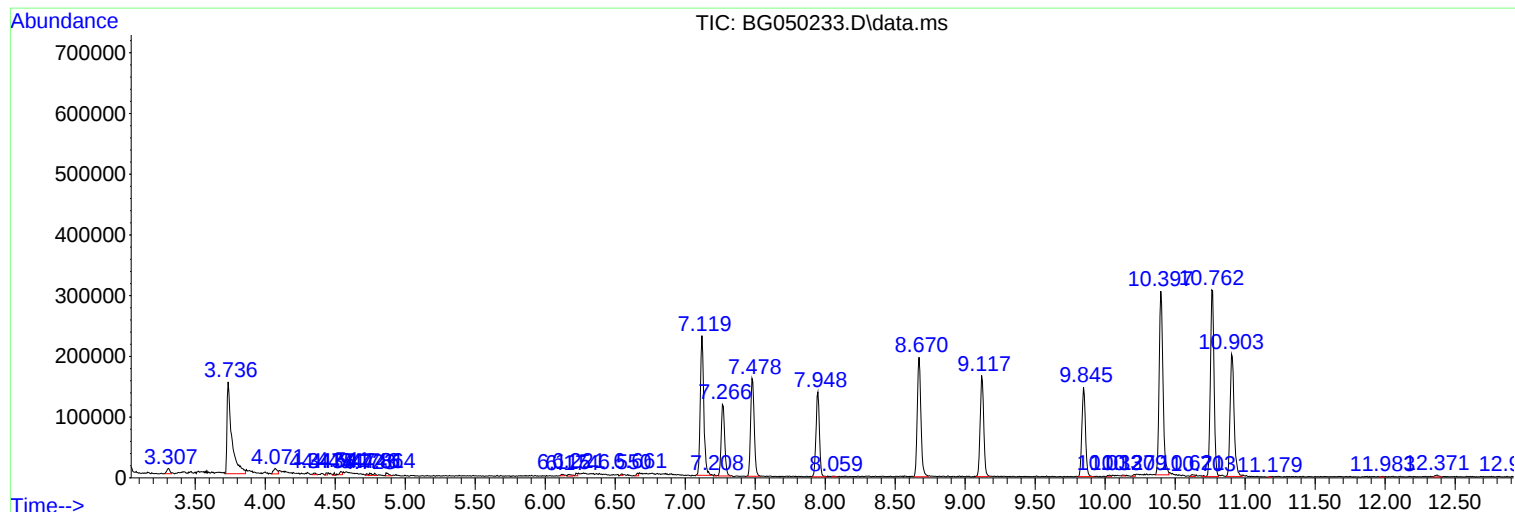

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050233.D
Acq On : 9 Sep 2021 17:19
Operator : CG/JU
Sample : PB138901BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050233.D
Acq On : 9 Sep 2021 17:19
Operator : CG/JU
Sample : PB138901BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------