

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050236.D
 Acq On : 9 Sep 2021 19:24
 Operator : CG/JU
 Sample : M3608-12
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.707	112	114	116	rBV3	2553	2632	0.22%	0.025%
2	3.748	118	121	126	rBV	29360	46570	3.87%	0.451%
3	3.860	135	140	141	rBV3	6403	7963	0.66%	0.077%
4	4.289	211	213	214	rBV2	3691	3269	0.27%	0.032%
5	4.441	237	239	240	rBV	3527	3098	0.26%	0.030%
6	4.653	270	275	277	rBV3	5154	8471	0.70%	0.082%
7	5.082	346	348	349	rBV2	2628	2072	0.17%	0.020%
8	5.252	375	377	382	rBV4	5159	10456	0.87%	0.101%
9	5.475	414	415	416	rBV	3907	2506	0.21%	0.024%
10	5.681	449	450	457	rVB2	3742	3573	0.30%	0.035%
11	5.769	464	465	469	rBV	3081	2837	0.24%	0.027%
12	7.126	690	696	704	rBV	55449	118625	9.87%	1.149%
13	7.267	714	720	731	rBV	185038	322524	26.83%	3.123%
14	7.478	750	756	767	rBV	168904	314508	26.16%	3.046%
15	7.942	829	835	845	rVB	183800	320116	26.63%	3.100%
16	8.600	945	947	953	rBV3	1707	2419	0.20%	0.023%
17	8.671	953	959	972	rVV	77352	139987	11.64%	1.356%
18	9.117	1026	1035	1043	rBV	116500	217842	18.12%	2.109%
19	9.599	1112	1117	1119	rBV2	1039	1677	0.14%	0.016%
20	9.846	1153	1159	1167	rBV2	104575	190106	15.81%	1.841%
21	10.075	1194	1198	1201	rBV2	2824	3436	0.29%	0.033%
22	10.210	1217	1221	1222	rBV2	2374	2699	0.22%	0.026%
23	10.333	1239	1242	1245	rBV	2058	3241	0.27%	0.031%
24	10.398	1247	1253	1266	rVV	157211	302613	25.17%	2.930%
25	10.486	1266	1268	1271	rVB2	3025	2640	0.22%	0.026%
26	10.557	1277	1280	1284	rVB4	1800	2202	0.18%	0.021%
27	10.762	1309	1315	1326	rBV	156604	280048	23.30%	2.712%
28	10.909	1333	1340	1350	rBV	120660	236477	19.67%	2.290%
29	11.966	1518	1520	1523	rBV2	1484	1727	0.14%	0.017%
30	12.360	1584	1587	1597	rVB4	2683	4961	0.41%	0.048%
31	13.094	1711	1712	1715	rBV2	2337	2842	0.24%	0.028%
32	13.188	1726	1728	1729	rBV	2634	2595	0.22%	0.025%
33	13.388	1759	1762	1764	rBV2	2588	2926	0.24%	0.028%
34	13.406	1764	1765	1767	rVV3	2485	1828	0.15%	0.018%
35	13.576	1793	1794	1800	rVB2	1657	1648	0.14%	0.016%
36	13.764	1823	1826	1828	rBV2	1507	1898	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
 Data File : BG050236.D
 Acq On : 9 Sep 2021 19:24
 Operator : CG/JU
 Sample : M3608-12
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBKK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
 Title : SVOA CALIBRATION

37	14.011	1861	1868	1878	rBV	327979	532594	44.30%	5.157%
38	14.299	1911	1917	1928	rVB	333060	526729	43.82%	5.101%
39	14.610	1963	1970	1978	rVB	264495	409711	34.08%	3.967%
40	14.868	2008	2014	2022	rBV5	12073	29809	2.48%	0.289%

41	15.350	2091	2096	2099	rBV	6563	9198	0.77%	0.089%
42	15.603	2132	2139	2147	rBV	464953	700881	58.30%	6.787%
43	15.744	2158	2163	2176	rBV	145623	248751	20.69%	2.409%
44	15.838	2177	2179	2185	rVB2	3599	5843	0.49%	0.057%
45	17.359	2432	2438	2448	rBV	345956	522264	43.44%	5.057%

46	17.459	2448	2455	2466	rVB2	590270	900340	74.90%	8.718%
47	17.588	2474	2477	2480	rVB	1303	1703	0.14%	0.016%
48	17.753	2500	2505	2507	rVB	1120	1840	0.15%	0.018%
49	18.011	2548	2549	2553	rVB2	2126	2131	0.18%	0.021%
50	19.204	2747	2752	2754	rBV4	1149	1753	0.15%	0.017%

51	19.315	2766	2771	2777	rBV5	6805	9509	0.79%	0.092%
52	19.392	2777	2784	2787	rBV3	8483	12280	1.02%	0.119%
53	19.615	2817	2822	2823	rBV3	1668	1943	0.16%	0.019%
54	19.644	2825	2827	2833	rVB3	2130	3005	0.25%	0.029%
55	19.750	2839	2845	2853	rBV	821287	1180779	98.22%	11.434%

56	19.826	2855	2858	2861	rVV4	1636	1993	0.17%	0.019%
57	19.967	2877	2882	2884	rBV5	2121	2684	0.22%	0.026%
58	20.108	2901	2906	2911	rBV3	1971	4878	0.41%	0.047%
59	20.261	2930	2932	2934	rBV2	2075	1777	0.15%	0.017%
60	20.578	2983	2986	2988	rBV2	3061	4122	0.34%	0.040%

61	20.649	2994	2998	3003	rBV5	9705	12760	1.06%	0.124%
62	20.760	3012	3017	3021	rBV7	2623	5461	0.45%	0.053%
63	21.107	3074	3076	3077	rBV2	2503	2332	0.19%	0.023%
64	21.266	3100	3103	3104	rBV2	4056	3850	0.32%	0.037%
65	21.430	3129	3131	3133	rBV3	2265	1923	0.16%	0.019%

66	21.630	3159	3165	3174	rVB	394731	645808	53.72%	6.254%
67	22.605	3330	3331	3334	rBV3	3002	2575	0.21%	0.025%
68	23.069	3406	3410	3411	rBV3	9129	10898	0.91%	0.106%
69	23.398	3464	3466	3471	rVB5	3468	4781	0.40%	0.046%
70	24.044	3574	3576	3579	rBV3	3497	4037	0.34%	0.039%

71	24.256	3610	3612	3614	rBV3	3052	2158	0.18%	0.021%
72	24.626	3663	3675	3686	rBV2	436901	1202129	100.00%	11.641%
73	24.749	3695	3696	3698	rBV2	3911	2213	0.18%	0.021%
74	24.843	3702	3712	3725	rVB	236671	681058	56.65%	6.595%
75	25.930	3891	3897	3906	rVB10	12721	37549	3.12%	0.364%

76	27.440	4152	4154	4155	rBV3	3567	1955	0.16%	0.019%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050236.D
Acq On : 9 Sep 2021 19:24
Operator : CG/JU
Sample : M3608-12
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKK8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Title : SVOA CALIBRATION

77	27.933	4236	4238	4240	rBV2	3089	2393	0.20%	0.023%
78	28.632	4355	4357	4358	rVB2	3363	1570	0.13%	0.015%
79	30.295	4638	4640	4641	rBV	3182	2550	0.21%	0.025%
80	30.588	4688	4690	4693	rBV4	2886	2471	0.21%	0.024%
81	31.064	4769	4771	4772	rBV2	3100	2165	0.18%	0.021%
82	32.239	4969	4971	4972	rVB	4811	2765	0.23%	0.027%




Sum of corrected areas: 10326950

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050236.D
Acq On : 9 Sep 2021 19:24
Operator : CG/JU
Sample : M3608-12
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKK8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

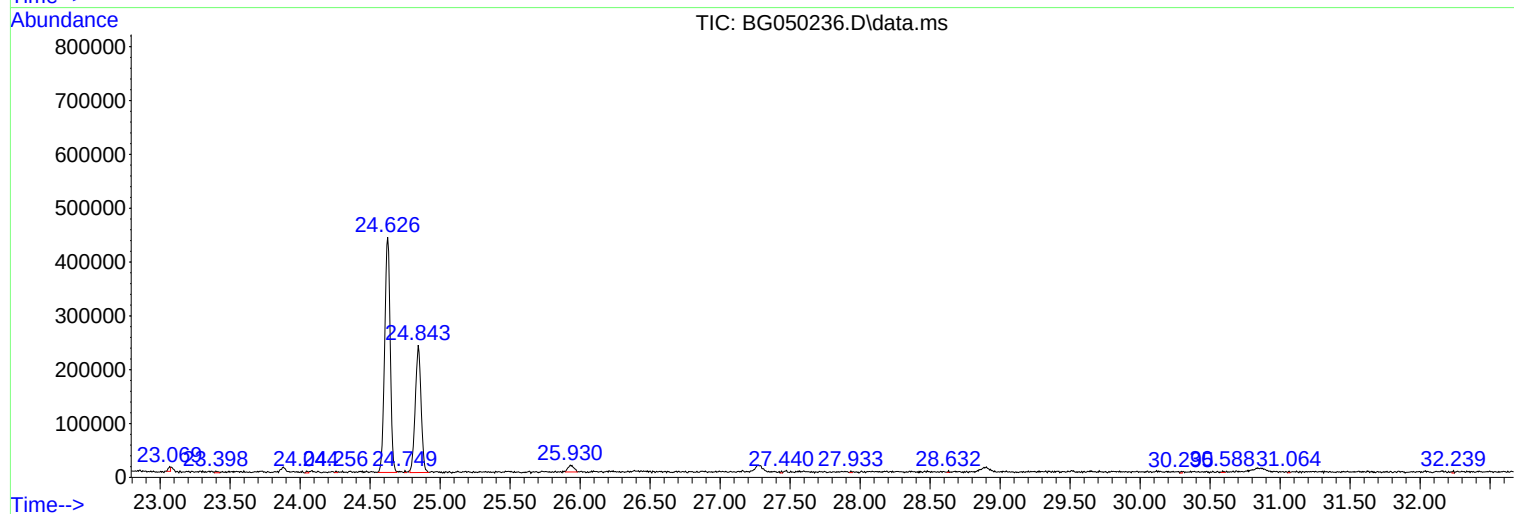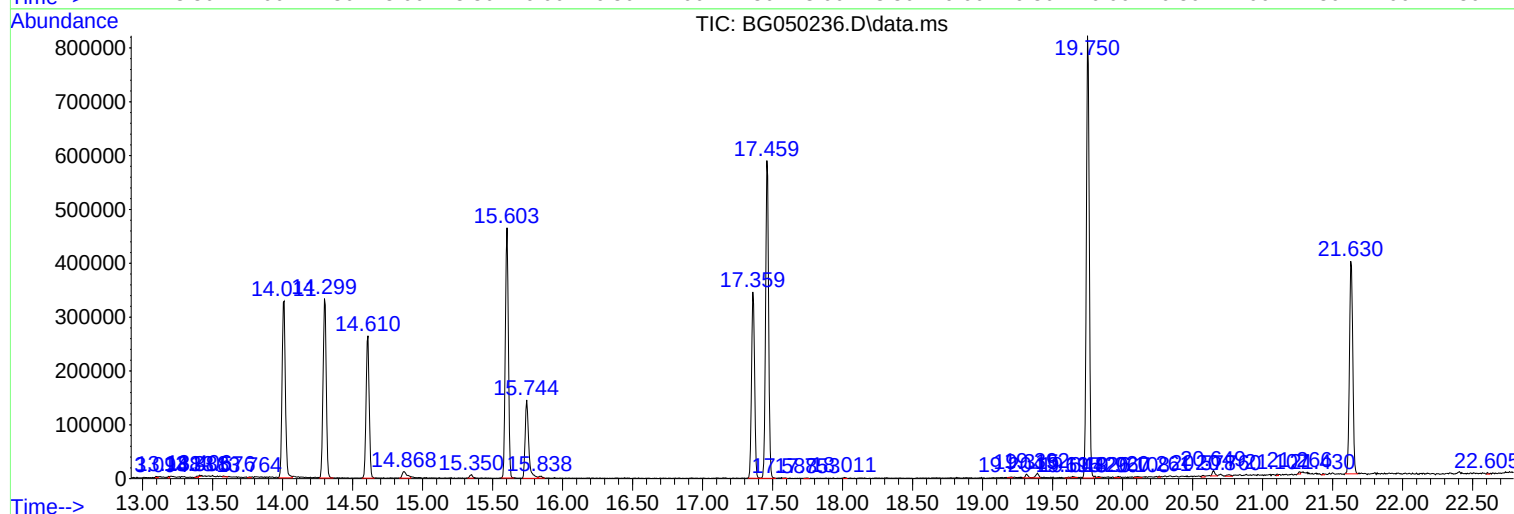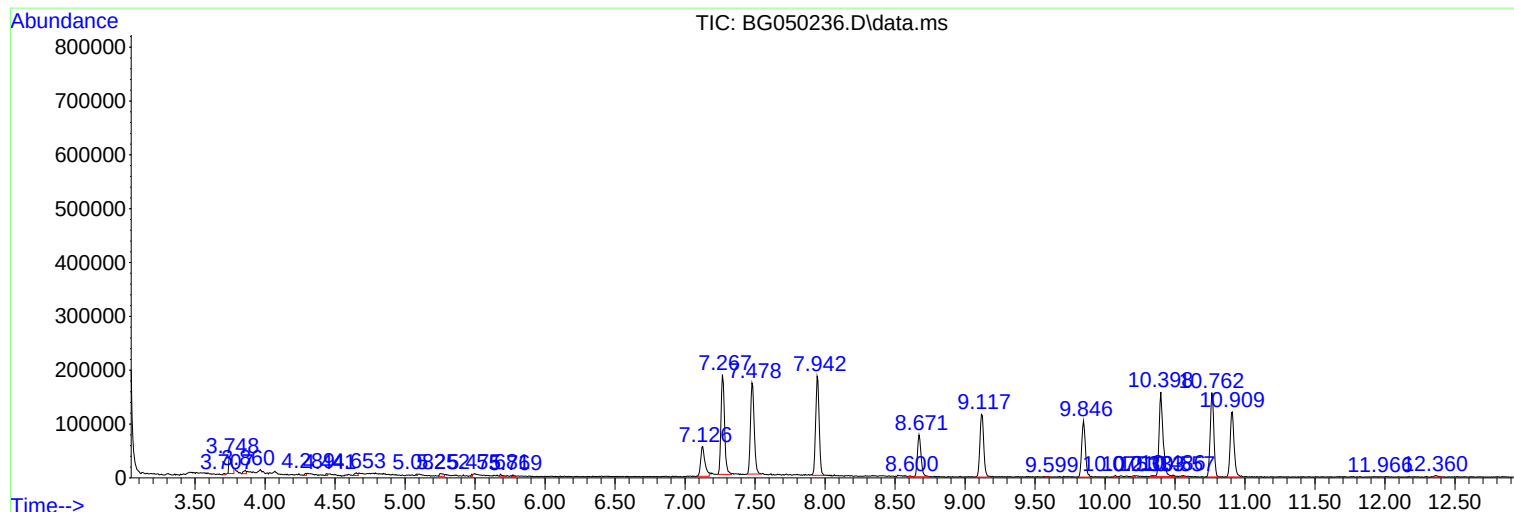

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050236.D
Acq On : 9 Sep 2021 19:24
Operator : CG/JU
Sample : M3608-12
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKK8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090721\
Data File : BG050236.D
Acq On : 9 Sep 2021 19:24
Operator : CG/JU
Sample : M3608-12
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBKK8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG090721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
