
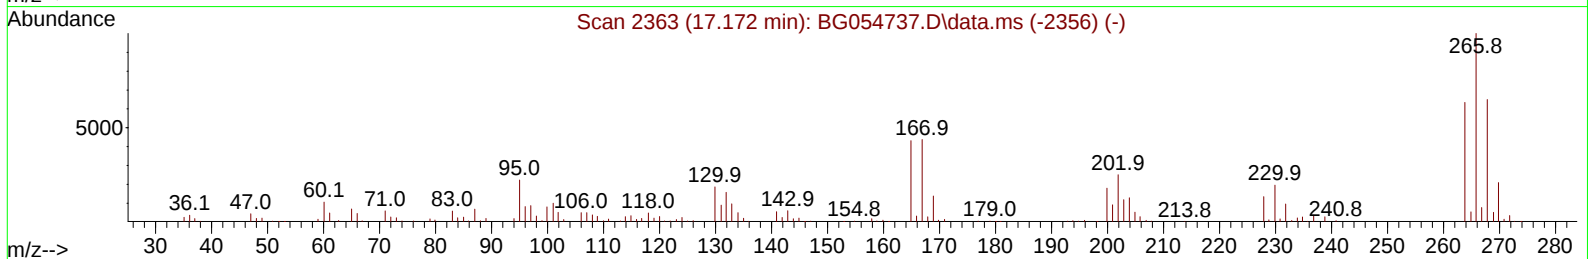
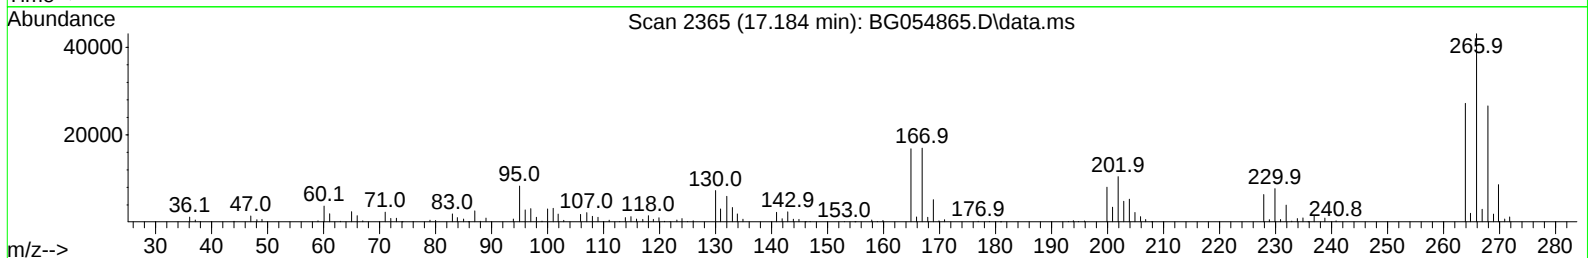


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
Data File : BG054865.D
Acq On : 7 Sep 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 06:29:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

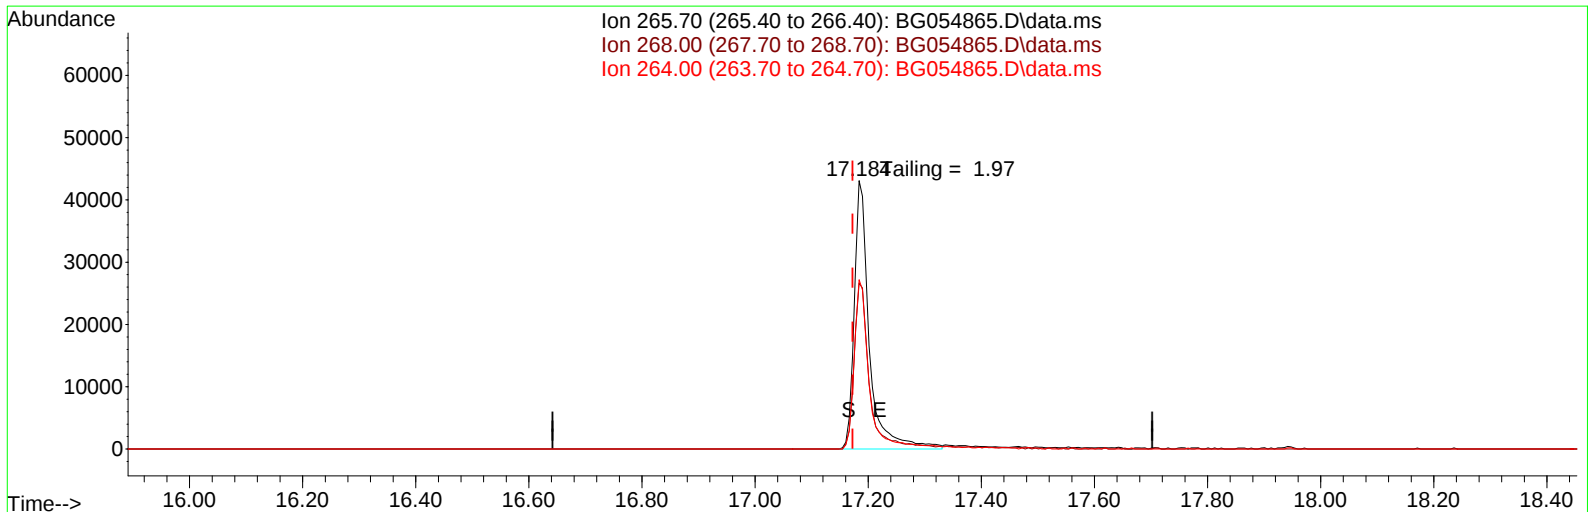

TIC: BG054865.D\data.ms

(70) Pentachlorophenol (C)




17.184min (+ 0.011) 218000.39 ng

response 80406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	61.80
264.00	61.70	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
Data File : BG054865.D
Acq On : 7 Sep 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 06:29:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

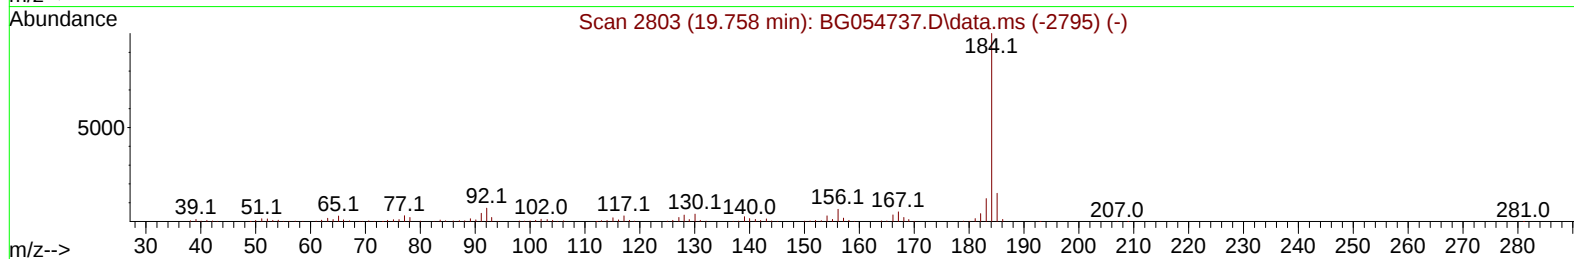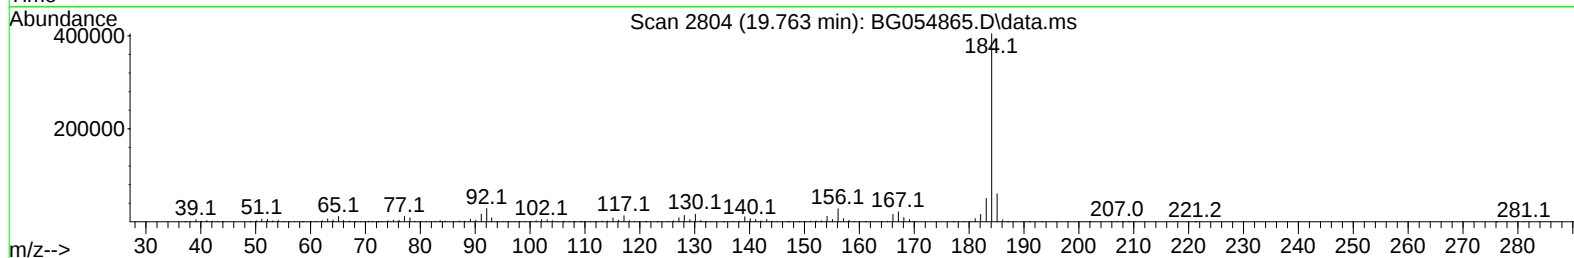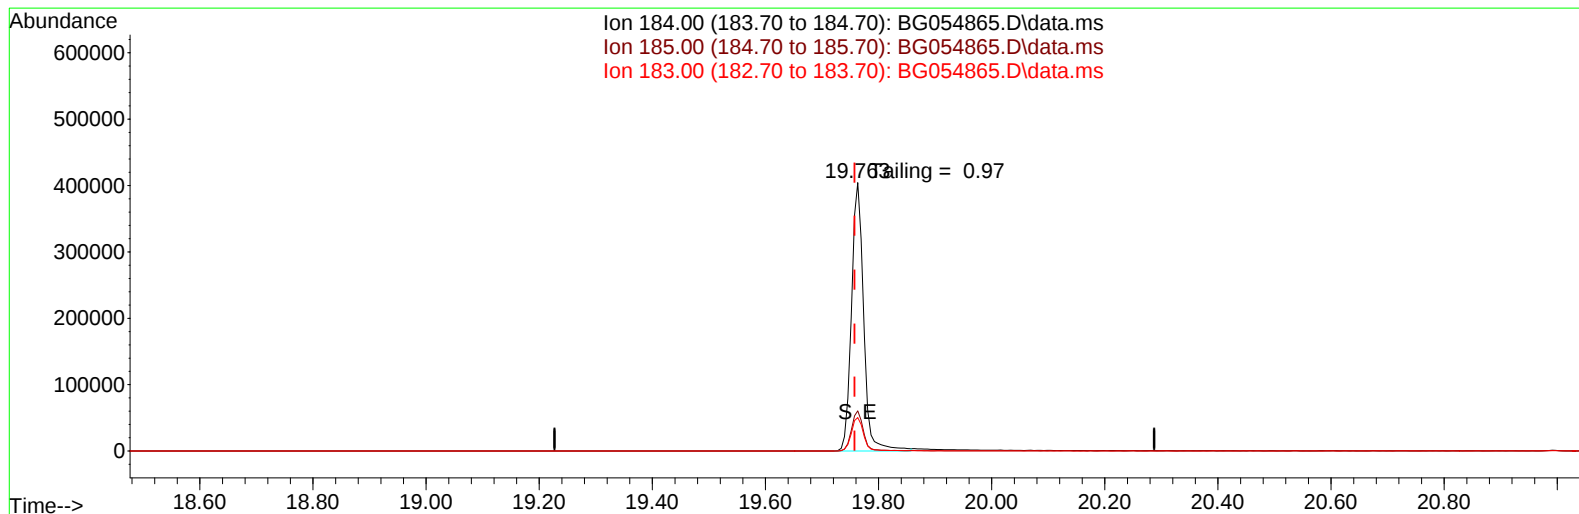

TIC: BG054865.D\data.ms

(77) Benzidine**19.763min (+ 0.006) 427241.10 ng****response 624352**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.97
183.00	12.30	12.46
0.00	0.00	0.00