

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
 Data File : BG054878.D
 Acq On : 7 Sep 2022 21:23
 Operator : CG/JU
 Sample : N4506-01 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OK-03-090222

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.691	403	409	418	rBV	37986	62401	8.27%	1.337%
2	7.307	677	684	693	rBV	35153	65338	8.66%	1.400%
3	8.147	820	827	837	rVB	184799	324464	43.02%	6.954%
4	9.322	1021	1027	1036	rBV	20351	39578	5.25%	0.848%
5	10.979	1301	1309	1322	rBV	251393	474645	62.93%	10.173%
6	13.406	1716	1722	1729	rBV	71251	110868	14.70%	2.376%
7	14.786	1948	1957	1965	rBV	413872	653994	86.71%	14.016%
8	16.273	2205	2210	2217	rBV	41157	64892	8.60%	1.391%
9	17.530	2418	2424	2430	rBV	469551	745647	98.87%	15.981%
10	17.577	2430	2432	2436	rVB	32282	35109	4.66%	0.752%
11	17.994	2500	2503	2508	rVB5	5895	9358	1.24%	0.201%
12	18.112	2520	2523	2528	rBV3	6794	10540	1.40%	0.226%
13	18.259	2544	2548	2553	rBV4	4735	10051	1.33%	0.215%
14	18.411	2569	2574	2577	rBV	19740	32948	4.37%	0.706%
15	18.453	2577	2581	2587	rVB	24409	39132	5.19%	0.839%
16	18.594	2600	2605	2609	rBV3	21628	41263	5.47%	0.884%
17	18.641	2610	2613	2617	rVB	15281	21933	2.91%	0.470%
18	18.682	2617	2620	2625	rBV4	8696	12963	1.72%	0.278%
19	18.899	2654	2657	2661	rBV5	9542	15320	2.03%	0.328%
20	19.199	2704	2708	2710	rBV2	15511	21029	2.79%	0.451%
21	19.310	2723	2727	2732	rBV2	41545	68345	9.06%	1.465%
22	19.581	2769	2773	2778	rVB	42548	59796	7.93%	1.282%
23	19.945	2831	2835	2841	rVB	75083	117808	15.62%	2.525%
24	20.127	2862	2866	2870	rVB	124809	155066	20.56%	3.323%
25	21.831	3150	3156	3161	rBV	431707	719211	95.36%	15.414%
26	25.215	3724	3732	3746	rVB2	239865	754194	100.00%	16.164%



Sum of corrected areas: 4665893

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
Data File : BG054878.D
Acq On : 7 Sep 2022 21:23
Operator : CG/JU
Sample : N4506-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-03-090222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

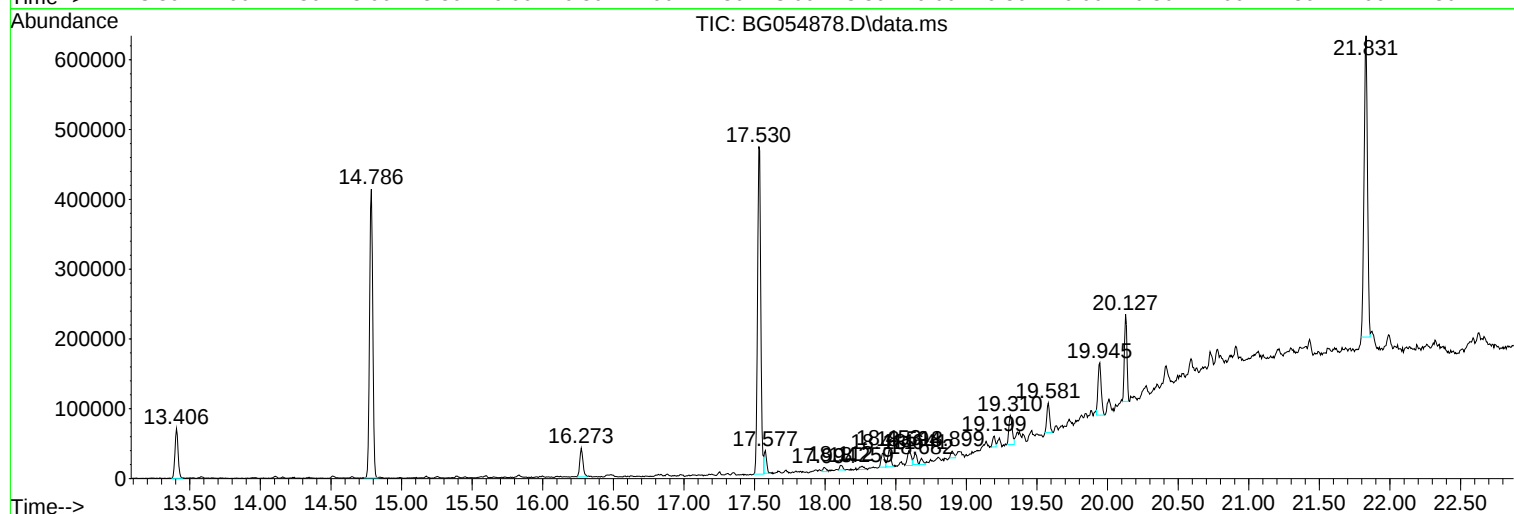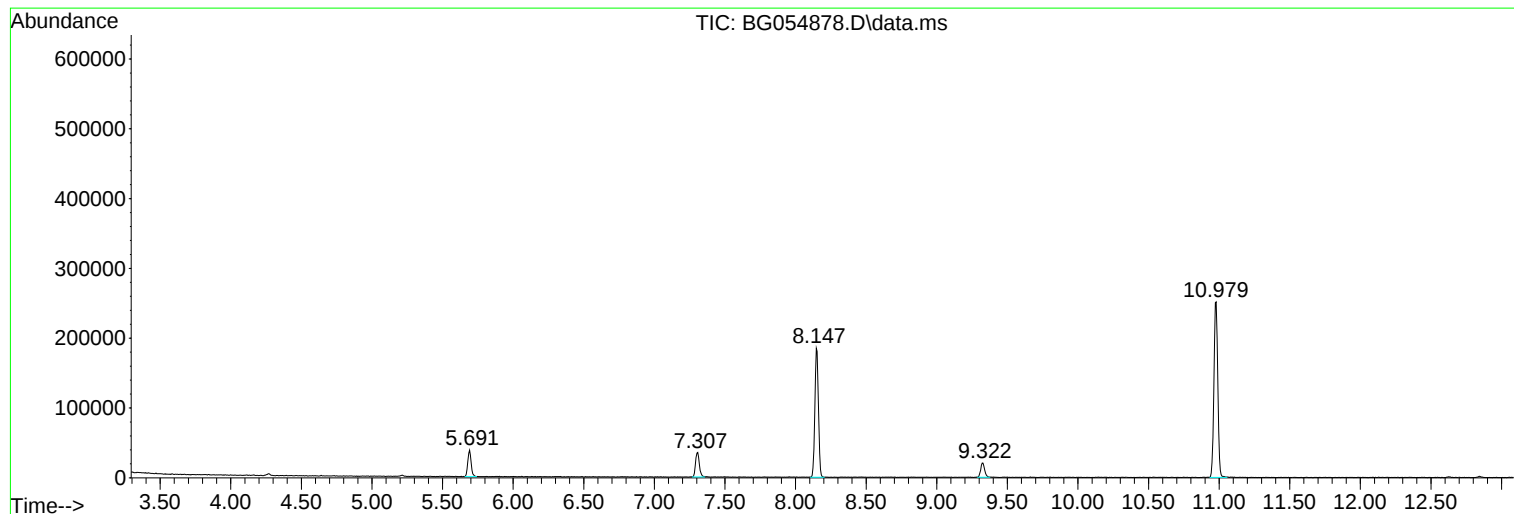

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
Data File : BG054878.D
Acq On : 7 Sep 2022 21:23
Operator : CG/JU
Sample : N4506-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-03-090222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
Data File : BG054878.D
Acq On : 7 Sep 2022 21:23
Operator : CG/JU
Sample : N4506-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-03-090222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------