


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
 Data File : BG054865.D
 Acq On : 7 Sep 2022 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

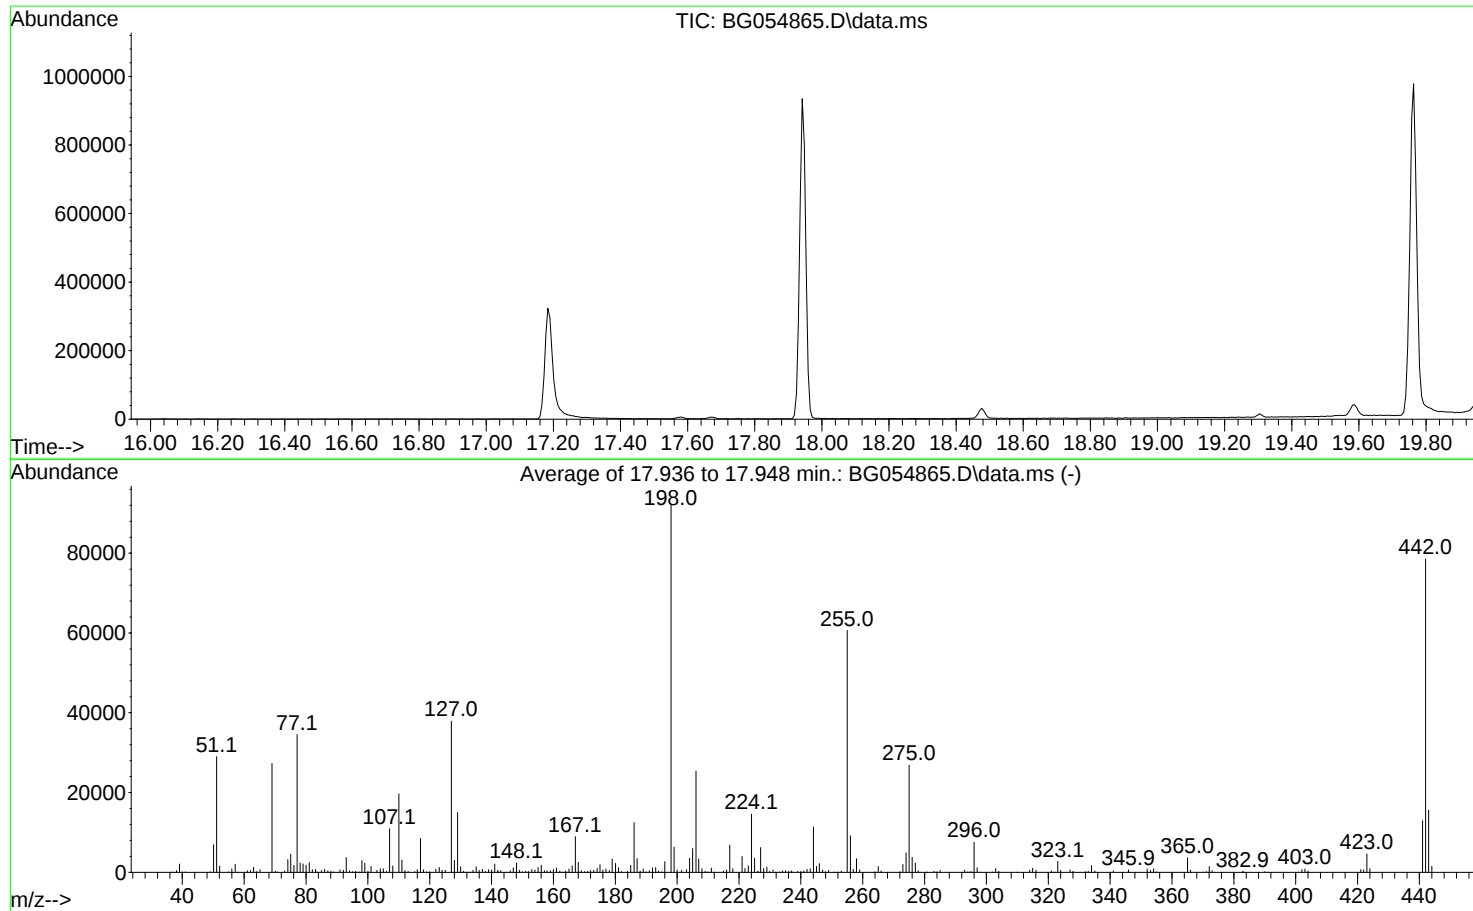




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	28976	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.6	27307	PASS
70	69	0.00	2	1.0	268	PASS
127	198	10	80	41.1	37896	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92229	PASS
199	198	5	9	6.8	6302	PASS
275	198	10	60	29.1	26861	PASS
365	198	1	100	3.9	3625	PASS
441	198	0.01	100	14.0	12931	PASS
442	442	50	100	100.0	78539	PASS
443	442	15	24	19.8	15537	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
Data File : BG054865.D
Acq On : 7 Sep 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 08 06:29:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

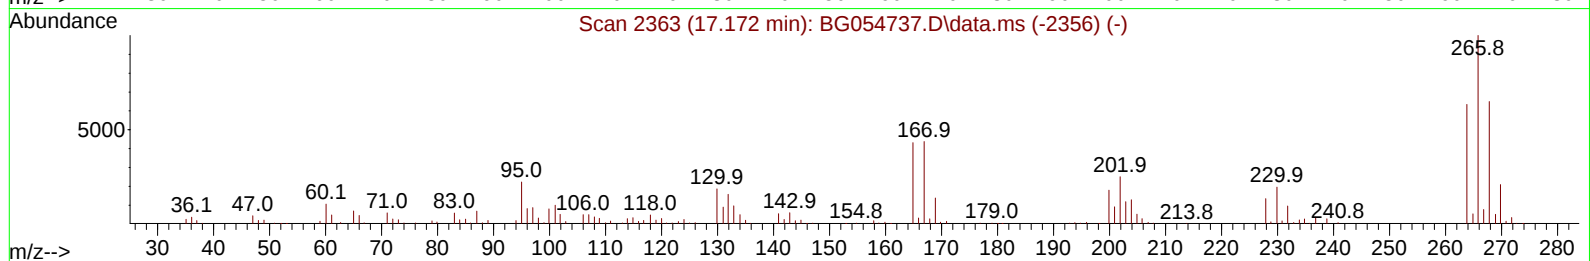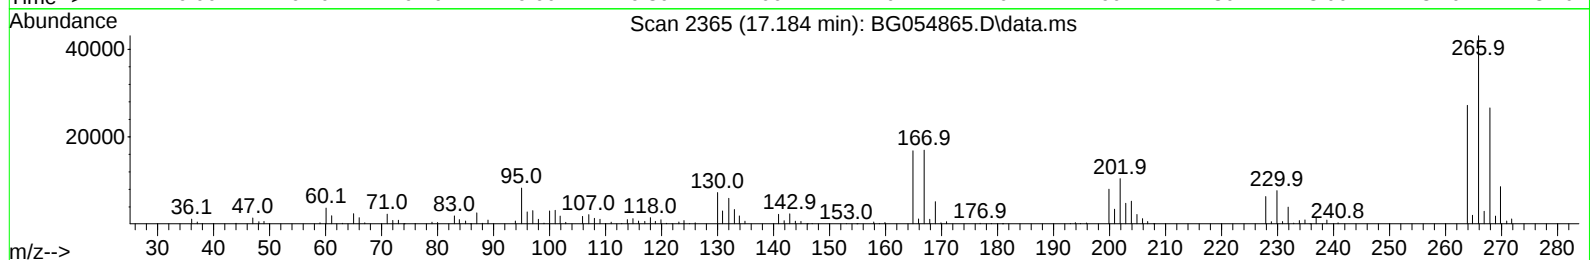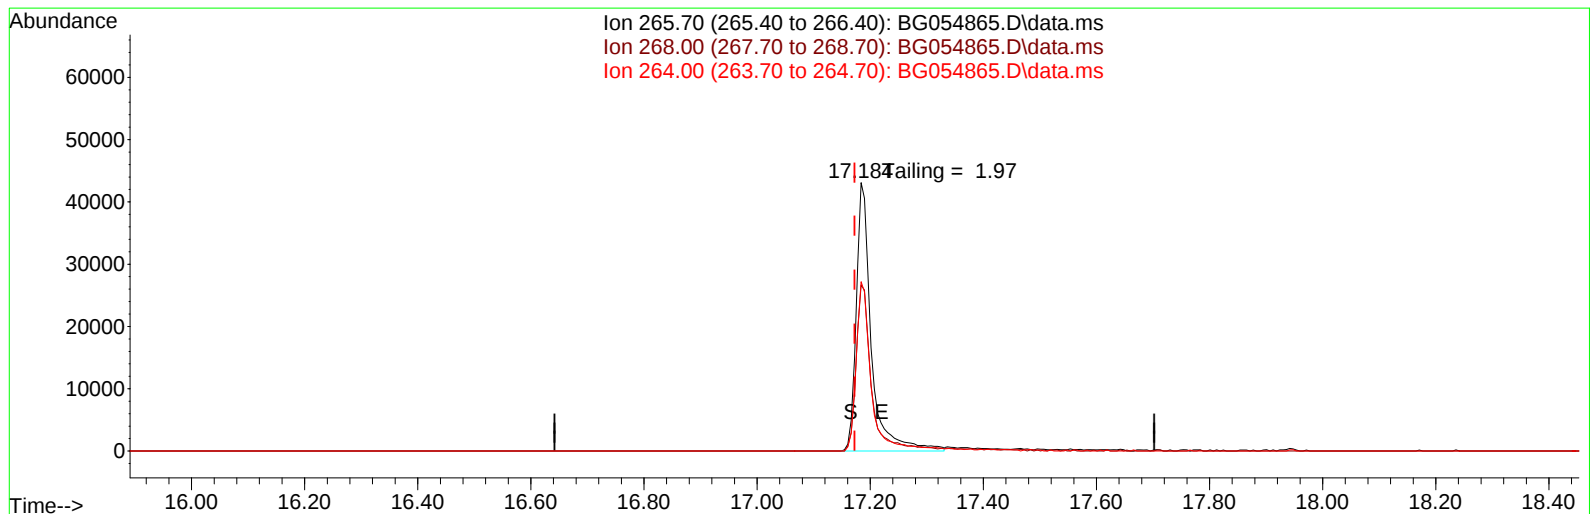

TIC: BG054865.D\data.ms

(70) Pentachlorophenol (C)

17.184min (+ 0.011) 218000.39 ng




response 80406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	61.80
264.00	61.70	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090722\
Data File : BG054865.D
Acq On : 7 Sep 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 08 06:29:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

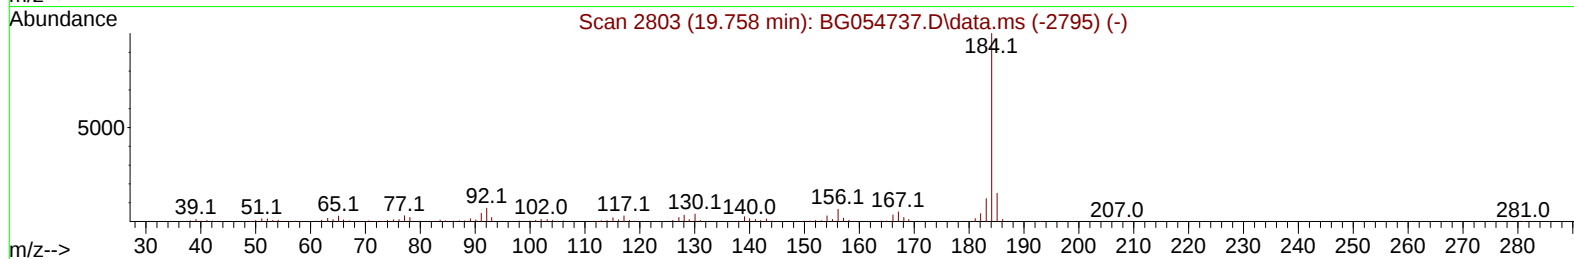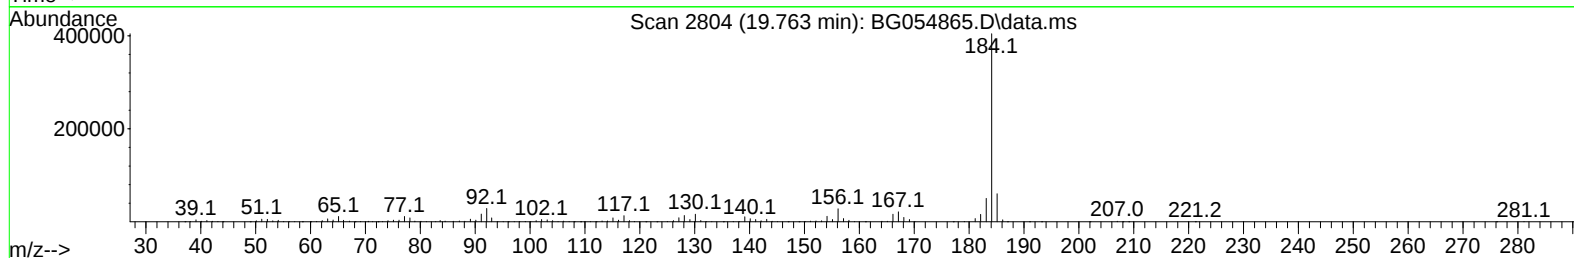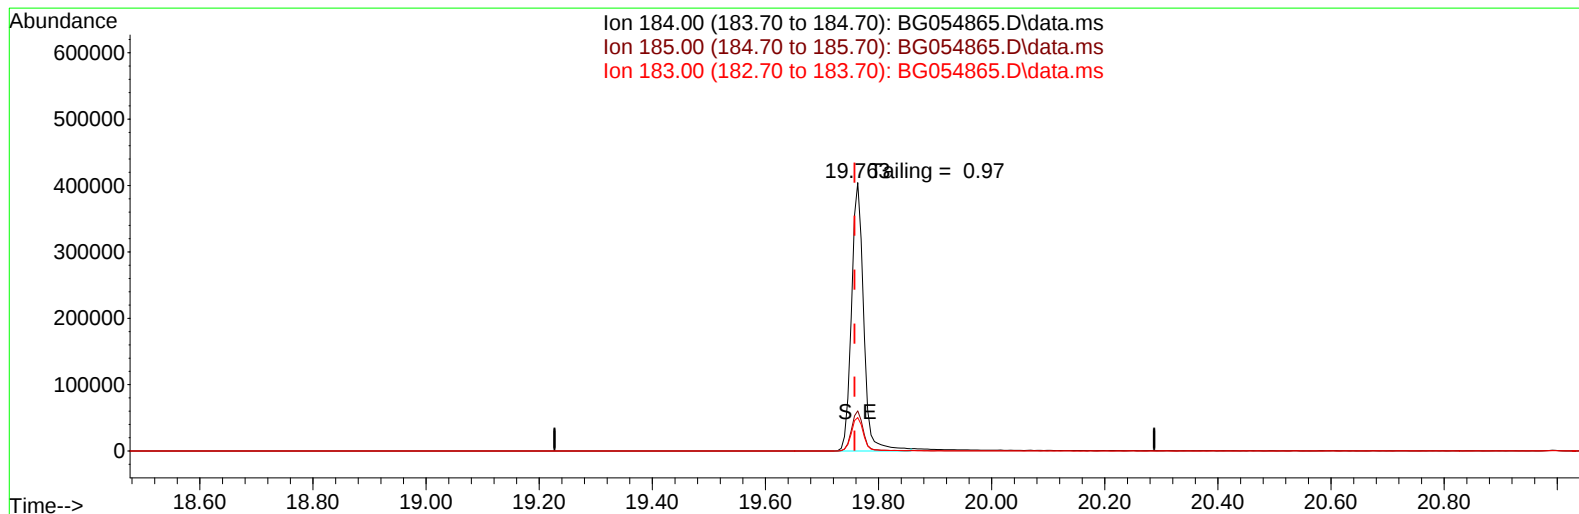

TIC: BG054865.D\data.ms

(77) Benzidine

19.763min (+ 0.006) 427241.10 ng

response 624352

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.97
183.00	12.30	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/7/2022	BNA_G	BG054865.D
Compound Name	Response	Retention Time
DDT	291148	20.991
DDD	10304	20.545
DDE	1222	20.039
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11526	302674	3.81

Instrument :
BNA_G
ClientSampleId :
DFTPP