
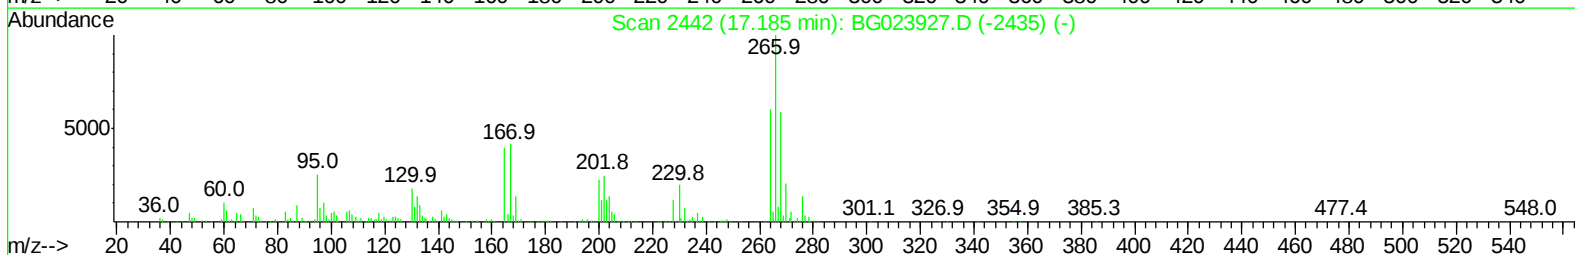
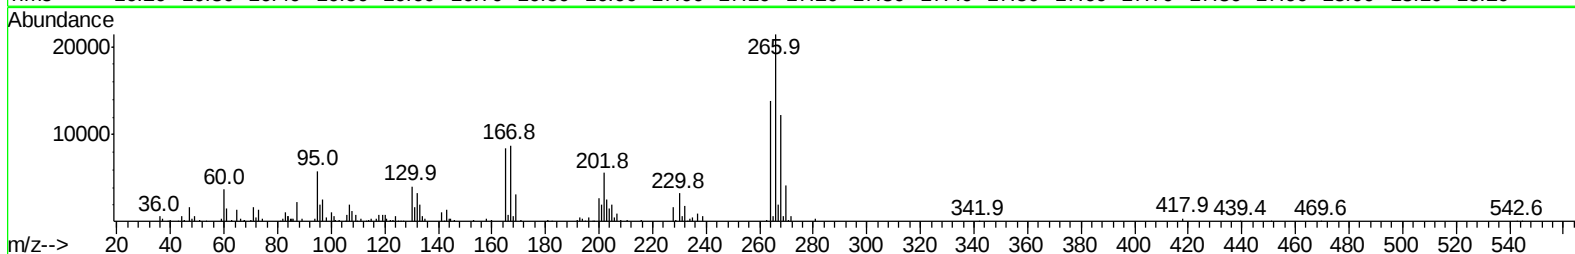


Data Path : Z:\HPCHEM1\BNA G\DATA\BG090816\
Data File : BG023963.D
Acq On : 8 Sep 2016 10:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 16:07:12 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 15 05:42:37 2004
Response via : Initial Calibration

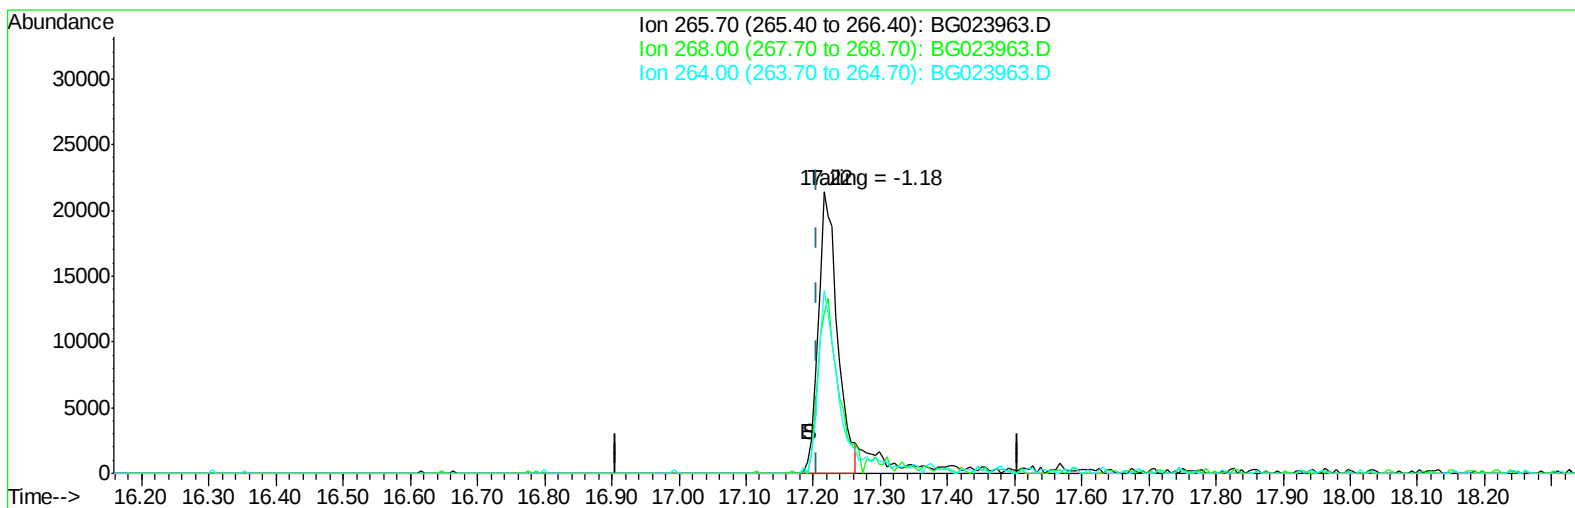

TIC: BG023963.D

(69) Pentachlorophenol (C)




17.216min (+0.010) 51753.02ng m

response 47065

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	56.88
264.00	63.20	64.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090816\
Data File : BG023963.D
Acq On : 8 Sep 2016 10:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 16:07:12 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 15 05:42:37 2004
Response via : Initial Calibration

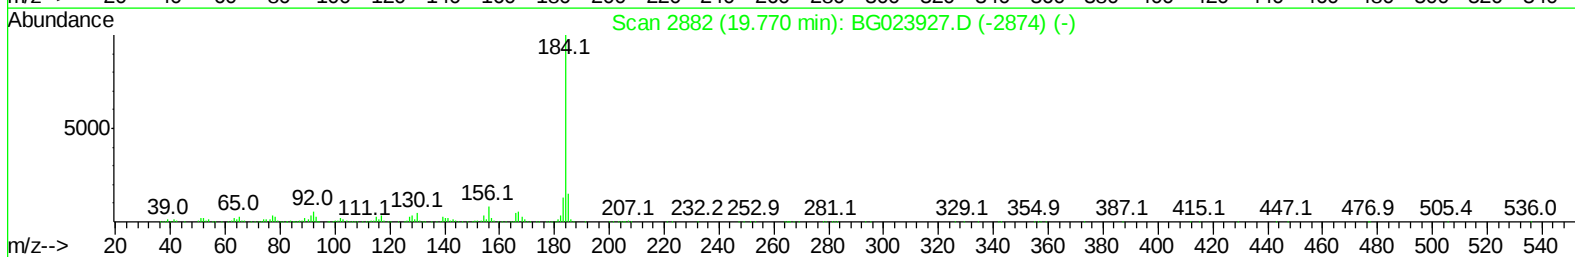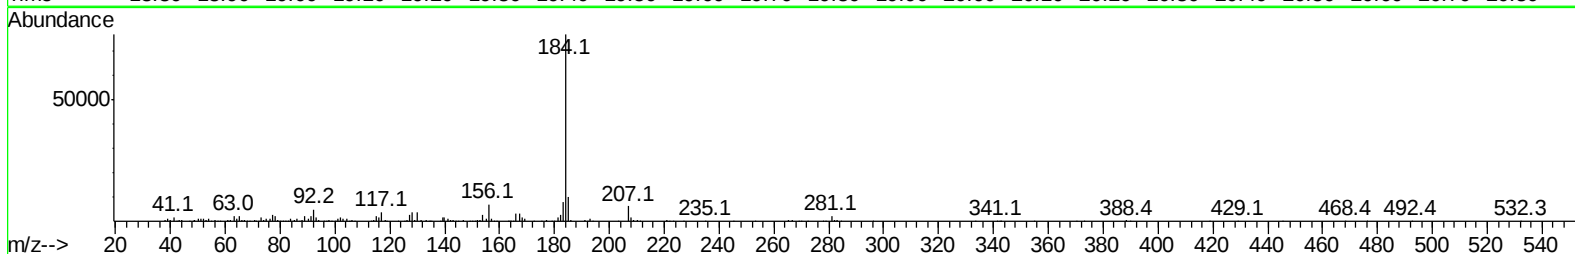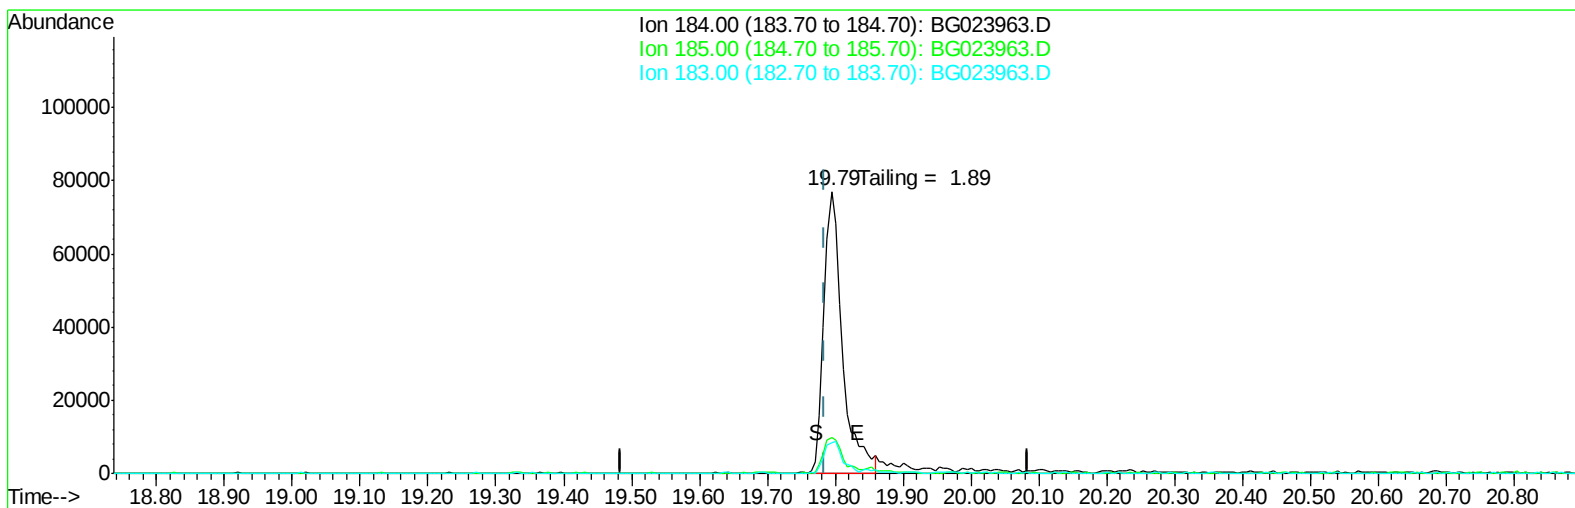

TIC: BG023963.D

(76) Benzidine

19.794min (+0.010) 41355.00ng

response 149829

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	12.93
183.00	13.40	10.75
0.00	0.00	0.00