


Data Path : Z:\HPCHEM1\BNA_G\Data\BG090816\
Data File : BG023963.D
Acq On : 8 Sep 2016 10:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 31 20:05:47 2016

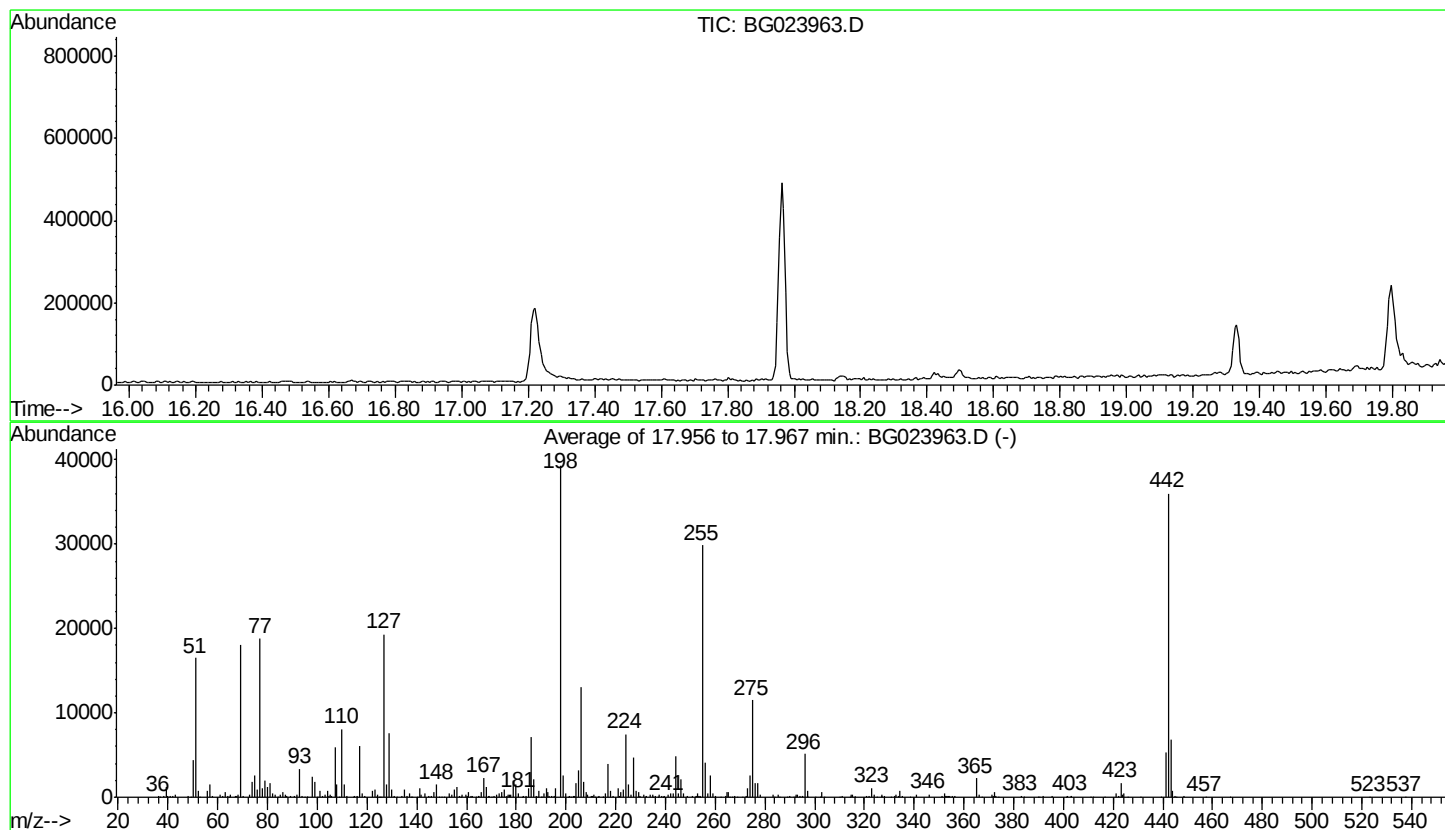

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	16478	PASS
68	69	0.00	2	1.4	261	PASS
69	198	0.00	100	45.8	18005	PASS
70	69	0.00	2	0.9	171	PASS
127	198	10	80	49.1	19282	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39309	PASS
199	198	5	9	6.5	2564	PASS
275	198	10	60	29.3	11522	PASS
365	198	1	100	5.7	2257	PASS
441	442	0.01	24	14.6	5255	PASS
442	198	50	100	91.6	36024	PASS
443	442	15	24	18.8	6758	PASS