
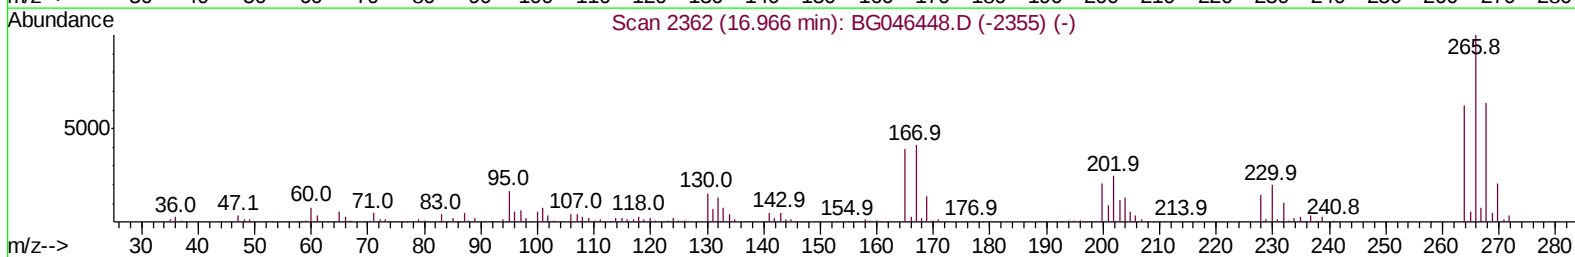
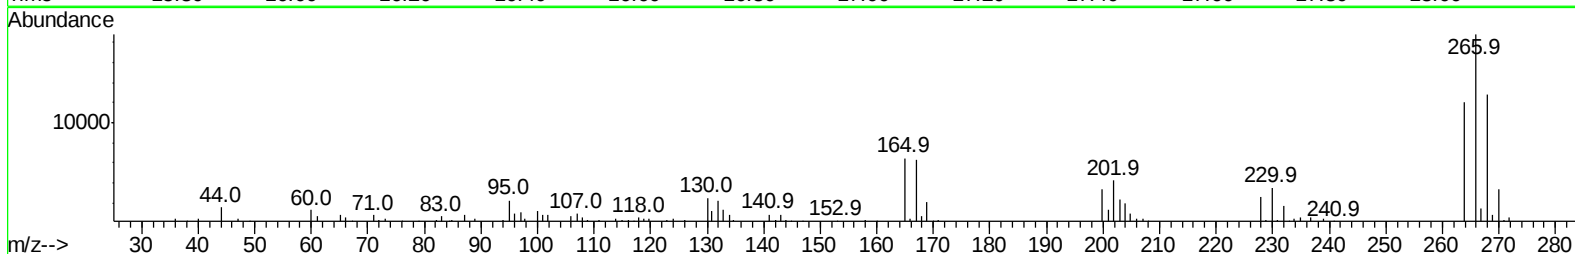


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090820\
Data File : BG046551.D
Acq On : 8 Sep 2020 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 08:50:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

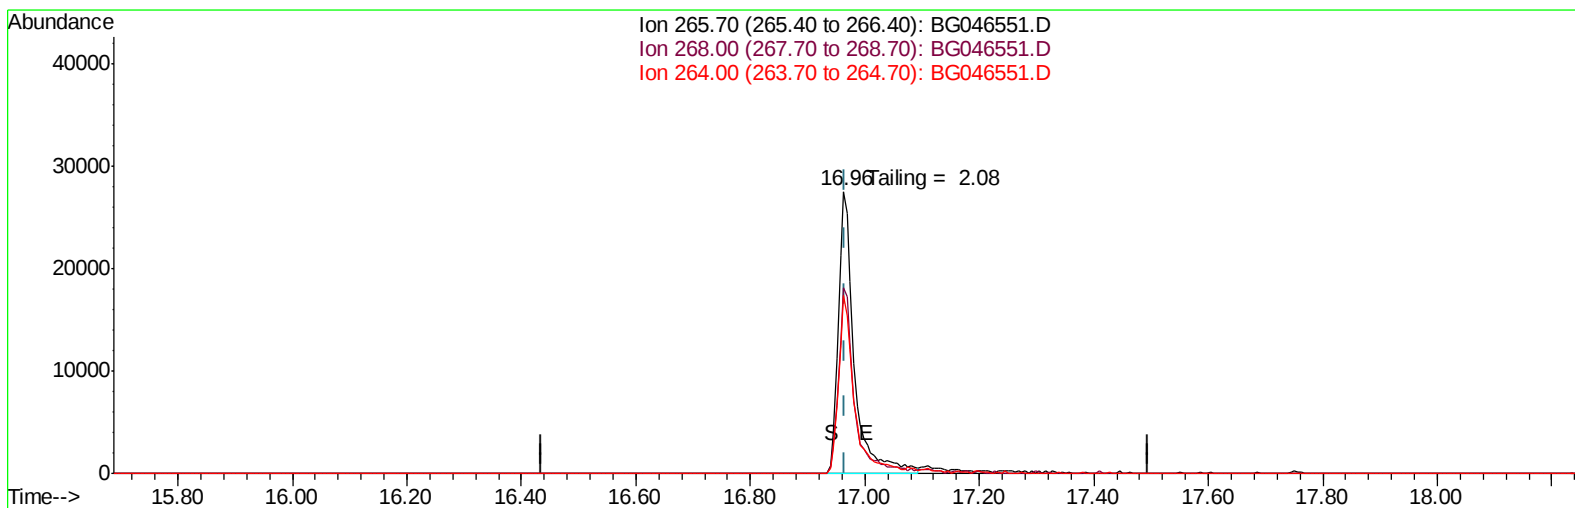

TIC: BG046551.D

(70) Pentachlorophenol (C)




16.963min (-0.002) 21728.08ng

response 53979

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.09
264.00	62.70	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090820\
 Data File : BG046551.D
 Acq On : 8 Sep 2020 9:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 08:50:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 15:06:53 2020
 Response via : Initial Calibration

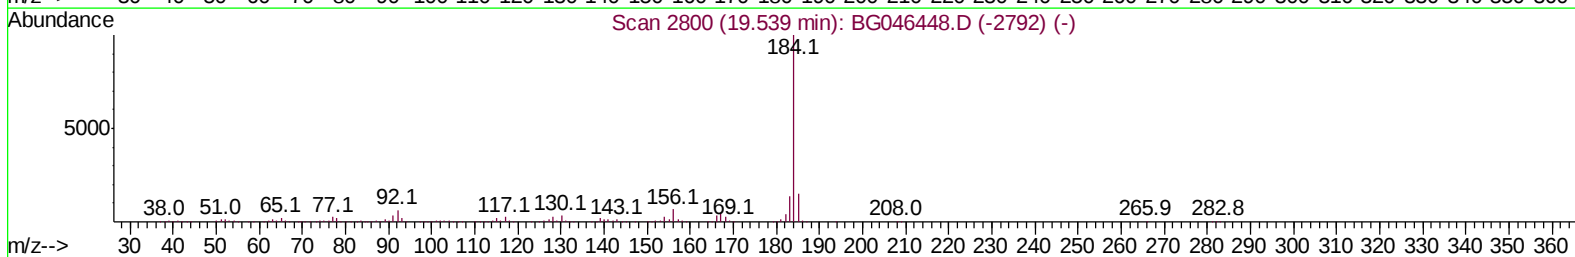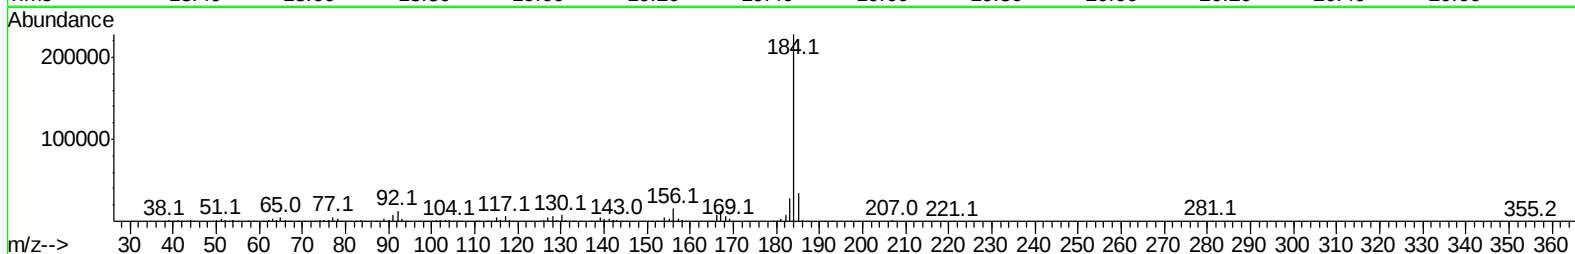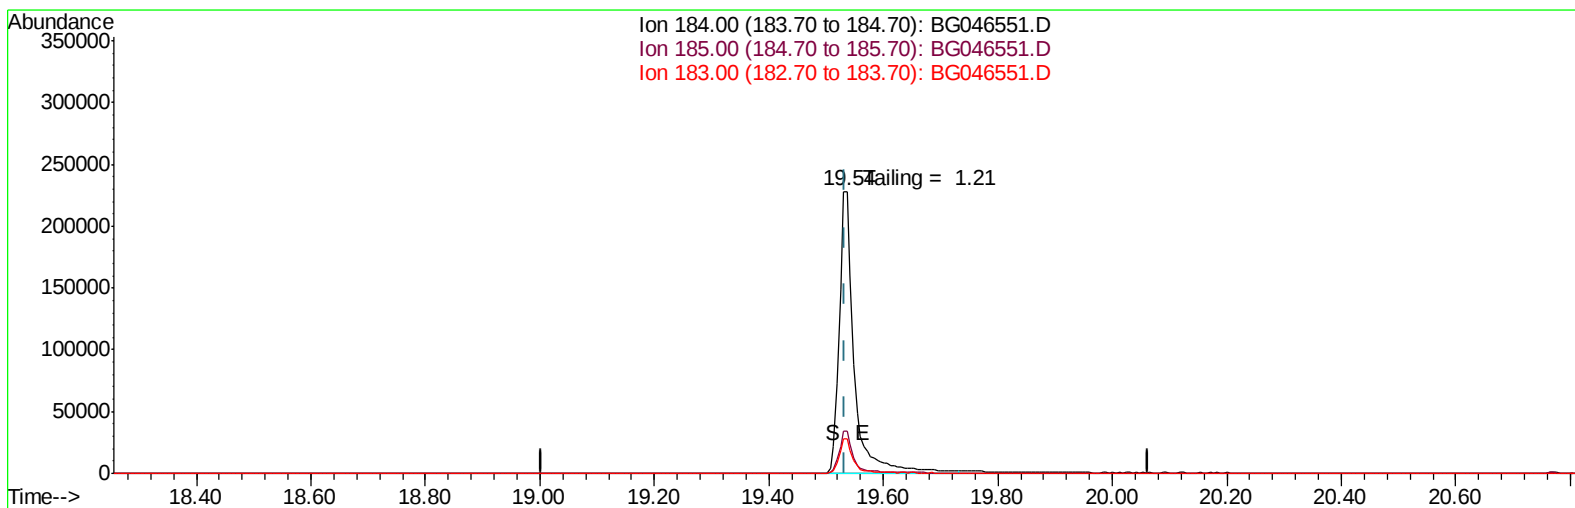

TIC: BG046551.D

(77) Benzidine

19.537min (+0.004) 326424.67ng

response 424766

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.00
183.00	13.40	12.46
0.00	0.00	0.00