


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090820\
 Data File : BG046551.D
 Acq On : 8 Sep 2020 9:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 15:06:53 2020

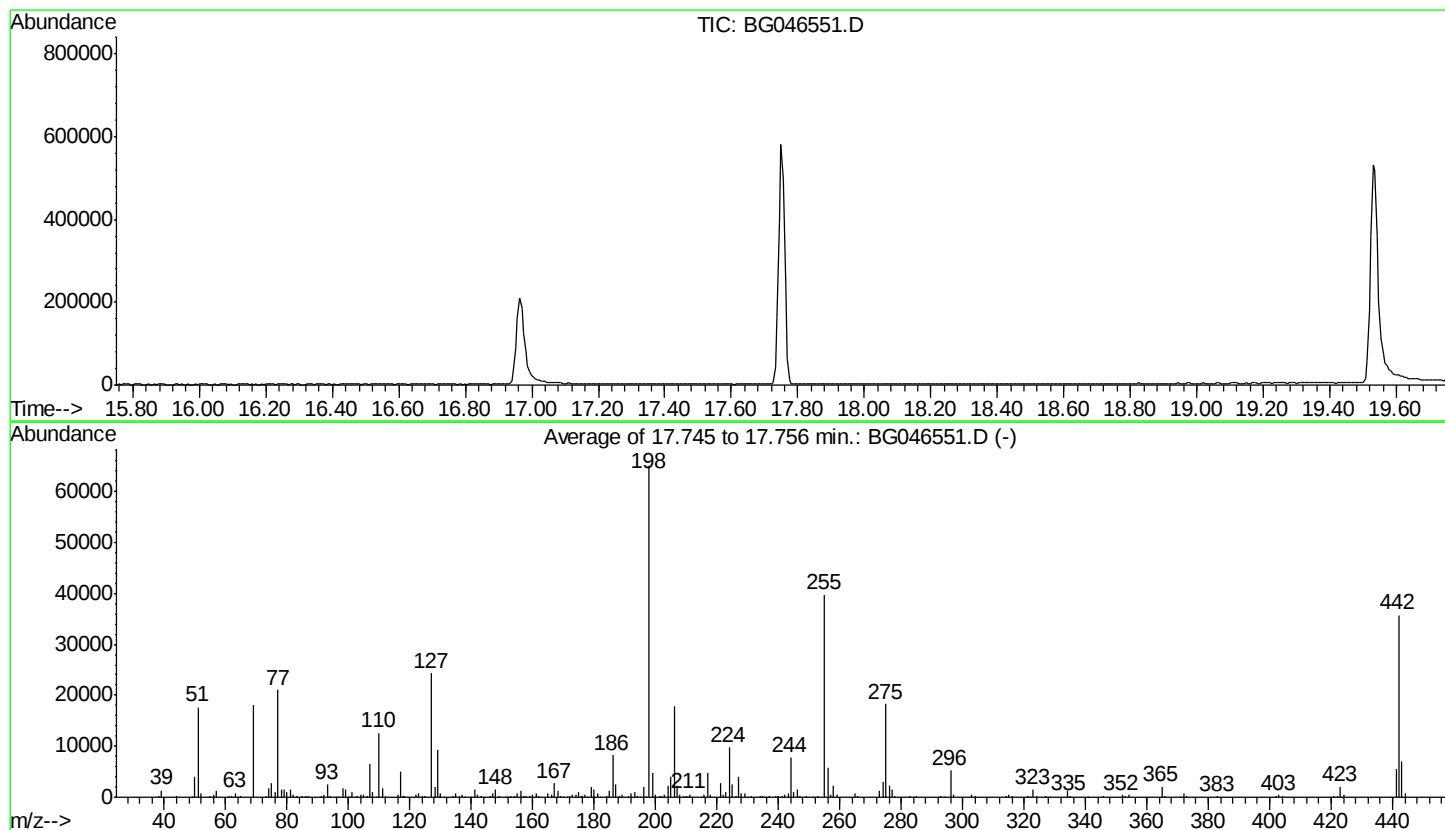

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.2	17706	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.8	18087	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.4	24341	PASS
197	198	0.00	2	0.3	170	PASS
198	198	100	100	100.0	65074	PASS
199	198	5	9	7.4	4814	PASS
275	198	10	60	28.1	18284	PASS
365	198	1	100	3.1	2018	PASS
441	198	0.01	100	8.6	5615	PASS
442	198	50	100	54.9	35736	PASS
443	442	15	24	19.8	7084	PASS