
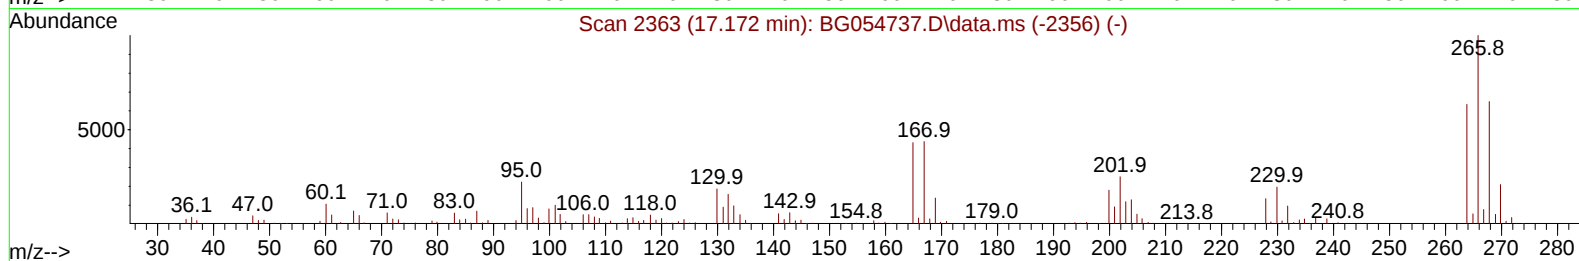
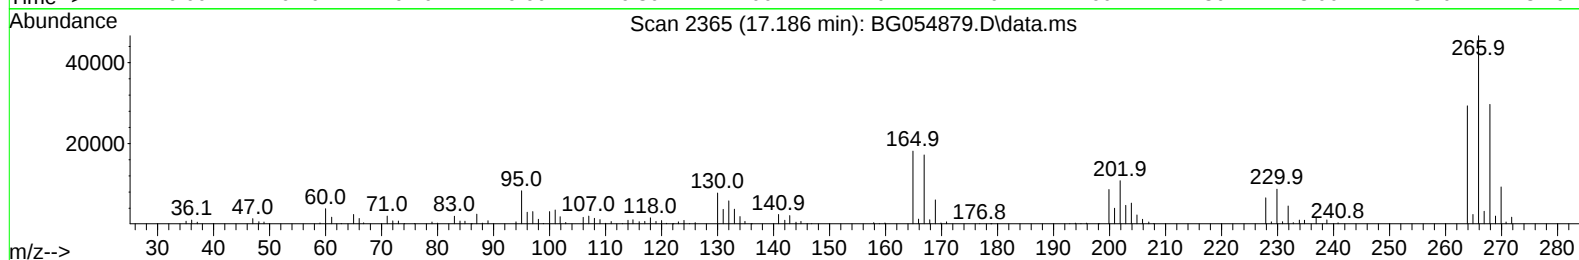


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090822\
Data File : BG054879.D
Acq On : 8 Sep 2022 9:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 03:54:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 02:45:21 2022
Response via : Initial Calibration

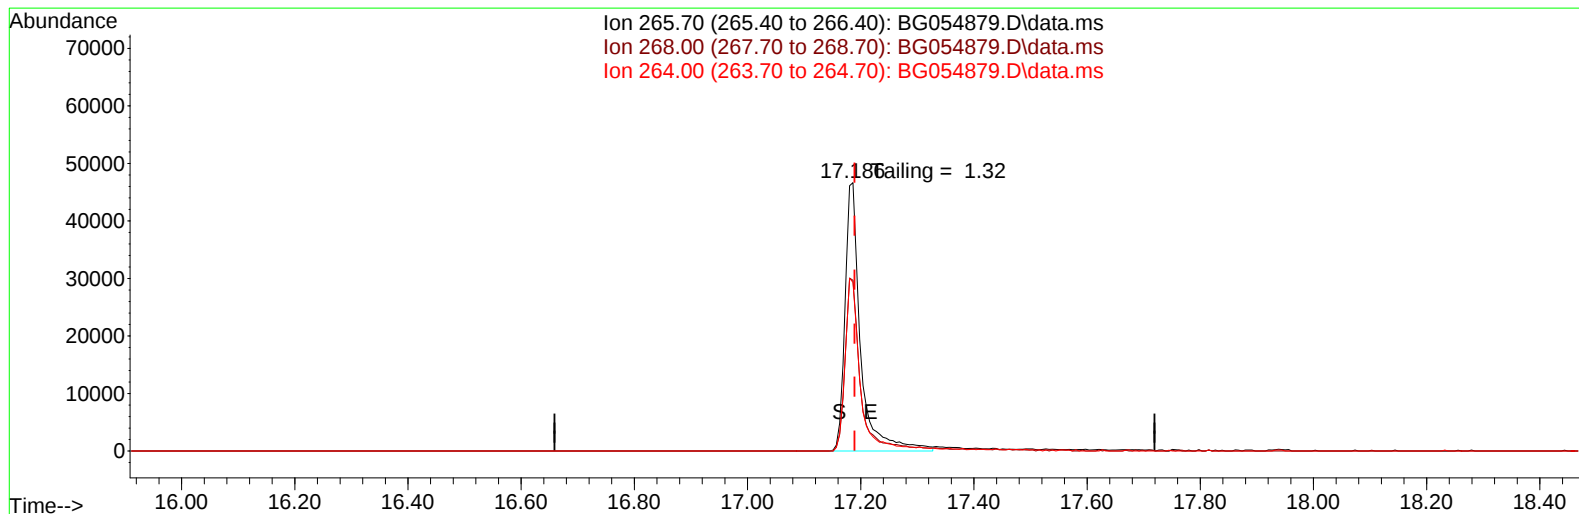

TIC: BG054879.D\data.ms

(70) Pentachlorophenol (C)




17.186min (-0.003) 32157.98 ng

response 89712

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.60
264.00	61.70	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090822\
Data File : BG054879.D
Acq On : 8 Sep 2022 9:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 03:54:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 02:45:21 2022
Response via : Initial Calibration

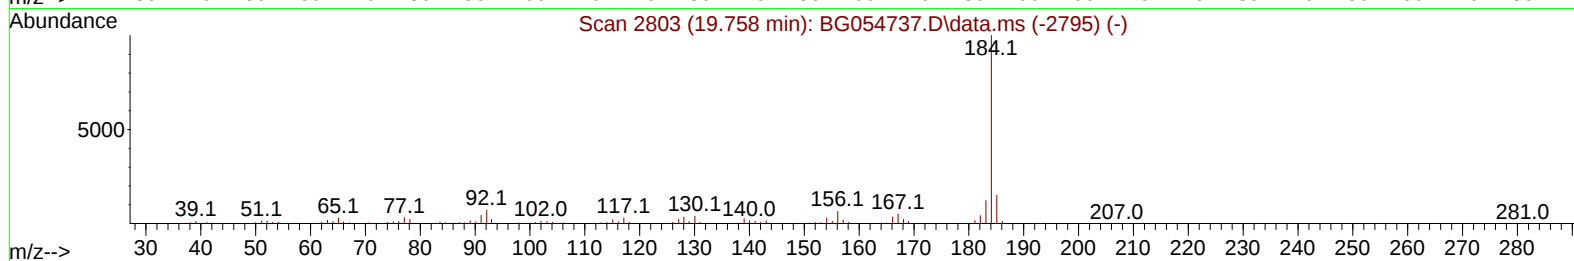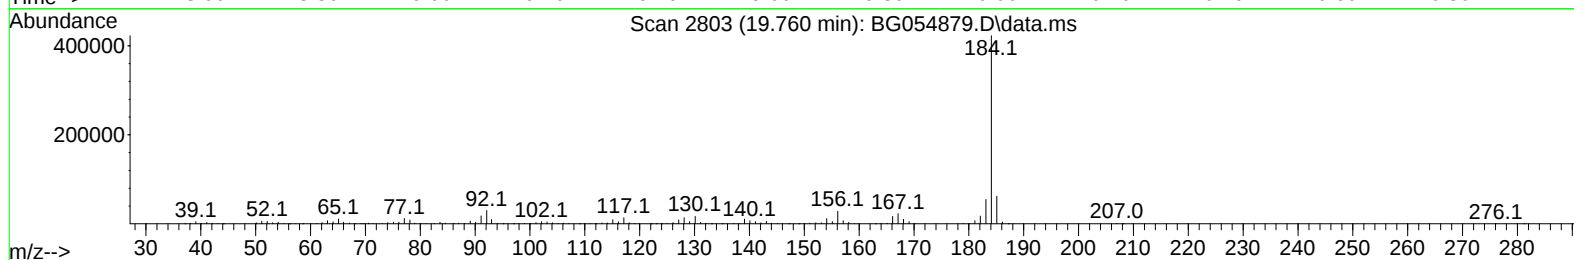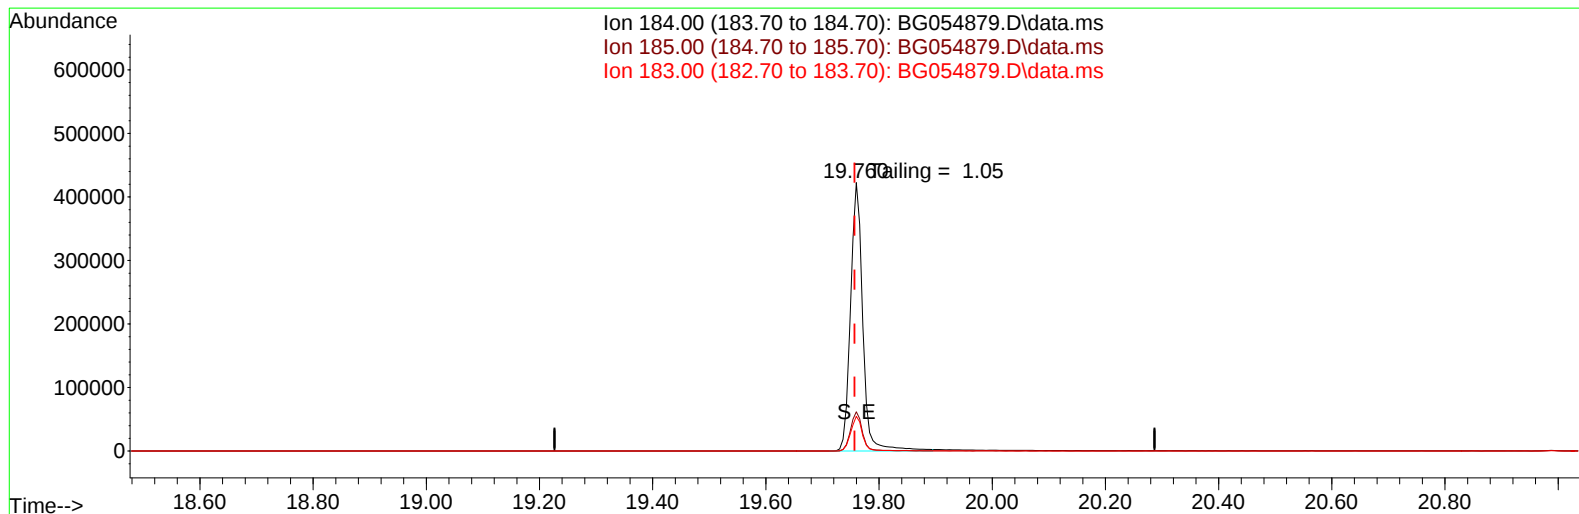

TIC: BG054879.D\data.ms

(77) Benzidine

19.760min (+ 0.003) 0.00 ng

response 644476

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.65
183.00	12.30	12.95
0.00	0.00	0.00