
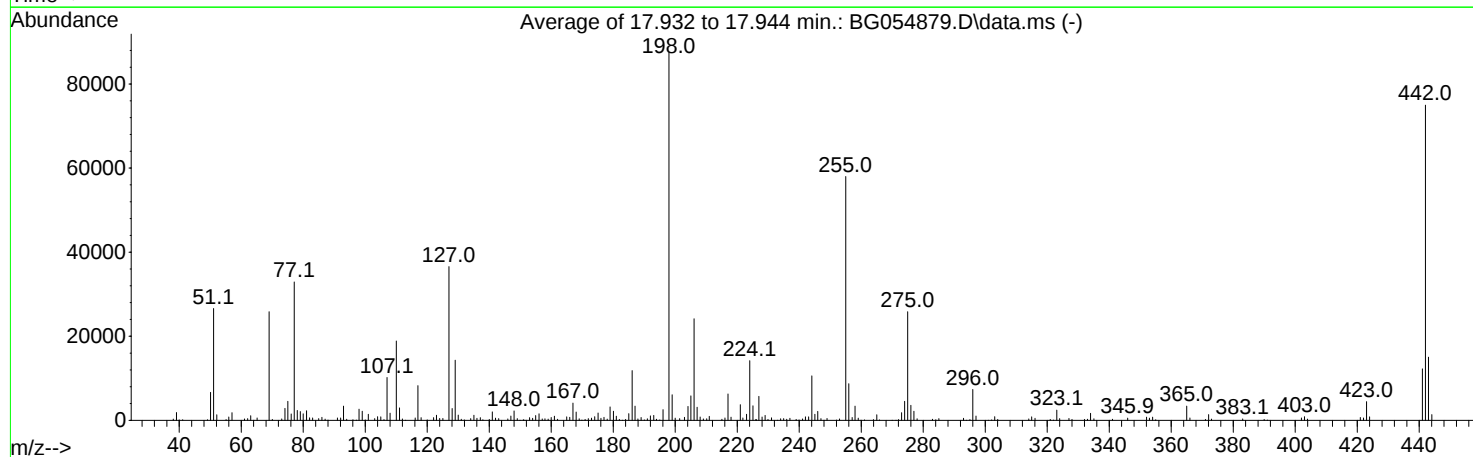


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090822\
 Data File : BG054879.D
 Acq On : 8 Sep 2022 9:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 09 02:45:21 2022

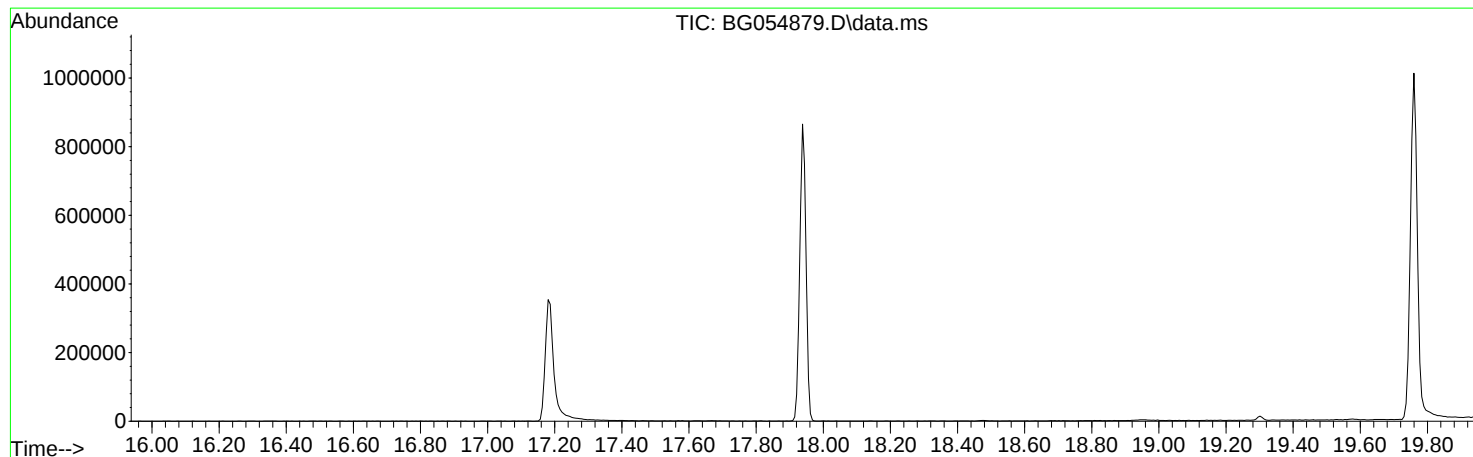

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	26608	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.5	25832	PASS
70	69	0.00	2	0.8	216	PASS
127	198	10	80	41.8	36568	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87491	PASS
199	198	5	9	7.0	6109	PASS
275	198	10	60	29.5	25829	PASS
365	198	1	100	3.9	3400	PASS
441	198	0.01	100	14.0	12239	PASS
442	442	50	100	100.0	74955	PASS
443	442	15	24	20.1	15036	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/8/2022	BNA_G	<u>BG054879.D</u>
Compound Name	Response	Retention Time
DDT	302994	20.988
DDD	8163	20.541
DDE	1135	20.036
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9298	312292	2.98

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090822\
Data File : BG054879.D
Acq On : 8 Sep 2022 9:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 09 03:54:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 02:45:21 2022
Response via : Initial Calibration

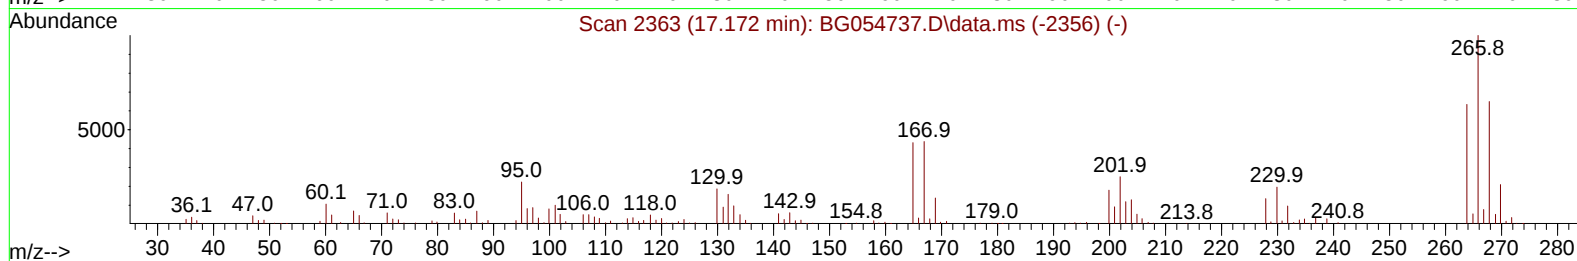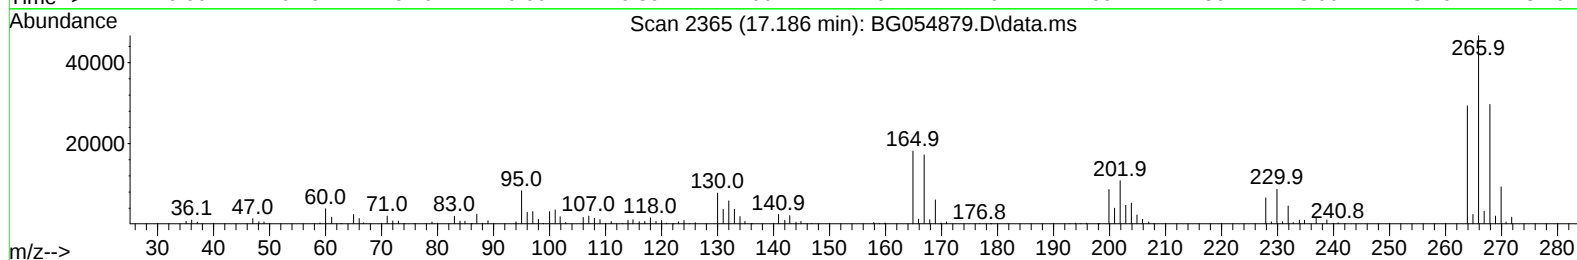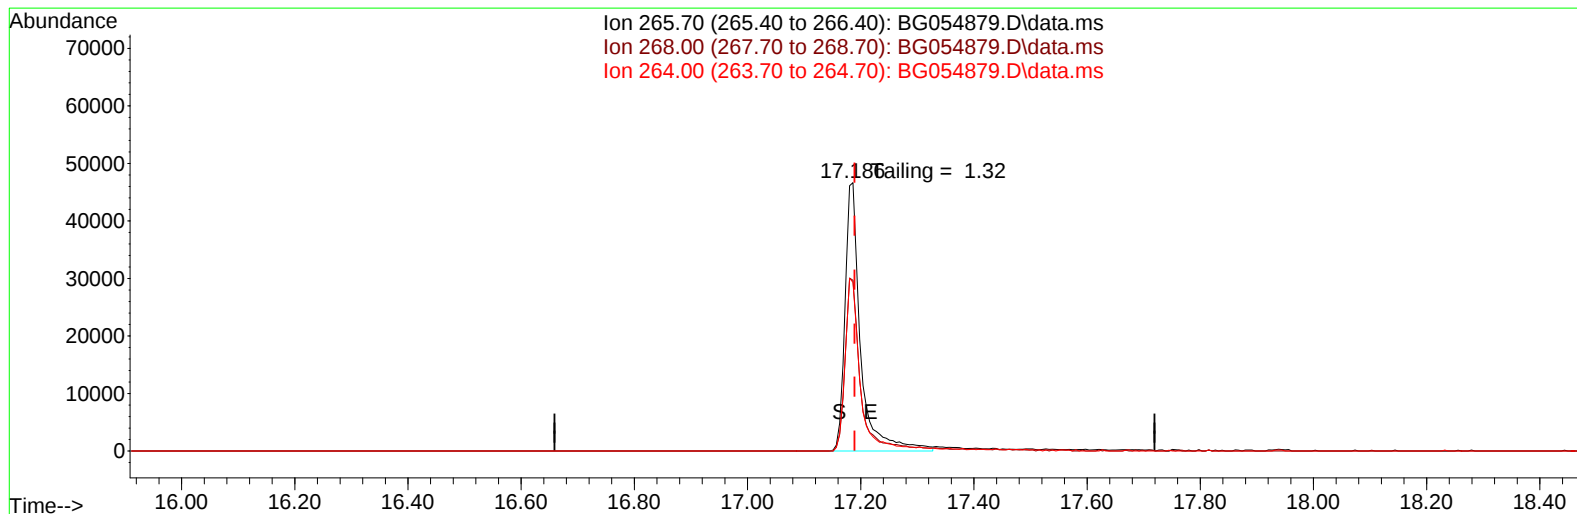

TIC: BG054879.D\data.ms

(70) Pentachlorophenol (C)

17.186min (-0.003) 32157.98 ng




response 89712

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.60
264.00	61.70	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090822\
Data File : BG054879.D
Acq On : 8 Sep 2022 9:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 09 03:54:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 02:45:21 2022
Response via : Initial Calibration

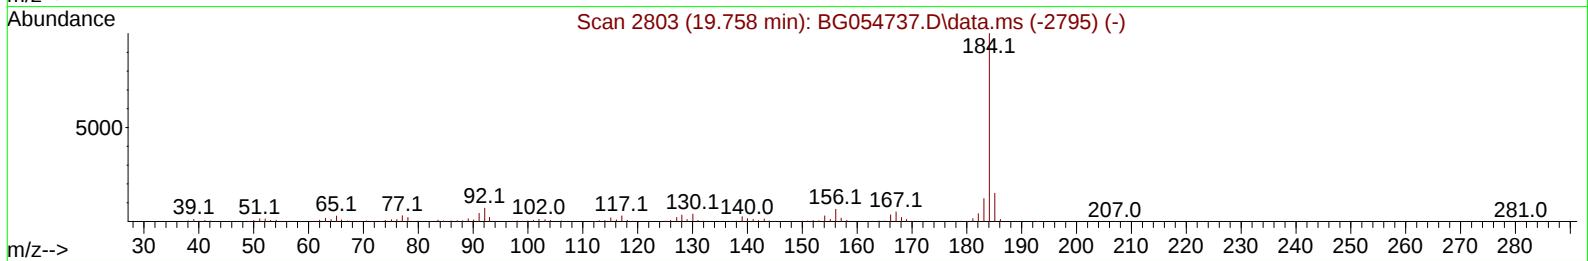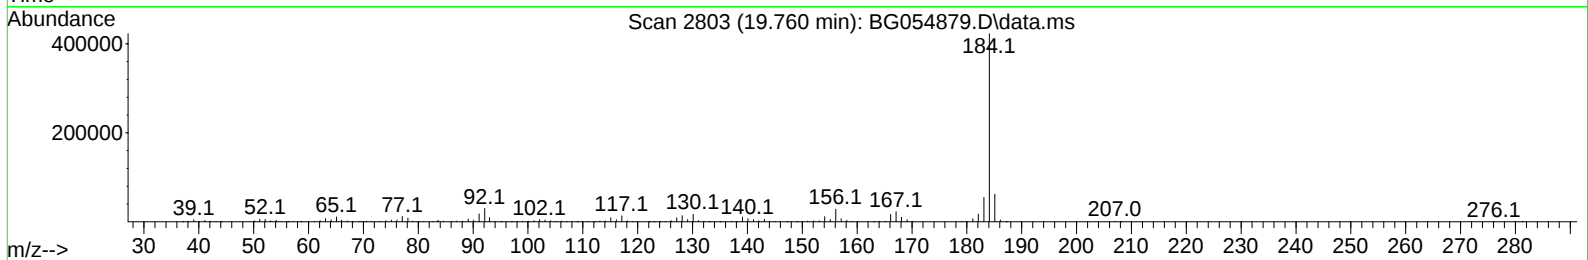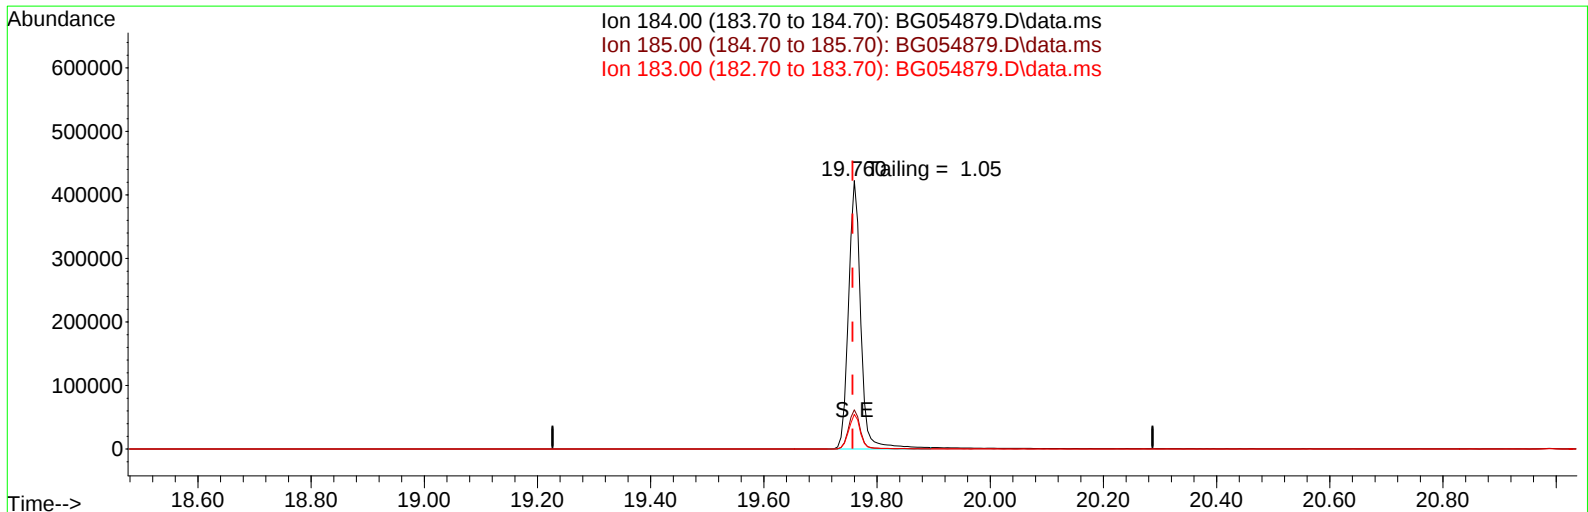

TIC: BG054879.D\data.ms

(77) Benzidine

19.760min (+ 0.003) 0.00 ng

response 644476

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.65
183.00	12.30	12.95
0.00	0.00	0.00