
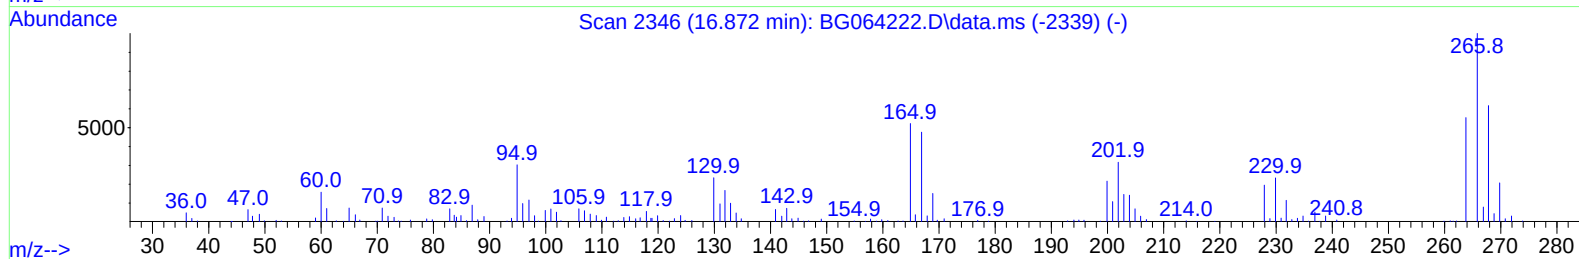
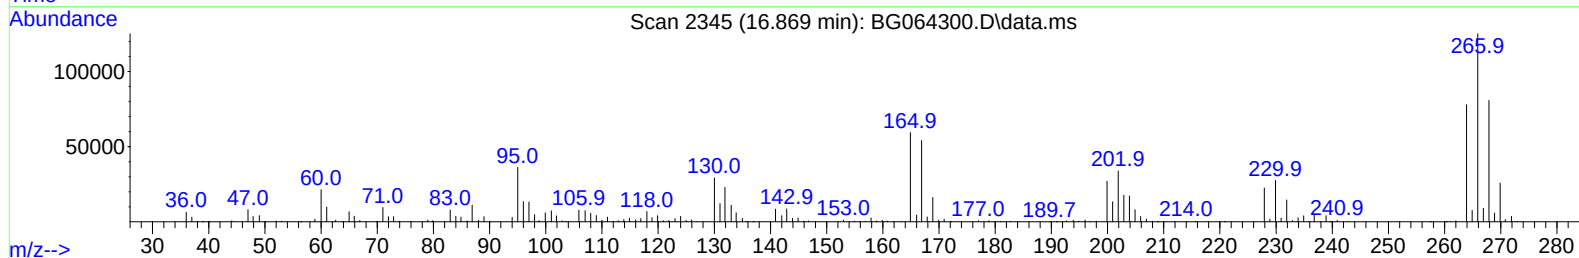


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090825\
Data File : BG064300.D
Acq On : 8 Sep 2025 9:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 09:42:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

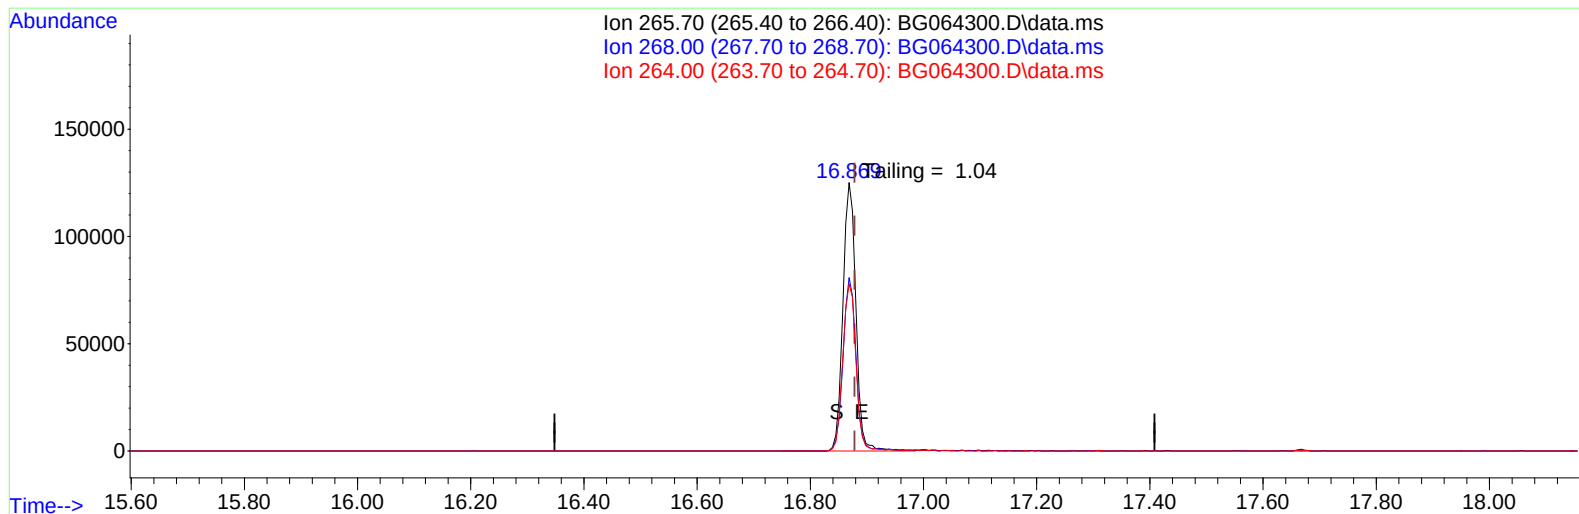

TIC: BG064300.D\data.ms

(70) Pentachlorophenol (C)




16.869min (-0.009) 433407.49 ng

response 198373

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.55
264.00	55.40	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090825\
Data File : BG064300.D
Acq On : 8 Sep 2025 9:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 09:42:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

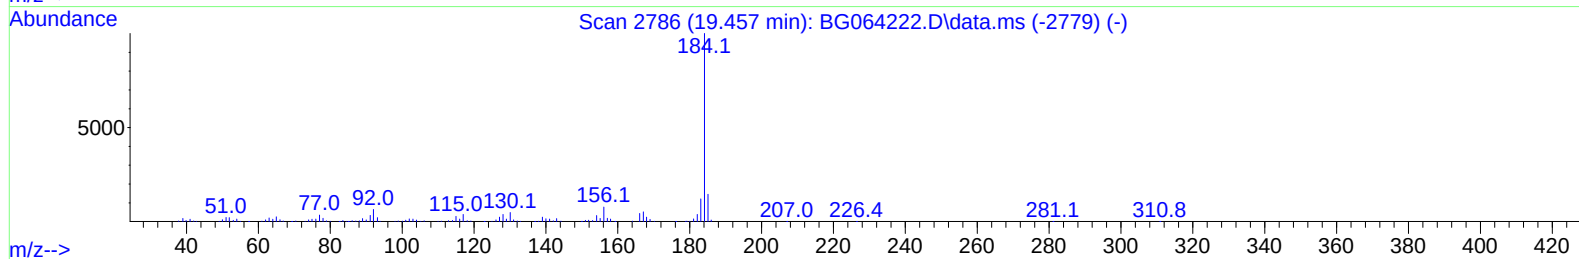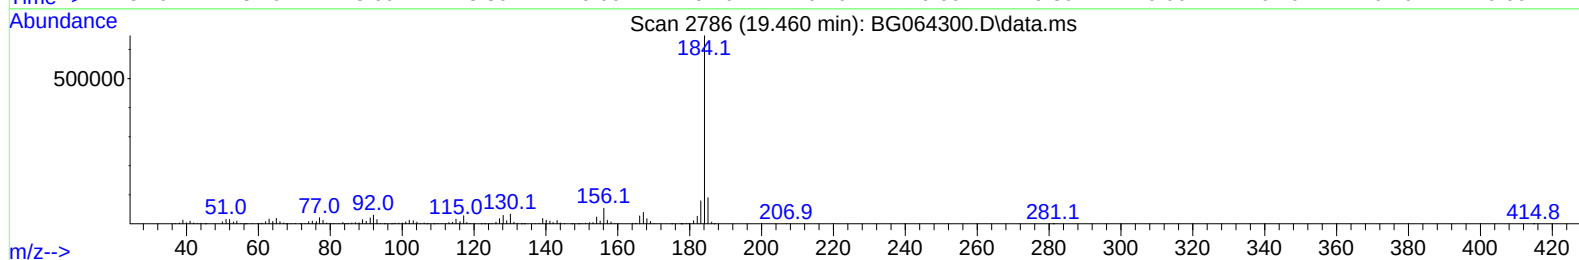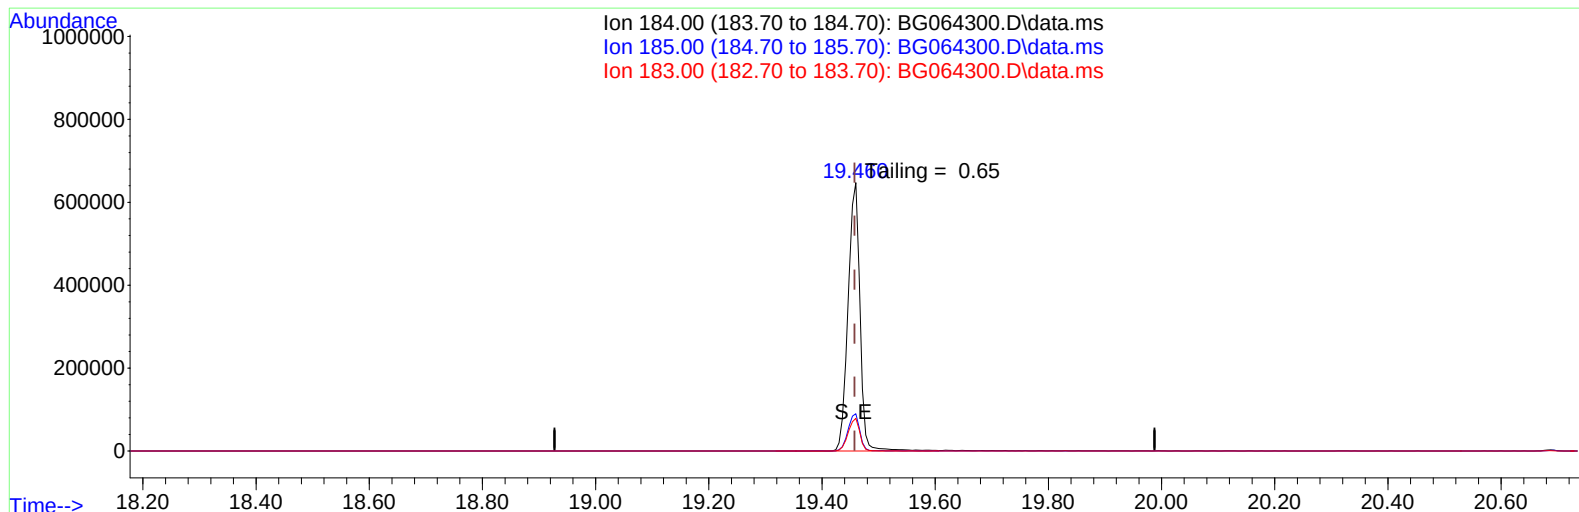

TIC: BG064300.D\data.ms

(77) Benzidine**19.460min (+ 0.002) 17072.46 ng****response 943114**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.94
183.00	12.10	12.20
0.00	0.00	0.00