


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090825\
Data File : BG064300.D
Acq On : 8 Sep 2025 9:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

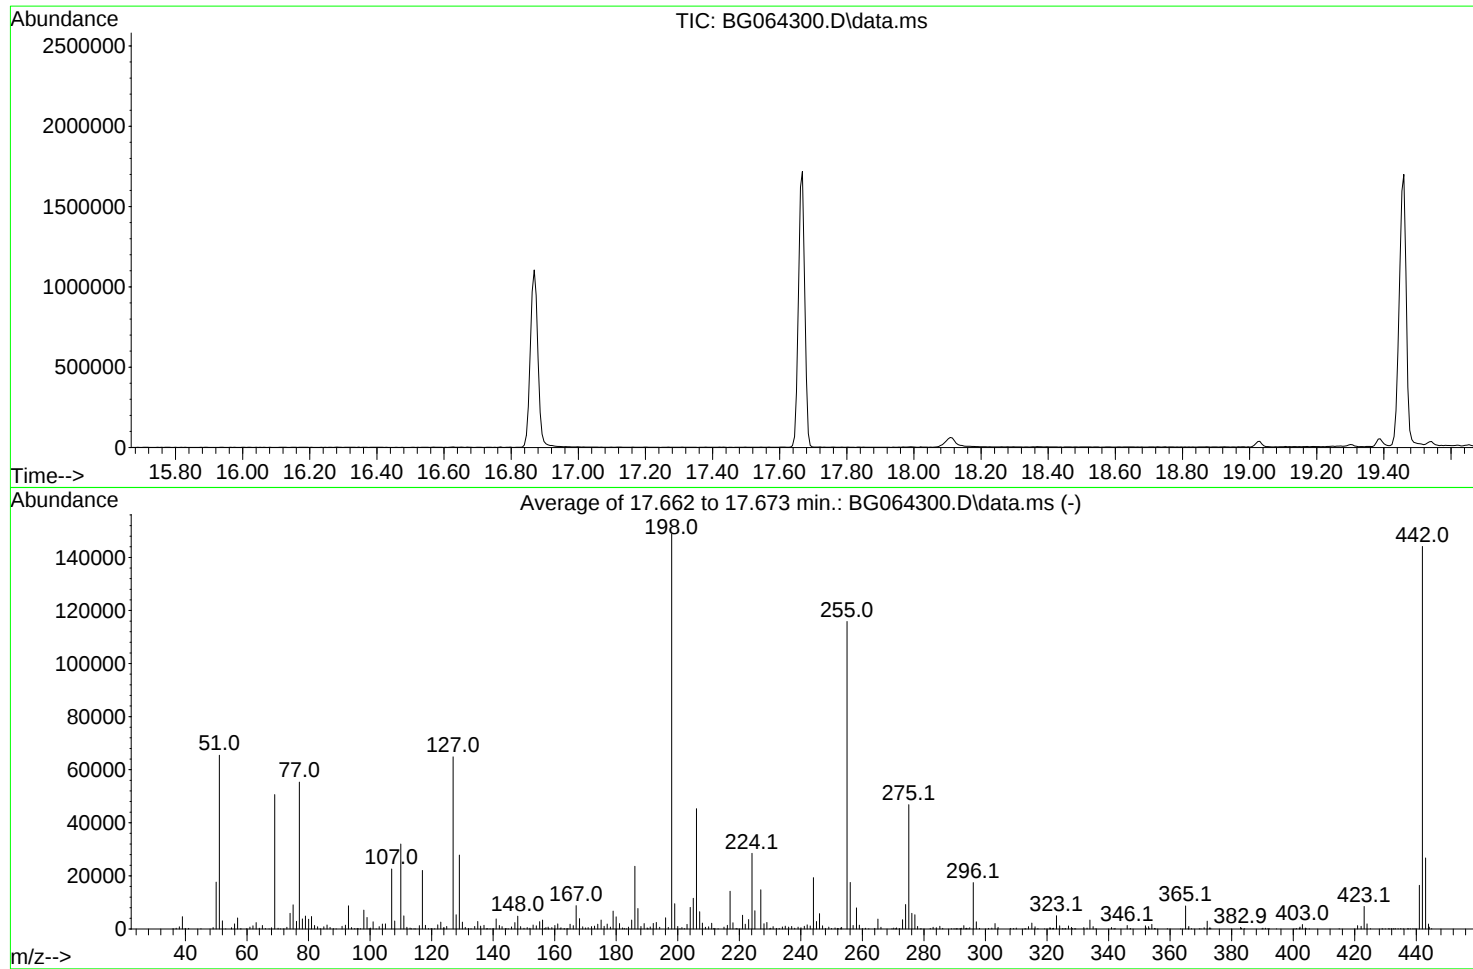




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2472

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.9	479	PASS
69	69	100	100	100.0	50621	PASS
70	69	0.00	2	0.6	288	PASS
197	198	0.00	2	0.4	554	PASS
198	198	100	100	100.0	148797	PASS
199	198	5	9	6.4	9499	PASS
365	198	1	100	5.8	8638	PASS
441	443	0.01	150	61.4	16440	PASS
442	442	100	100	100.0	144155	PASS
443	442	15	24	18.6	26757	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090825\
Data File : BG064300.D
Acq On : 8 Sep 2025 9:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 08 09:42:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

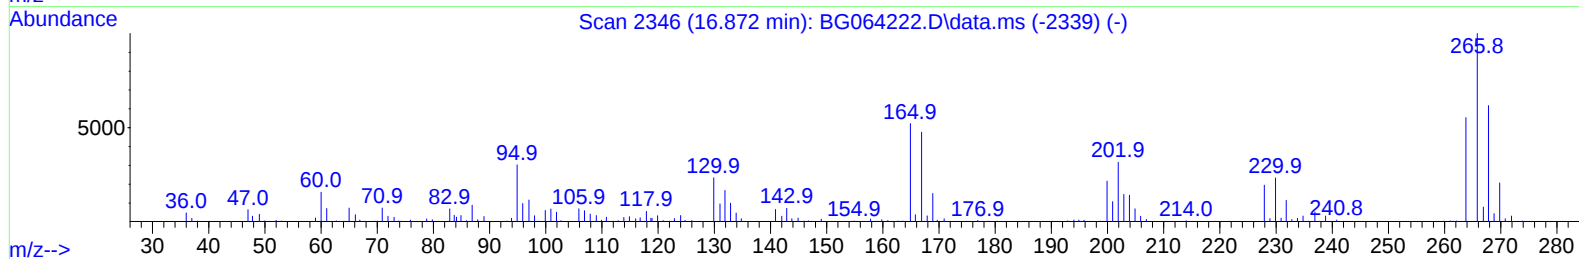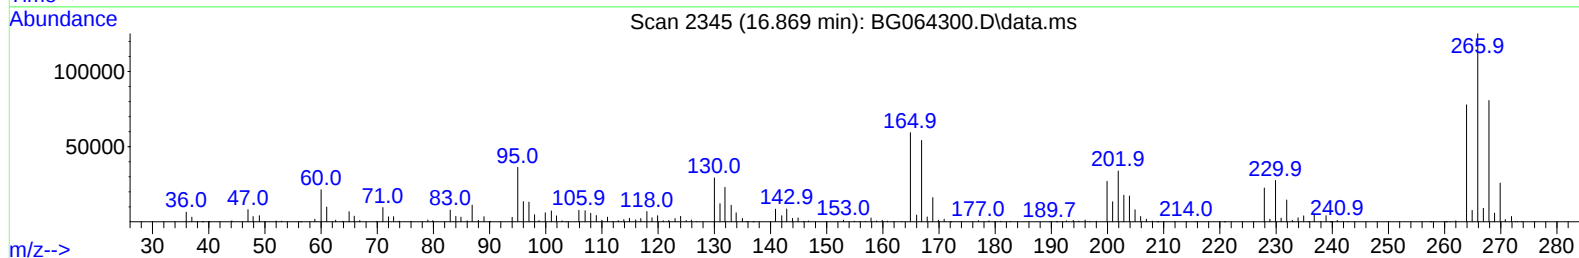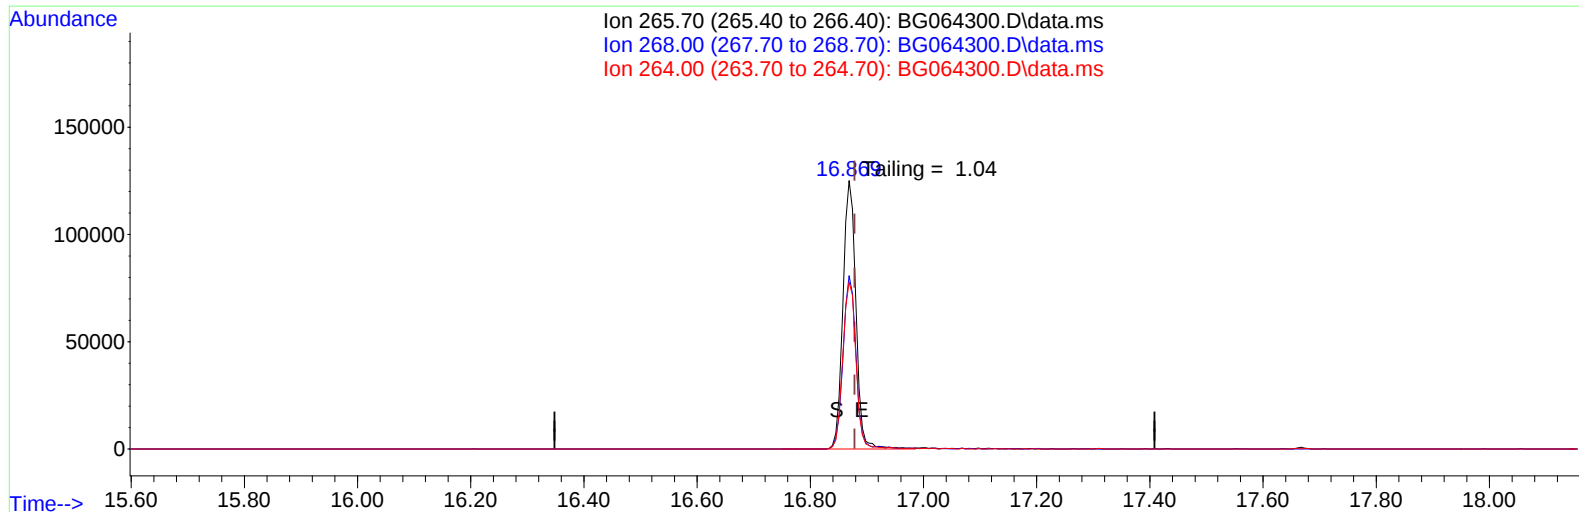

TIC: BG064300.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.009) 433407.49 ng




response 198373

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.55
264.00	55.40	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090825\
Data File : BG064300.D
Acq On : 8 Sep 2025 9:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 08 09:42:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

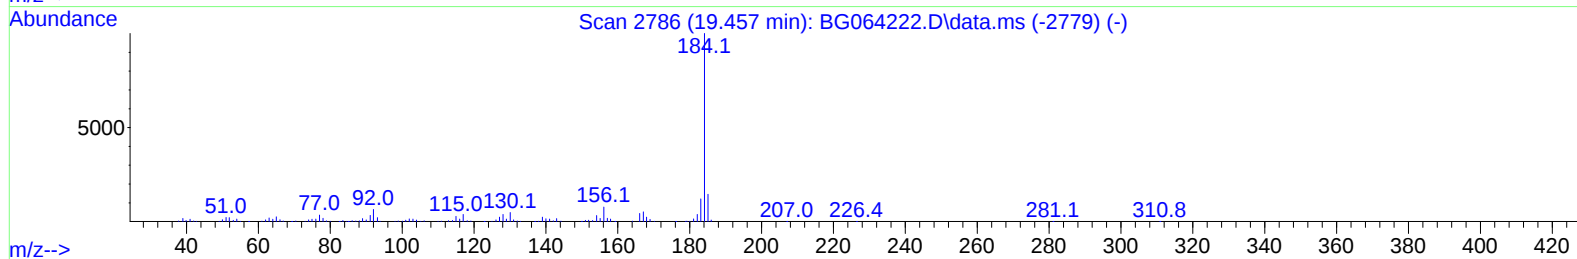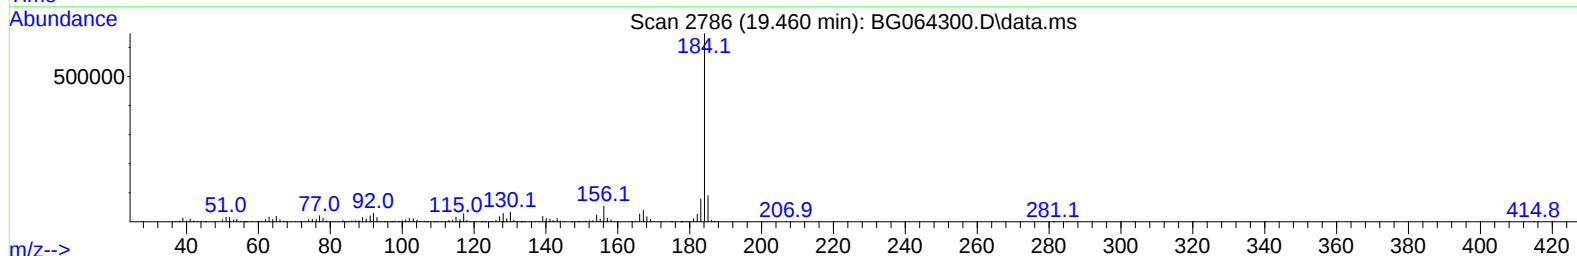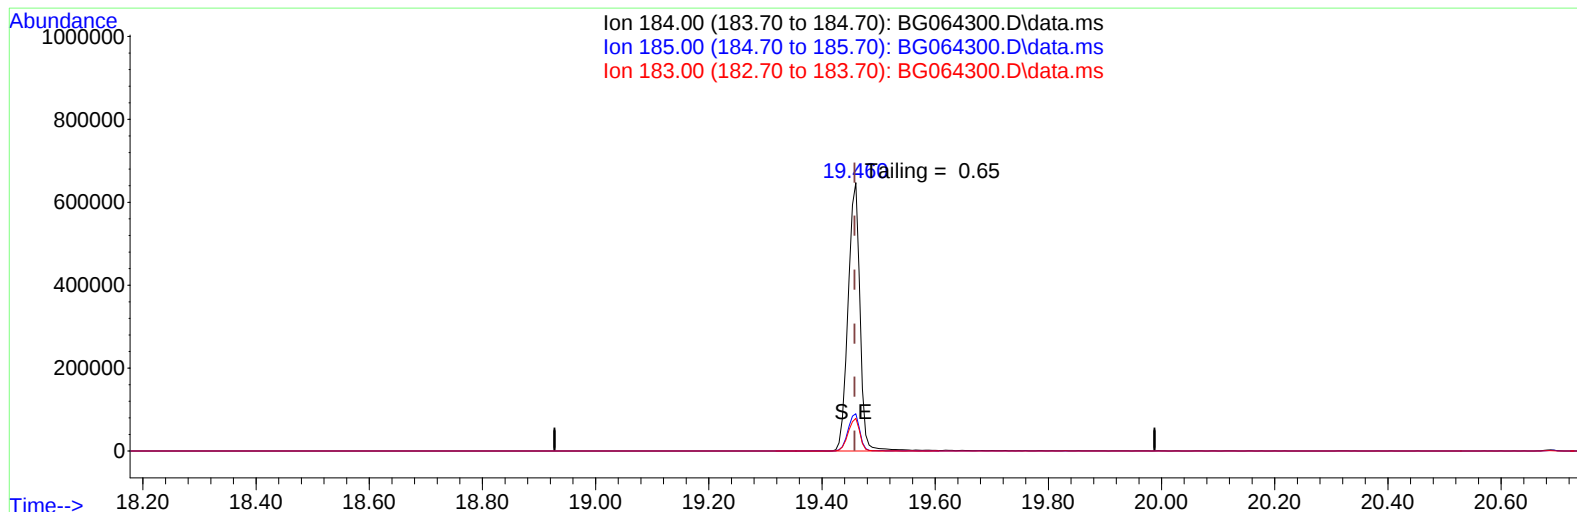

TIC: BG064300.D\data.ms

(77) Benzidine

19.460min (+ 0.002) 17072.46 ng

response 943114

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.94
183.00	12.10	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/8/2025	BNA_G	<u>BG064300.D</u>
Compound Name	Response	Retention Time
DDT	548799	20.688
DDD	7520	20.247
DDE	109	19.818
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7629	556428	1.37

Instrument :
BNA_G
ClientSampleId :
DFTPP