
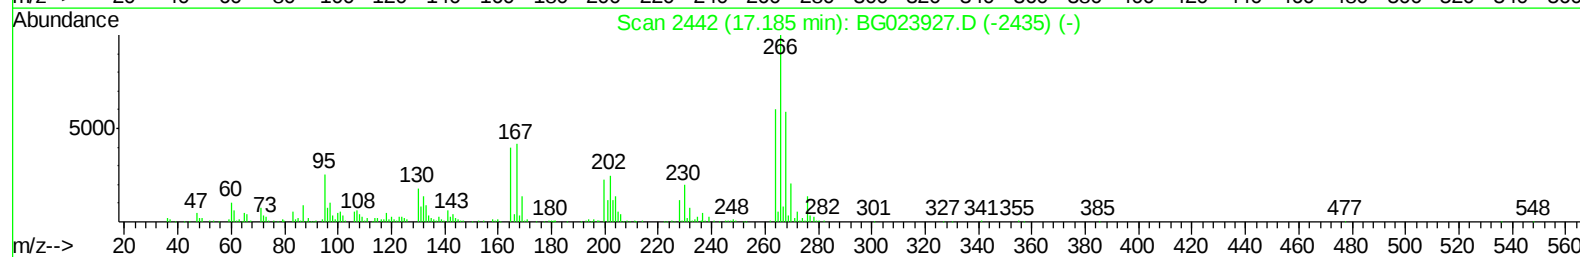
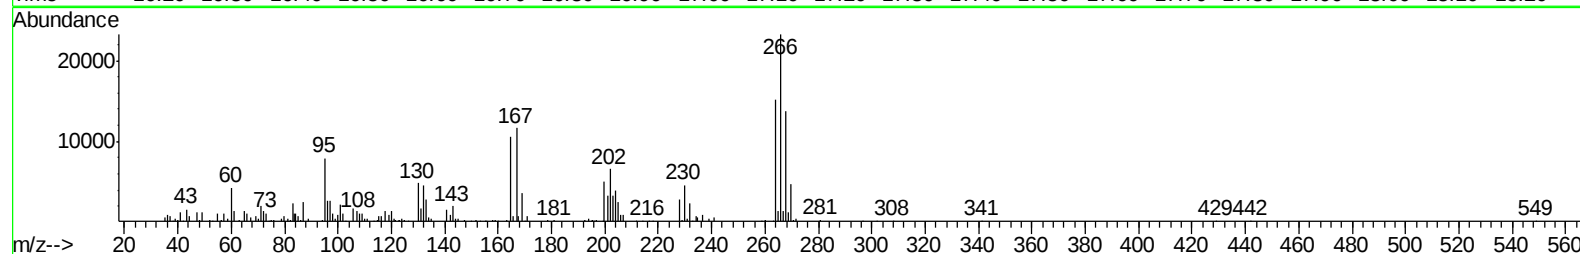


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090916\
Data File : BG023970.D
Acq On : 9 Sep 2016 9:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 01:50:11 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 16:24:09 2016
Response via : Initial Calibration

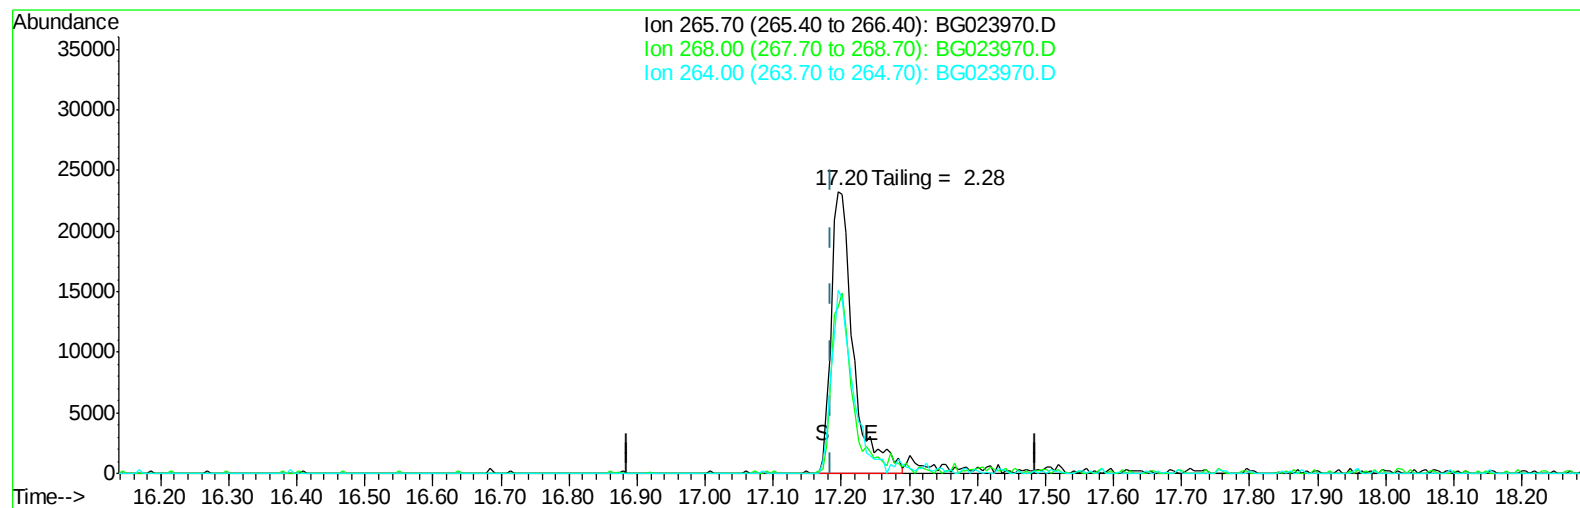

TIC: BG023970.D

(69) Pentachlorophenol (C)




17.196min (+0.010) 70512.16ng

response 52903

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	59.18
264.00	63.20	64.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090916\
Data File : BG023970.D
Acq On : 9 Sep 2016 9:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 01:50:11 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 16:24:09 2016
Response via : Initial Calibration

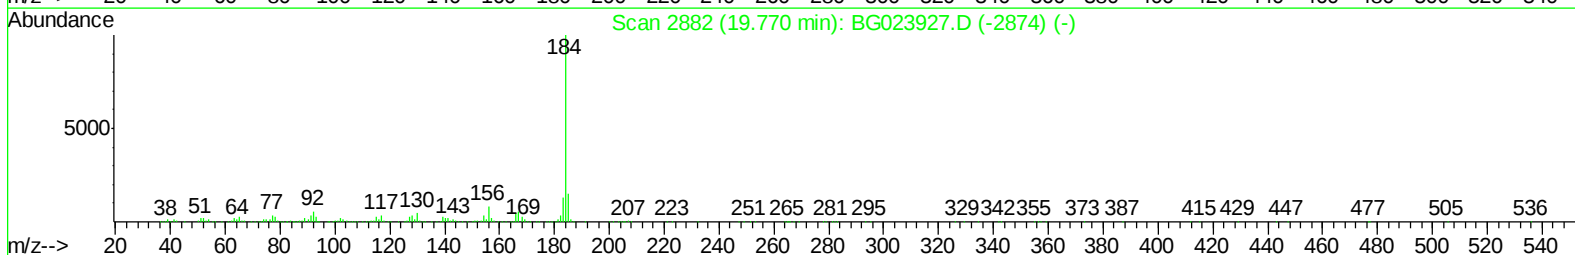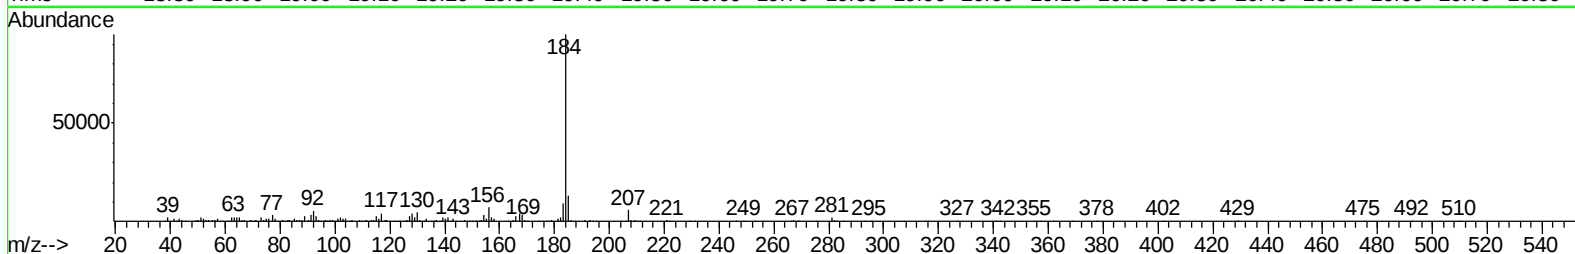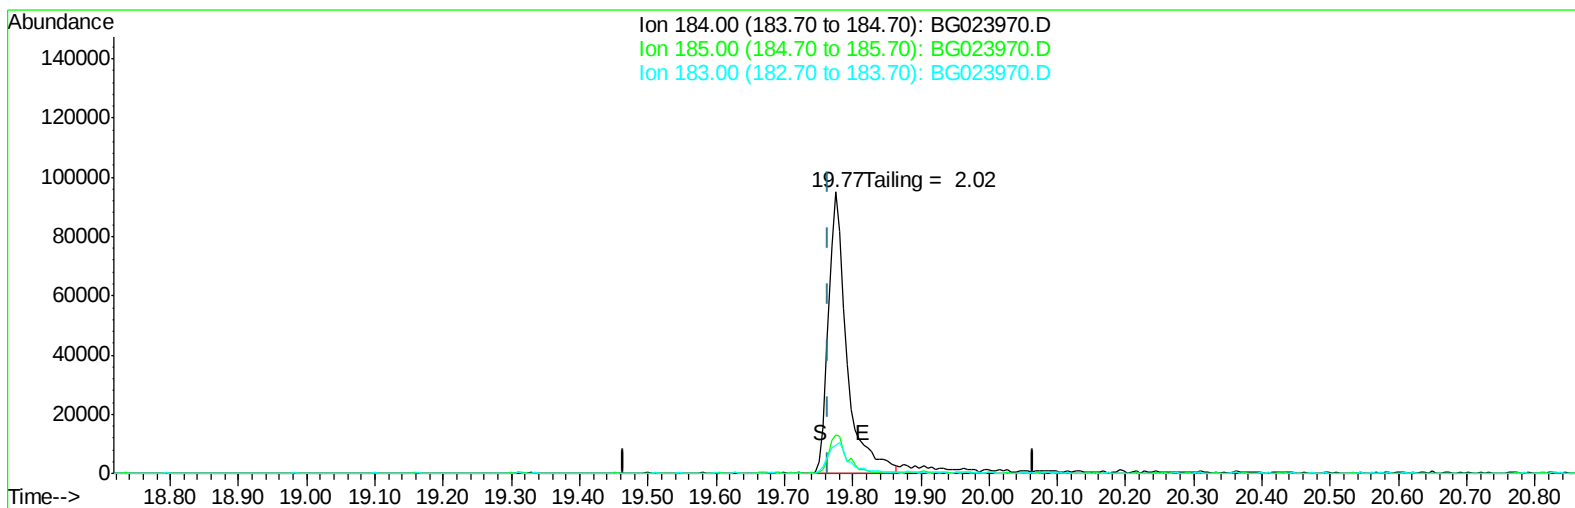

TIC: BG023970.D

(76) Benzidine

19.775min (+0.010) 47857.41ng

response 179315

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	13.58
183.00	13.40	10.08#
0.00	0.00	0.00