


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090920\
 Data File : BG046567.D
 Acq On : 9 Sep 2020 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 15:06:53 2020

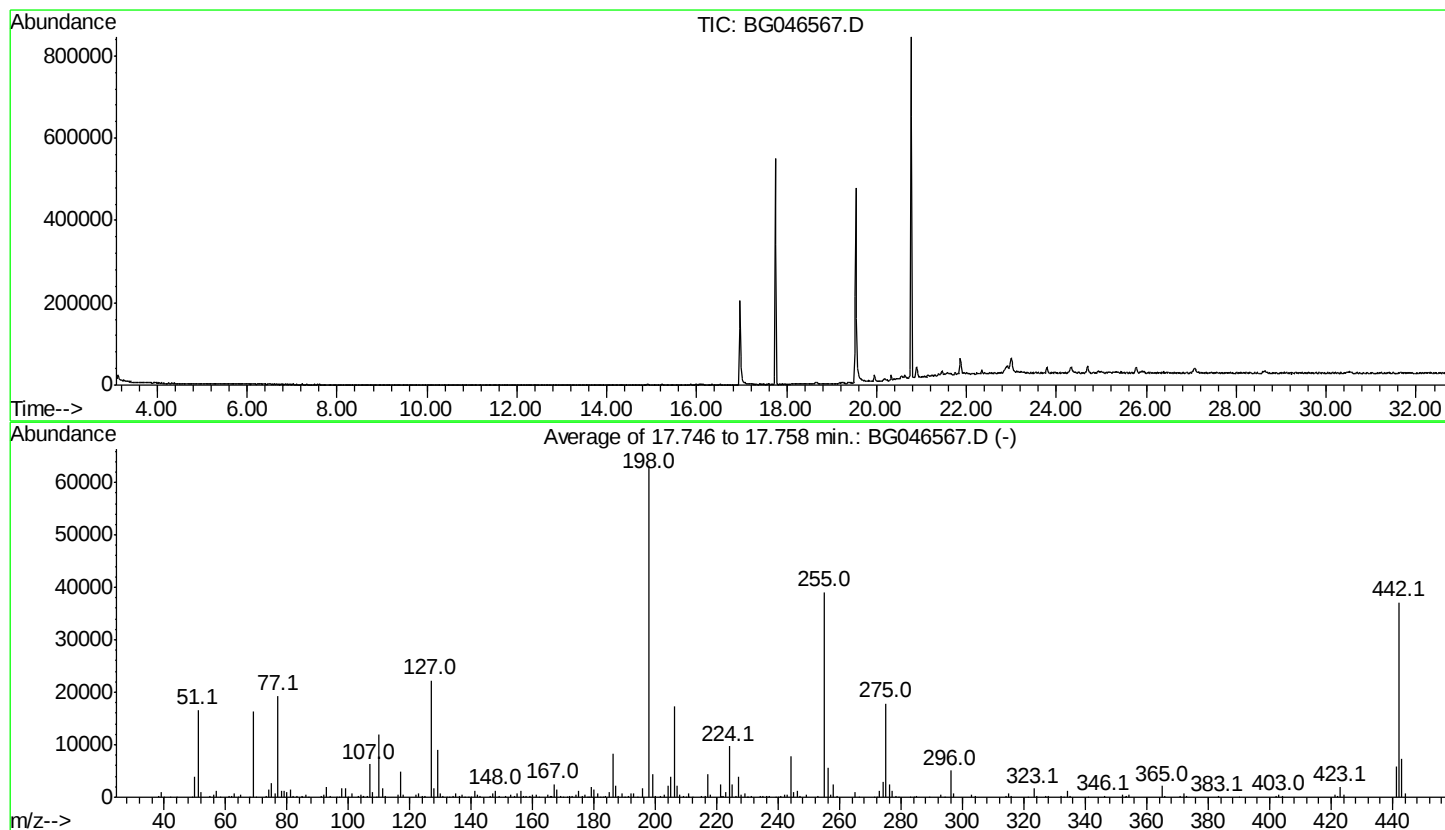

Spectrum Information: Average of 17.746 to 17.758 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	16714	PASS
68	69	0.00	2	0.6	99	PASS
69	198	0.00	100	25.7	16242	PASS
70	69	0.00	2	0.3	52	PASS
127	198	10	80	35.2	22265	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63205	PASS
199	198	5	9	7.0	4452	PASS
275	198	10	60	28.3	17869	PASS
365	198	1	100	3.3	2098	PASS
441	198	0.01	100	9.4	5961	PASS
442	198	50	100	58.7	37128	PASS
443	442	15	24	19.8	7349	PASS