

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090924\
 Data File : BG062692.D
 Acq On : 9 Sep 2024 17:04
 Operator : JU/RC
 Sample : SST08056
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST080442

Quant Time: Sep 10 00:52:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 00:41:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	65336	20.000	ng/u1	0.00
20) Naphthalene-d8	10.702	136	300125	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.533	164	243065	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.282	188	606911	20.000	ng/u1	0.00
79) Chrysene-d12	21.530	240	617639	20.000	ng/u1	0.00
88) Perylene-d12	24.597	264	665469	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.446	96	239	0.165	ng/uL	0.08
4) Pyridine-d5	3.769	84	382305	83.095	ng/u1	0.00
7) Phenol-d5	7.077	99	477073	83.271	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.241	67	276321	80.445	ng/u1	0.00
11) 2-Chlorophenol-d4	7.441	132	353937	84.813	ng/u1	0.00
15) 4-Methylphenol-d8	8.622	113	398943	83.560	ng/u1	0.01
21) Nitrobenzene-d5	9.063	128	184222	85.883	ng/u1	0.00
24) 2-Nitrophenol-d4	9.785	143	208929	89.061	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.326	165	427868	83.750	ng/u1	0.00
31) 4-Chloroaniline-d4	10.837	131	572186	81.479	ng/u1	0.00
46) Dimethylphthalate-d6	13.945	166	1438519	76.854	ng/u1	0.00
49) Acenaphthylene-d8	14.233	160	1642867	79.029	ng/u1	0.00
54) 4-Nitrophenol-d4	14.750	143	259369	81.570	ng/u1	0.02
60) Fluorene-d10	15.532	176	1287765	76.348	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.655	200	304666	87.270	ng/u1	0.01
73) Anthracene-d10	17.382	188	2215637	77.355	ng/u1	0.00
81) Pyrene-d10	19.674	212	2646575	76.147	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.398	264	2862344	81.458	ng/u1	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.399	88	51005	31.486	ng/uL	93
5) Pyridine	3.787	79	396197	82.103	ng/u1	97
6) Benzaldehyde	7.047	77	205183	65.733	ng/u1	97
8) Phenol	7.106	94	489785	82.240	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.329	93	359443	79.839	ng/u1	96
12) 2-Chlorophenol	7.476	128	365847	85.740	ng/u1	97
13) 2-Methylphenol	8.352	108	370737	83.015	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.428	45	651873	80.444	ng/u1	100
16) Acetophenone	8.728	105	631125	81.335	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.728	70	345747	85.116	ng/u1	97
18) 4-Methylphenol	8.687	108	415303	82.658	ng/u1	95
19) Hexachloroethane	8.986	117	139896	81.443	ng/u1	96
22) Nitrobenzene	9.110	77	484100	83.425	ng/u1	94
23) Isophorone	9.639	82	977994	82.435	ng/u1	100
25) 2-Nitrophenol	9.821	139	223512	86.446	ng/u1	96
26) 2,4-Dimethylphenol	9.879	107	462270	83.671	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.114	93	532420	80.301	ng/u1	96
29) 2,4-Dichlorophenol	10.355	162	420862	83.639	ng/u1	97
30) Naphthalene	10.755	128	1261784	78.410	ng/u1	99
32) 4-Chloroaniline	10.861	127	574885	82.313	ng/u1	100
33) Hexachlorobutadiene	11.043	225	332908	79.418	ng/u1	94
34) Caprolactam	11.636	113	81139	44.110	ng/u1	91
35) 4-Chloro-3-methylphenol	11.989	107	459589	83.728	ng/u1	95
36) 2-Methylnaphthalene	12.359	142	949599	79.955	ng/u1	96


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090924\
 Data File : BG062692.D
 Acq On : 9 Sep 2024 17:04
 Operator : JU/RC
 Sample : SSTD08056
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD080442

Quant Time: Sep 10 00:52:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 00:41:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.582	142	964836	79.308	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.729	216	660702	79.067	ng/ul	98
40) Hexachlorocyclopentadiene	12.711	237	356068	83.277	ng/ul	94
41) 2,4,6-Trichlorophenol	12.970	196	419499	82.881	ng/ul	97
42) 2,4,5-Trichlorophenol	13.046	196	458624	84.393	ng/ul	95
43) 1,1'-Biphenyl	13.369	154	1327014	77.637	ng/ul	99
44) 2-Chloronaphthalene	13.416	162	1094069	78.716	ng/ul	99
45) 2-Nitroaniline	13.616	65	336601	88.256	ng/ul	98
47) Dimethylphthalate	13.998	163	1479904	76.773	ng/ul	99
48) 2,6-Dinitrotoluene	14.116	165	299517	88.196	ng/ul	95
50) Acenaphthylene	14.262	152	1679933	76.544	ng/ul	98
51) 3-Nitroaniline	14.445	138	259010	76.178	ng/ul	97
52) Acenaphthene	14.603	153	1202096	77.325	ng/ul	97
53) 2,4-Dinitrophenol	14.650	184	201263	89.749	ng/ul	99
55) 4-Nitrophenol	14.762	109	235218	82.296	ng/ul	96
56) Dibenzofuran	14.938	168	1752974	75.905	ng/ul	100
57) 2,4-Dinitrotoluene	14.903	165	461391	86.897	ng/ul#	100
58) 2,3,4,6-Tetrachlorophenol	15.167	232	454900	82.601	ng/ul	98
59) Diethylphthalate	15.361	149	1451169	76.312	ng/ul	99
61) Fluorene	15.590	166	1342918	74.022	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.579	204	794966	74.702	ng/ul	96
63) 4-Nitroaniline	15.614	138	270680	73.981	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.673	198	312934	86.475	ng/ul#	97
67) N-Nitrosodiphenylamine	15.796	169	1240111	79.673	ng/ul	99
68) 4-Bromophenyl-phenylether	16.472	248	556848	79.734	ng/ul	99
69) Hexachlorobenzene	16.595	284	630280	79.043	ng/ul	99
70) Atrazine	16.748	200	559139	80.656	ng/ul	97
71) Pentachlorophenol	16.936	266	412607	86.511	ng/ul	98
72) Phenanthrene	17.329	178	2367933	75.027	ng/ul	97
74) Anthracene	17.418	178	2416953	75.118	ng/ul	96
75) 1,2,3,4-Tetrachloroben...	13.334	216	688121	83.025	ng/ul	100
76) Pentachlorobenzene	14.862	250	738650	80.424	ng/ul	98
77) Carbazole	17.688	167	2081907	78.027	ng/ul	97
78) Di-n-butylphthalate	18.246	149	2388790	75.702	ng/ul	97
80) Fluoranthene	19.339	202	2861392	74.334	ng/ul#	96
82) Pyrene	19.703	202	2977359	71.854	ng/ul#	95
83) Butylbenzylphthalate	20.590	149	1059183	86.108	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.431	252	975129	74.990	ng/ul	100
85) Benzo(a)anthracene	21.513	228	3218186	74.916	ng/ul	93
86) Bis(2-ethylhexyl)phtha...	21.431	149	1489030	82.211	ng/ul	98
87) Chrysene	21.577	228	3036918	74.519	ng/ul	92
89) Di-n-octyl phthalate	22.588	149	2598020	83.931	ng/ul	100
90) Benzo(b)fluoranthene	23.634	252	3308197	80.518	ng/ul	97
91) Benzo(k)fluoranthene	23.698	252	3288814	78.174	ng/ul	96
93) Benzo(a)pyrene	24.468	252	3102286	80.053	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	28.070	276	3969549	83.137	ng/ul	98
95) Dibenzo(a,h)anthracene	28.134	278	3188093	83.127	ng/ul	98
96) Benzo(g,h,i)perylene	29.163	276	3045796	82.594	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 31.486 ng/uL
RT: 3.399 min Scan# 51
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion: 88 Resp: 51005
Ion Ratio Lower Upper
88 100
43 29.6 23.1 34.7
58 79.4 57.2 85.8



#5
Pyridine
Concen: 82.103 ng/uL
RT: 3.787 min Scan# 119
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion: 79 Resp: 396197
Ion Ratio Lower Upper
79 100
52 90.1 69.8 104.8
51 41.1 34.0 51.0









#6
Benzaldehyde
Concen: 65.733 ng/ul
RT: 7.047 min Scan# 611
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion: 77 Resp: 205183
Ion Ratio Lower Upper
77 100
105 93.2 79.0 118.4
106 87.2 69.0 103.6

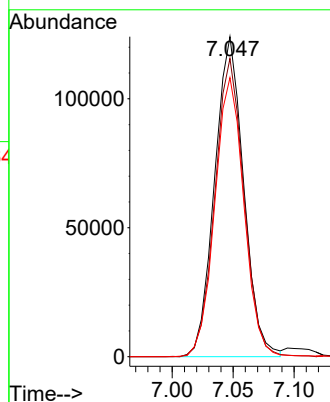

#8
Phenol
Concen: 82.240 ng/ul
RT: 7.106 min Scan# 684
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion: 94 Resp: 489785
Ion Ratio Lower Upper
94 100
65 30.5 25.1 37.7
66 40.0 30.8 46.2









#10
 Bis(2-Chloroethyl)ether
 Concen: 79.839 ng/ul
 RT: 7.329 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BG062692.D
 Acq: 9 Sep 2024 17:04

Instrument :
 BNA_G
 ClientSampleId :
 SST080442

Tgt Ion: 93 Resp: 359443




Ion	Ratio	Lower	Upper
93	100		
63	82.4	62.0	93.0
95	32.3	25.9	38.9




#12
 2-Chlorophenol
 Concen: 85.740 ng/ul
 RT: 7.476 min Scan# 747
 Delta R.T. 0.006 min
 Lab File: BG062692.D
 Acq: 9 Sep 2024 17:04

Tgt Ion:128 Resp: 365847

Ion	Ratio	Lower	Upper
128	100		
64	50.7	42.0	63.0
130	31.7	24.0	36.0





#13

2-Methylphenol

Concen: 83.015 ng/ul

RT: 8.352 min Scan# 895

Delta R.T. 0.006 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :





SSTD080442

Tgt Ion:108 Resp: 370737

Ion Ratio Lower Upper

108 100

107 90.7 72.1 108.1

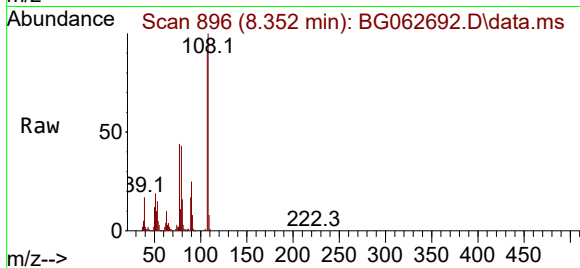

#14

2,2'-oxybis(1-Chloropropane)

Concen: 80.444 ng/ul

RT: 8.428 min Scan# 909

Delta R.T. 0.006 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04




Tgt Ion: 45 Resp: 651873


Ion Ratio Lower Upper

45 100

77 11.3 9.0 13.6

79 8.5 6.6 9.8




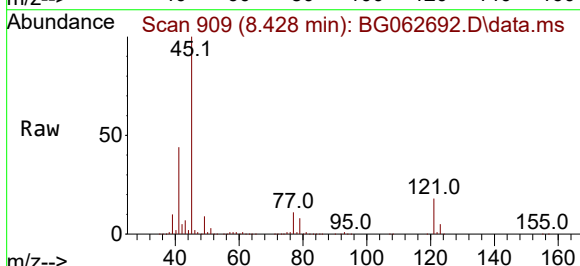




#16
Acetophenone
Concen: 81.335 ng/ul
RT: 8.728 min Scan# 90
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:105 Resp: 631125
Ion Ratio Lower Upper
105 100
77 80.0 63.3 94.9
51 31.2 26.5 39.7

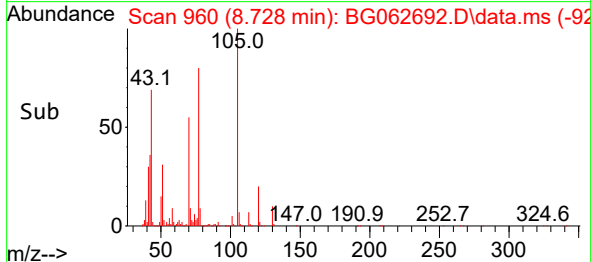

#17
N-Nitroso-di-n-propylamine
Concen: 85.116 ng/ul
RT: 8.728 min Scan# 960
Delta R.T. 0.018 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion: 70 Resp: 345747
Ion Ratio Lower Upper
70 100
42 65.7 50.2 75.2
101 9.0 6.2 9.4
130 18.7 15.1 22.7


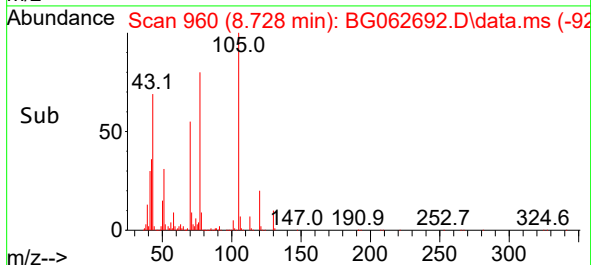
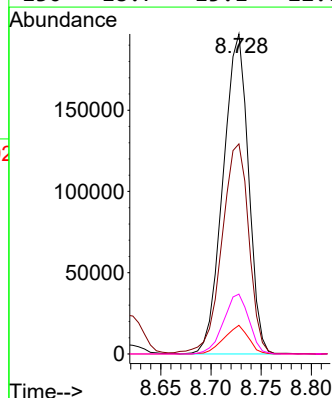





#18
4-Methylphenol
Concen: 82.658 ng/ul
RT: 8.687 min Scan# 91
Delta R.T. 0.012 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:108 Resp: 415303
Ion Ratio Lower Upper
108 100
107 113.2 86.4 129.6

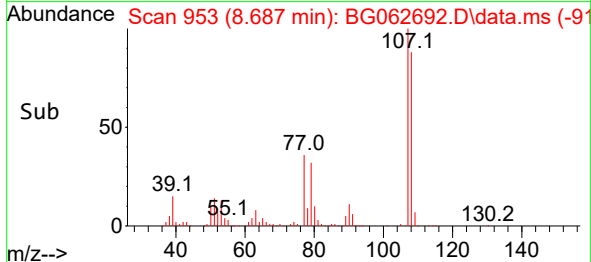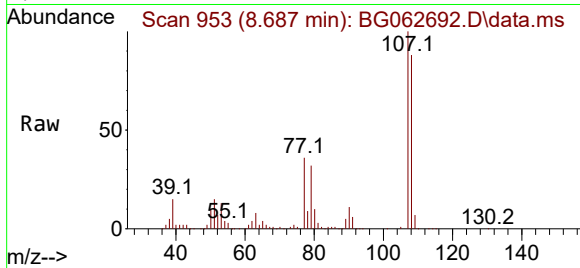

#19
Hexachloroethane
Concen: 81.443 ng/ul
RT: 8.986 min Scan# 1004
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:117 Resp: 139896
Ion Ratio Lower Upper
117 100
201 134.4 106.6 160.0
199 85.8 62.0 93.0




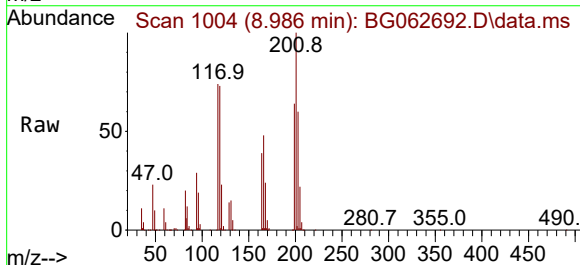




#22
Nitrobenzene
Concen: 83.425 ng/ul
RT: 9.110 min Scan# 1024
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion: 77 Resp: 484100
Ion Ratio Lower Upper
77 100
123 42.3 30.9 46.3
65 13.8 9.7 14.5

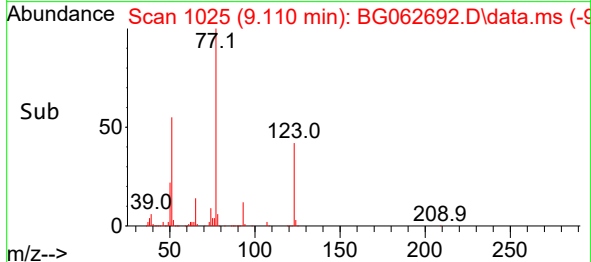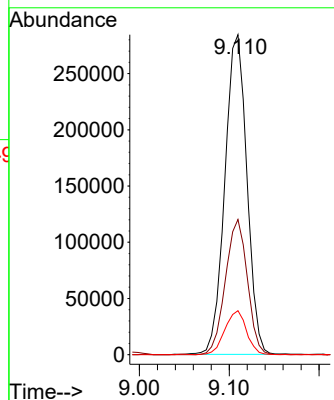

#23
Isophorone
Concen: 82.435 ng/ul
RT: 9.639 min Scan# 1115
Delta R.T. 0.018 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion: 82 Resp: 977994
Ion Ratio Lower Upper
82 100
95 6.9 5.8 8.8
138 16.3 13.0 19.6



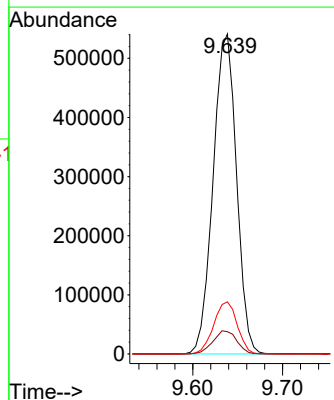





#25
2-Nitrophenol
Concen: 86.446 ng/ul
RT: 9.821 min Scan# 1145
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:139 Resp: 223512
Ion Ratio Lower Upper
139 100
65 54.6 45.4 68.0
109 33.8 23.9 35.9

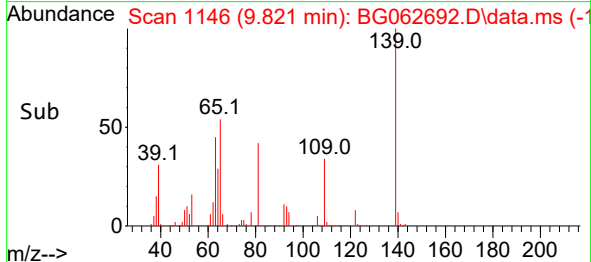

#26
2,4-Dimethylphenol
Concen: 83.671 ng/ul
RT: 9.879 min Scan# 1156
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:107 Resp: 462270
Ion Ratio Lower Upper
107 100
121 48.1 38.8 58.2
122 85.6 70.5 105.7




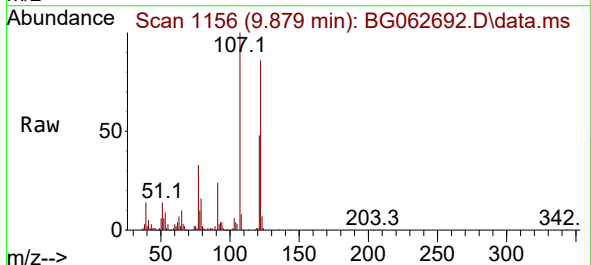




#27
 Bis(2-Chloroethoxy)methane
 Concen: 80.301 ng/ul
 RT: 10.114 min Scan# 1196
 Delta R.T. 0.006 min
 Lab File: BG062692.D
 Acq: 9 Sep 2024 17:04




Instrument :
 BNA_G
 ClientSampleId :
 SSTD080442


Tgt Ion: 93 Resp: 532420
 Ion Ratio Lower Upper
 93 100
 95 31.9 27.4 41.2
 123 9.8 9.1 13.7

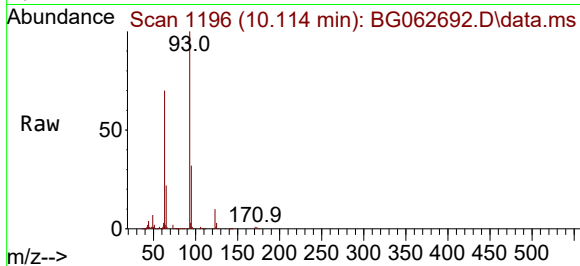

#29
 2,4-Dichlorophenol
 Concen: 83.639 ng/ul
 RT: 10.355 min Scan# 1237
 Delta R.T. 0.012 min
 Lab File: BG062692.D
 Acq: 9 Sep 2024 17:04

Tgt Ion:162 Resp: 420862
 Ion Ratio Lower Upper
 162 100
 164 65.4 51.9 77.9
 98 33.4 23.8 35.6




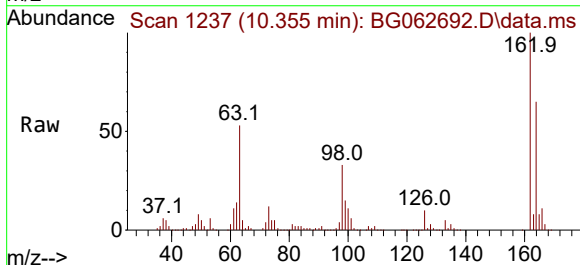




#30
Naphthalene
Concen: 78.410 ng/ul
RT: 10.755 min Scan# 11
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:128 Resp: 1261784
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.6
127 13.8 10.7 16.1



#32
4-Chloroaniline
Concen: 82.313 ng/ul
RT: 10.861 min Scan# 1323
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:127 Resp: 574885
Ion Ratio Lower Upper
127 100
129 32.3 25.8 38.8





#33

Hexachlorobutadiene

Concen: 79.418 ng/ul

RT: 11.043 min Scan# 11

Delta R.T. 0.006 min

Lab File: BG062692.D


Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :

SSTD080442






Tgt Ion:225 Resp: 332908

Ion Ratio Lower Upper

225 100

223 60.6 52.3 78.5

227 65.3 56.4 84.6

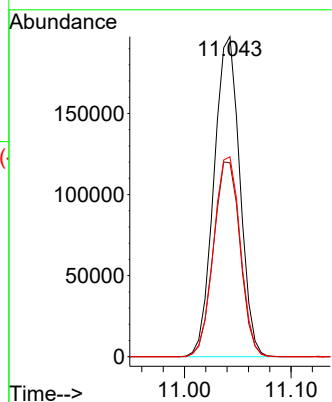

#34

Caprolactam

Concen: 44.110 ng/ul

RT: 11.636 min Scan# 1455

Delta R.T. 0.035 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04




Tgt Ion:113 Resp: 81139


Ion Ratio Lower Upper

113 100

55 213.0 150.8 226.2

56 155.5 125.0 187.6


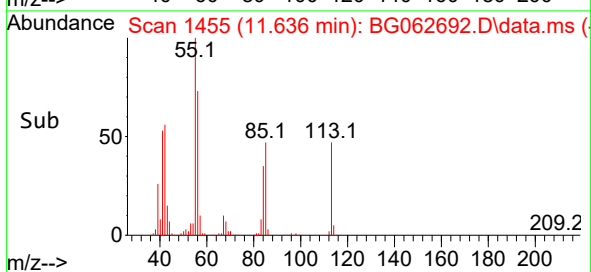






#35
4-Chloro-3-methylphenol
Concen: 83.728 ng/ul
RT: 11.989 min Scan# 11
Delta R.T. 0.012 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:107 Resp: 459589
Ion Ratio Lower Upper
107 100
144 24.5 21.8 32.6
142 76.8 64.8 97.2

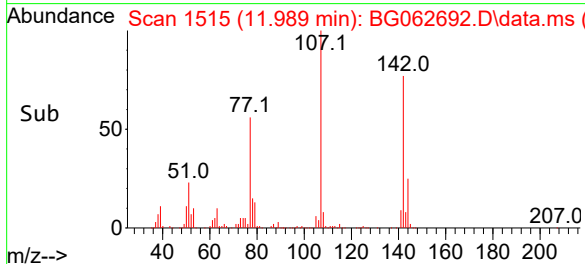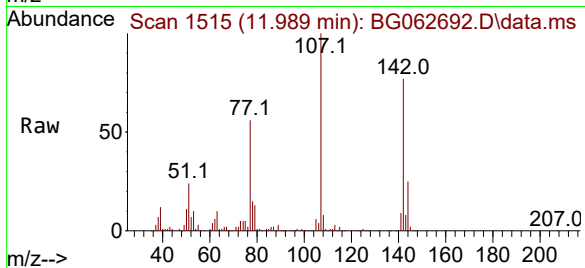

#36
2-Methylnaphthalene
Concen: 79.955 ng/ul
RT: 12.359 min Scan# 1578
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:142 Resp: 949599
Ion Ratio Lower Upper
142 100
141 88.4 73.4 110.2


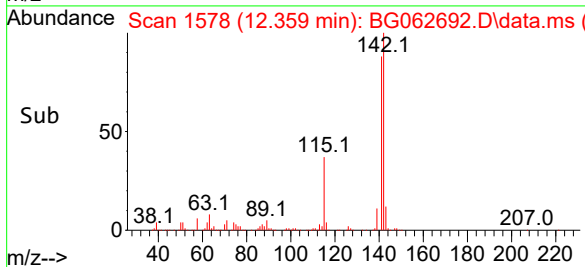

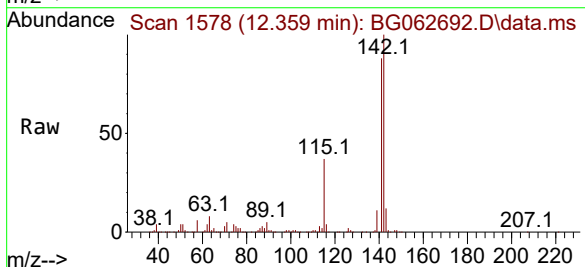




#37
1-Methylnaphthalene
Concen: 79.308 ng/ul
RT: 12.582 min Scan# 1616
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:142 Resp: 964836
Ion Ratio Lower Upper
142 100
141 90.6 71.1 106.7
116 3.8 3.0 4.6



#39
1,2,4,5-Tetrachlorobenzene
Concen: 79.067 ng/ul
RT: 12.729 min Scan# 1641
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:216 Resp: 660702
Ion Ratio Lower Upper
216 100
214 78.5 61.8 92.8
179 19.5 13.6 20.4
108 13.6 10.7 16.1









#40
Hexachlorocyclopentadiene
Concen: 83.277 ng/ul
RT: 12.711 min Scan# 1638
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:237 Resp: 356068
Ion Ratio Lower Upper
237 100
235 63.1 47.0 70.6
272 13.7 9.4 14.0

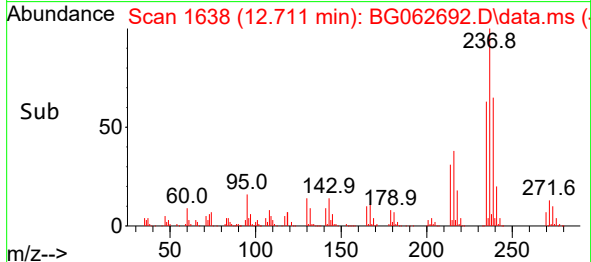

#41
2,4,6-Trichlorophenol
Concen: 82.881 ng/ul
RT: 12.970 min Scan# 1682
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:196 Resp: 419499
Ion Ratio Lower Upper
196 100
198 93.2 76.2 114.4
200 30.4 26.0 39.0









#42
 2,4,5-Trichlorophenol
 Concen: 84.393 ng/ul
 RT: 13.046 min Scan# 1
 Delta R.T. 0.006 min
 Lab File: BG062692.D
 Acq: 9 Sep 2024 17:04




Instrument :
 BNA_G
 ClientSampleId :
 SST080442


Tgt Ion:196 Resp: 458624
 Ion Ratio Lower Upper
 196 100
 198 94.2 71.2 106.8
 200 32.9 24.6 37.0



#43
 1,1'-Biphenyl
 Concen: 77.637 ng/ul
 RT: 13.369 min Scan# 1750
 Delta R.T. 0.006 min
 Lab File: BG062692.D
 Acq: 9 Sep 2024 17:04

Tgt Ion:154 Resp: 1327014
 Ion Ratio Lower Upper
 154 100
 153 40.8 33.4 50.0
 76 12.7 10.1 15.1





#44

2-Chloronaphthalene

Concen: 78.716 ng/ul

RT: 13.416 min Scan# 1757

Delta R.T. 0.006 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :

SSTD080442





Tgt Ion:162 Resp: 1094069

Ion Ratio Lower Upper

162 100

164 33.5 27.1 40.7

127 36.2 28.5 42.7

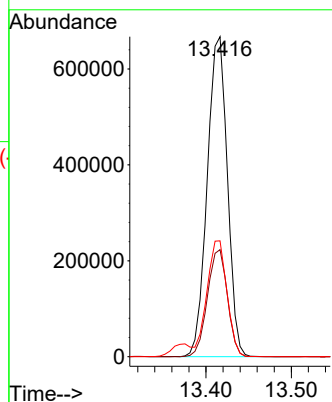

#45

2-Nitroaniline

Concen: 88.256 ng/ul

RT: 13.616 min Scan# 1792

Delta R.T. 0.006 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04




Tgt Ion: 65 Resp: 336601


Ion Ratio Lower Upper

65 100

92 66.9 55.0 82.4

138 97.8 80.0 120.0





#47

Dimethylphthalate

Concen: 76.773 ng/ul

RT: 13.998 min Scan# 1857

Delta R.T. 0.012 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :

SSTD080442





Tgt Ion:163 Resp: 1479904

Ion Ratio Lower Upper

163 100

194 4.1 3.0 4.6

164 10.1 8.3 12.5



#48

2,6-Dinitrotoluene

Concen: 88.196 ng/ul

RT: 14.116 min Scan# 1877

Delta R.T. 0.012 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04




Tgt Ion:165 Resp: 299517


Ion Ratio Lower Upper

165 100

89 55.4 47.4 71.0

121 19.0 17.0 25.6









#50
Acenaphthylene
Concen: 76.544 ng/ul
RT: 14.262 min Scan# 1902
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:152 Resp: 1679933
Ion Ratio Lower Upper
152 100
151 20.6 15.9 23.9
153 13.9 10.2 15.2



#51
3-Nitroaniline
Concen: 76.178 ng/ul
RT: 14.445 min Scan# 1933
Delta R.T. 0.012 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:138 Resp: 259010
Ion Ratio Lower Upper
138 100
108 10.5 7.7 11.5
92 119.5 92.6 138.8









#52
Acenaphthene
Concen: 77.325 ng/ul
RT: 14.603 min Scan# 1959
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:153 Resp: 1202096
Ion Ratio Lower Upper
153 100
152 49.2 37.2 55.8
154 87.0 67.8 101.6

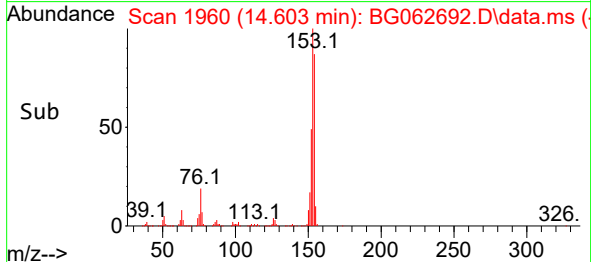

#53
2,4-Dinitrophenol
Concen: 89.749 ng/ul
RT: 14.650 min Scan# 1968
Delta R.T. 0.012 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:184 Resp: 201263
Ion Ratio Lower Upper
184 100
63 59.9 49.0 73.4
154 62.1 50.4 75.6


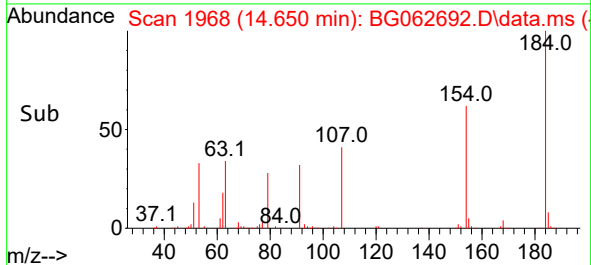






#55
4-Nitrophenol
Concen: 82.296 ng/ul
RT: 14.762 min Scan# 1987
Delta R.T. 0.018 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:109 Resp: 235218
Ion Ratio Lower Upper
109 100
139 112.8 92.5 138.7
65 128.9 97.8 146.8

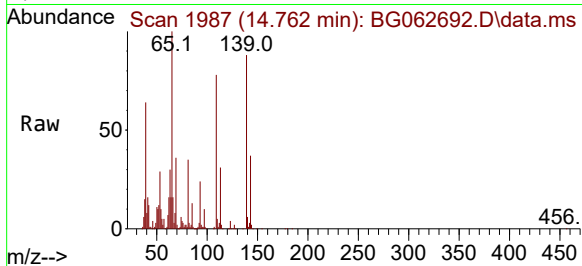

#56
Dibenzofuran
Concen: 75.905 ng/ul
RT: 14.938 min Scan# 2017
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:168 Resp: 1752974
Ion Ratio Lower Upper
168 100
139 34.8 27.6 41.4

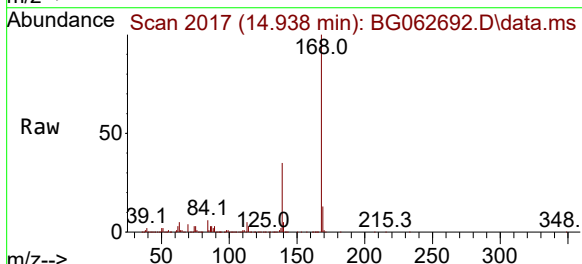



#57

2,4-Dinitrotoluene

Concen: 86.897 ng/ul

RT: 14.903 min Scan# 20

Delta R.T. 0.012 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :

SSTD080442





Tgt Ion:165 Resp: 461391

Ion Ratio Lower Upper

165 100

63 42.3 33.8 50.8

182 2.0 2.4 3.6#

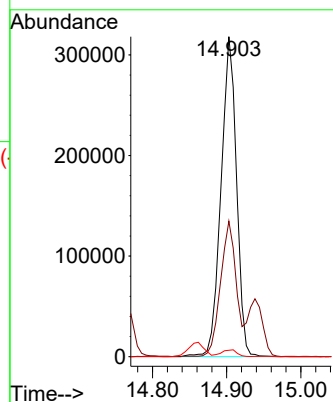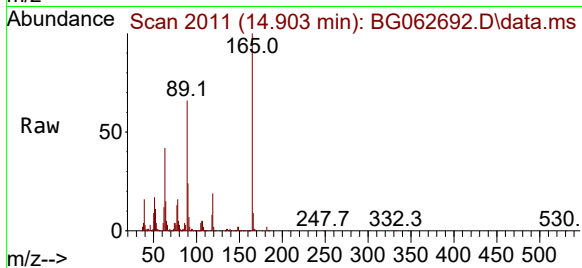

#58

2,3,4,6-Tetrachlorophenol

Concen: 82.601 ng/ul

RT: 15.167 min Scan# 2056

Delta R.T. 0.012 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Tgt Ion:232 Resp: 454900




Ion Ratio Lower Upper


232 100

131 32.1 26.6 40.0

130 1.8 1.6 2.4

166 25.4 20.6 31.0

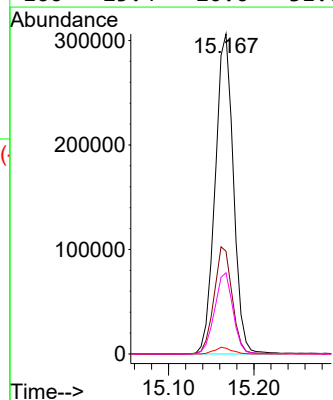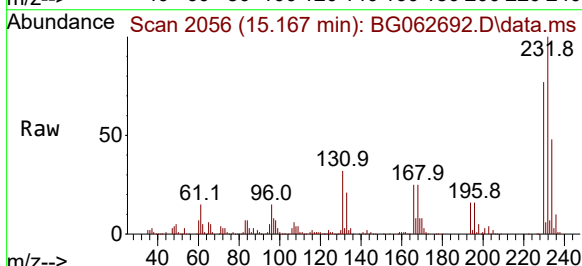



#59

Diethylphthalate

Concen: 76.312 ng/ul

RT: 15.361 min Scan# 2088

Delta R.T. 0.006 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :

SSTD080442





Tgt Ion:149 Resp: 1451169

Ion Ratio Lower Upper

149 100

177 23.1 18.4 27.6

150 12.6 9.7 14.5



#61

Fluorene

Concen: 74.022 ng/ul

RT: 15.590 min Scan# 2128

Delta R.T. 0.012 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04




Tgt Ion:166 Resp: 1342918


Ion Ratio Lower Upper

166 100

165 100.3 80.9 121.3

167 13.7 10.9 16.3









#62
4-Chlorophenyl-phenylether
Concen: 74.702 ng/ul
RT: 15.579 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:204 Resp: 794966
Ion Ratio Lower Upper
204 100
206 32.3 25.3 37.9
141 50.6 37.4 56.0

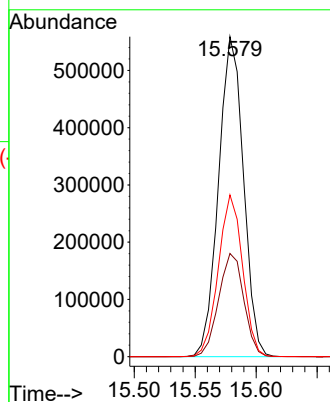

#63
4-Nitroaniline
Concen: 73.981 ng/ul
RT: 15.614 min Scan# 2132
Delta R.T. 0.018 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:138 Resp: 270680
Ion Ratio Lower Upper
138 100
92 52.8 42.8 64.2
108 91.6 71.0 106.4


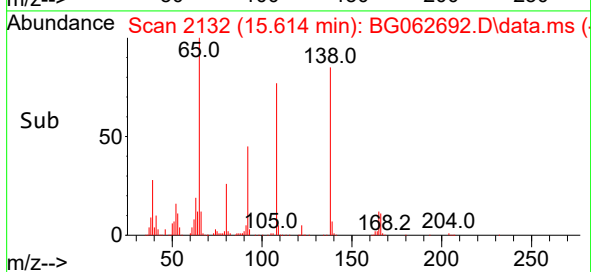
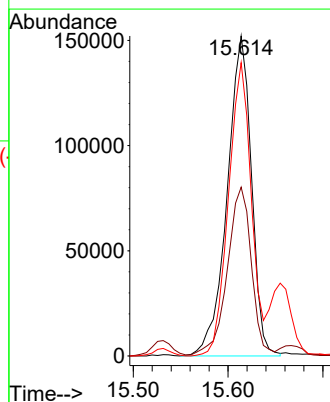
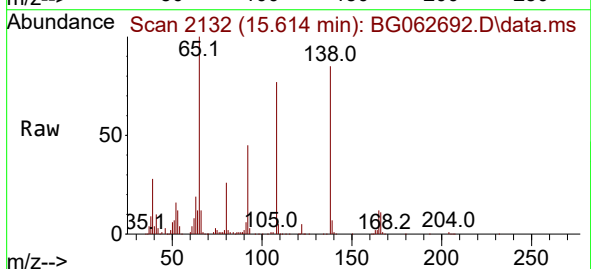


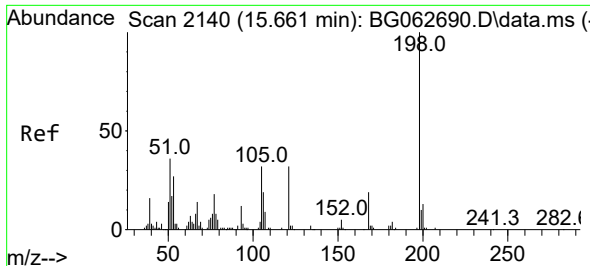

#66
4,6-Dinitro-2-methylphenol
Concen: 86.475 ng/ul
RT: 15.673 min Scan# 2142
Delta R.T. 0.012 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:198 Resp: 312934
Ion Ratio Lower Upper
198 100
182 3.2 3.3 4.9#
77 20.4 15.0 22.6

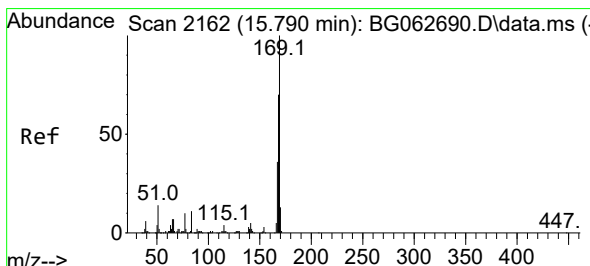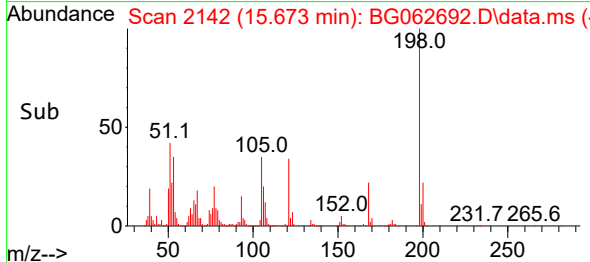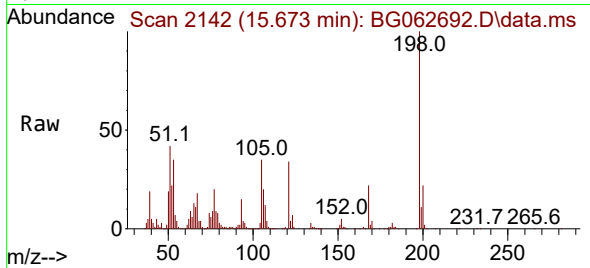

#67
N-Nitrosodiphenylamine
Concen: 79.673 ng/ul
RT: 15.796 min Scan# 2163
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:169 Resp: 1240111
Ion Ratio Lower Upper
169 100
168 70.1 55.7 83.5
167 37.0 28.9 43.3


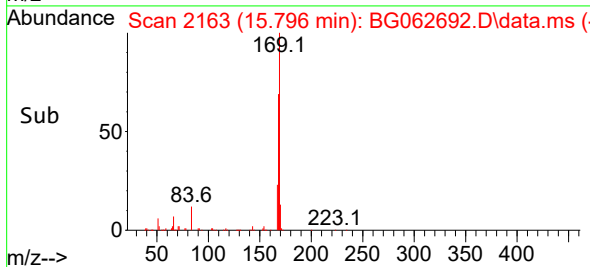

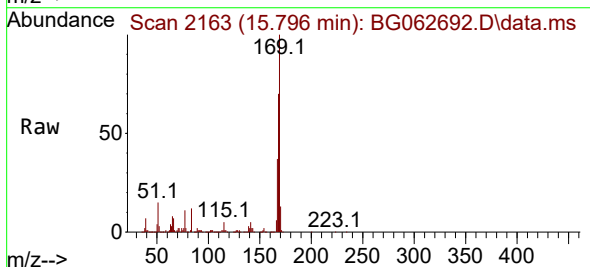




#68
4-Bromophenyl-phenylether
Concen: 79.734 ng/ul
RT: 16.472 min Scan# 21
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:248 Resp: 556848
Ion Ratio Lower Upper
248 100
250 98.2 77.9 116.9
141 61.2 47.9 71.9

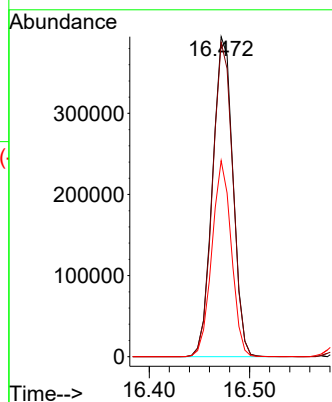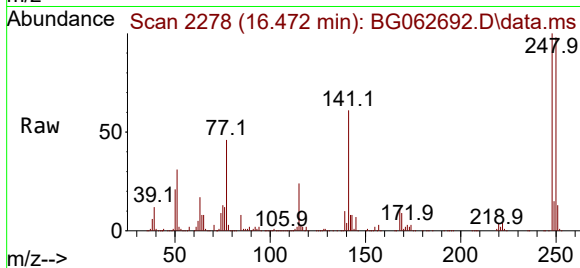

#69
Hexachlorobenzene
Concen: 79.043 ng/ul
RT: 16.595 min Scan# 2299
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:284 Resp: 630280
Ion Ratio Lower Upper
284 100
142 23.7 18.6 27.8
249 30.5 23.7 35.5




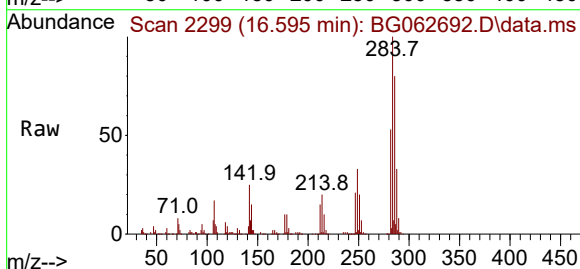




#70
Atrazine
Concen: 80.656 ng/ul
RT: 16.748 min Scan# 21
Delta R.T. 0.012 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:200 Resp: 559139
Ion Ratio Lower Upper
200 100
173 24.1 18.6 27.8
215 49.0 37.6 56.4



#71
Pentachlorophenol
Concen: 86.511 ng/ul
RT: 16.936 min Scan# 2357
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:266 Resp: 412607
Ion Ratio Lower Upper
266 100
264 62.1 48.6 72.8
268 63.1 49.5 74.3







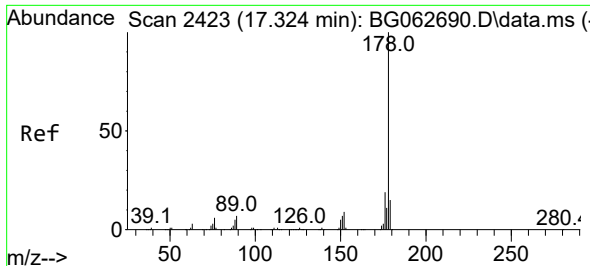

#72
Phenanthrene
Concen: 75.027 ng/ul
RT: 17.329 min Scan# 2423
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:178 Resp: 2367933
Ion Ratio Lower Upper
178 100
179 16.0 12.1 18.1
176 20.0 14.9 22.3

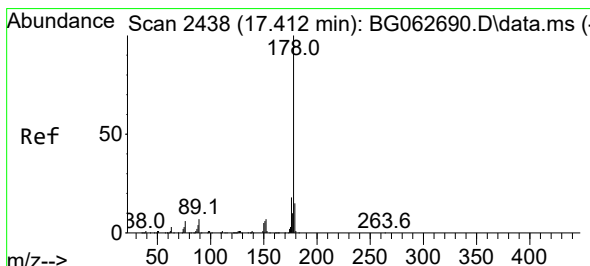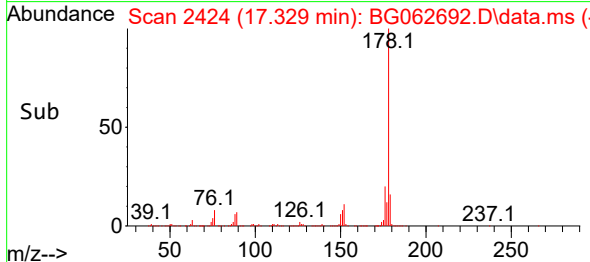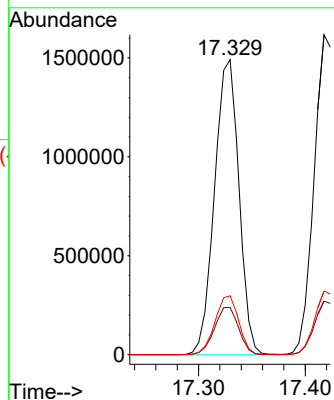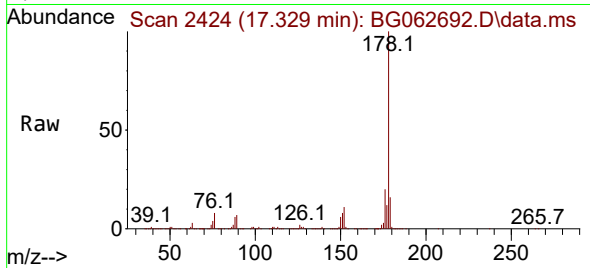

#74
Anthracene
Concen: 75.118 ng/ul
RT: 17.418 min Scan# 2439
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:178 Resp: 2416953
Ion Ratio Lower Upper
178 100
179 16.7 12.4 18.6
176 19.9 14.4 21.6


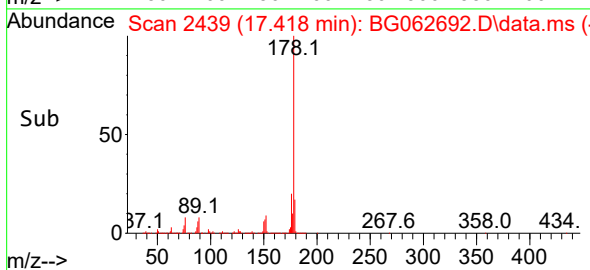
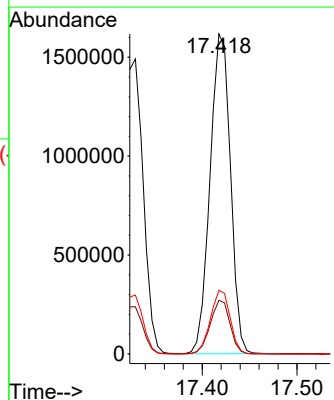
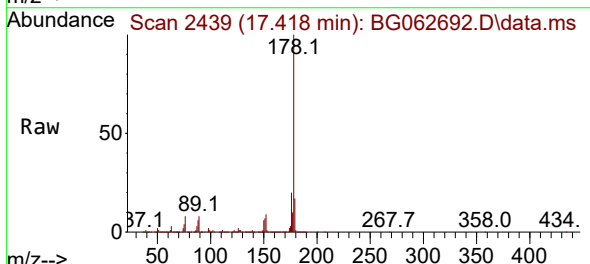




#75
1,2,3,4-Tetrachlorobenzene
Concen: 83.025 ng/ul
RT: 13.334 min Scan# 1
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:216 Resp: 688121
Ion Ratio Lower Upper
216 100
214 77.0 61.5 92.3
218 47.7 38.0 57.0

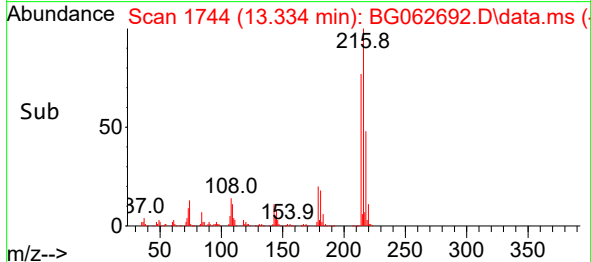

#76
Pentachlorobenzene
Concen: 80.424 ng/ul
RT: 14.862 min Scan# 2004
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:250 Resp: 738650
Ion Ratio Lower Upper
250 100
248 62.9 51.5 77.3
252 62.4 50.8 76.2




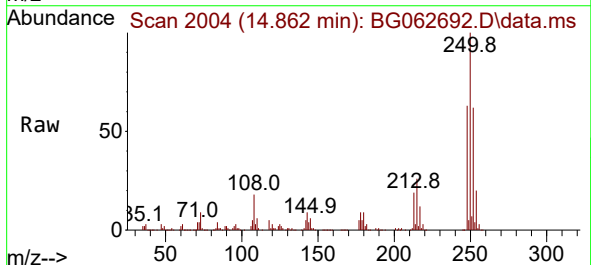


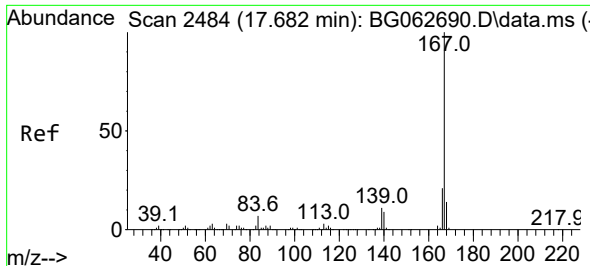

#77
Carbazole
Concen: 78.027 ng/ul
RT: 17.688 min Scan# 2485
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:167 Resp: 2081907
Ion Ratio Lower Upper
167 100
166 23.0 17.2 25.8
139 12.5 9.0 13.6

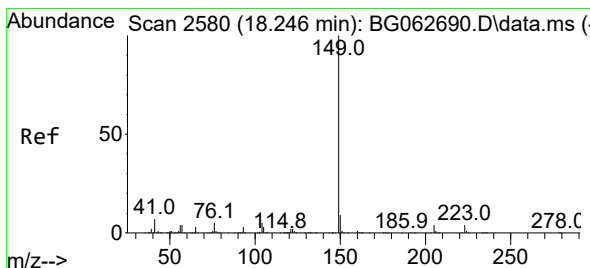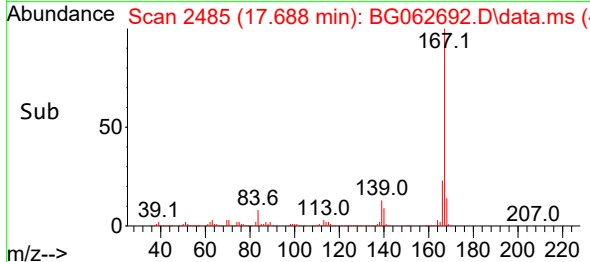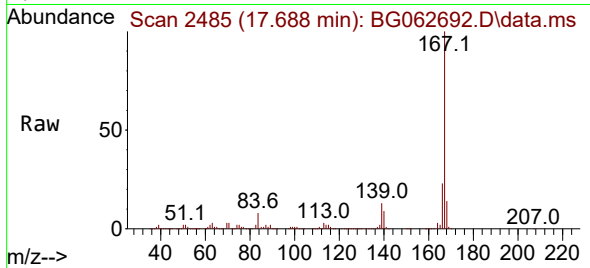

#78
Di-n-butylphthalate
Concen: 75.702 ng/ul
RT: 18.246 min Scan# 2580
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:149 Resp: 2388790
Ion Ratio Lower Upper
149 100
150 10.3 7.0 10.6
104 5.9 4.1 6.1


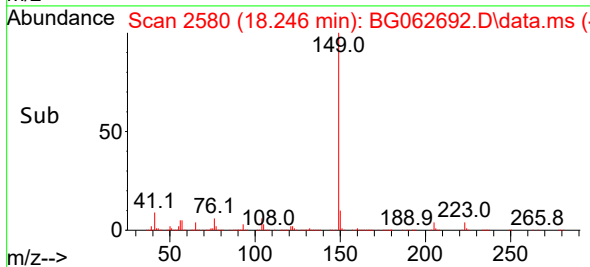

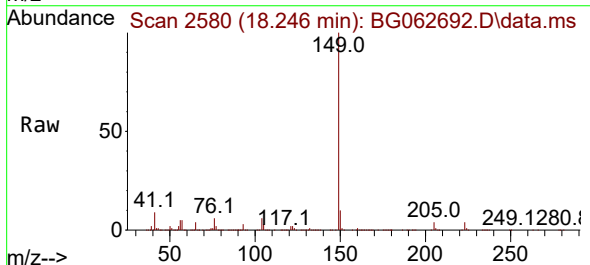




#80
Fluoranthene
Concen: 74.334 ng/ul
RT: 19.339 min Scan# 21
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:202 Resp: 2861392
Ion Ratio Lower Upper
202 100
101 9.7 6.6 10.0
100 8.0 5.3 7.9#

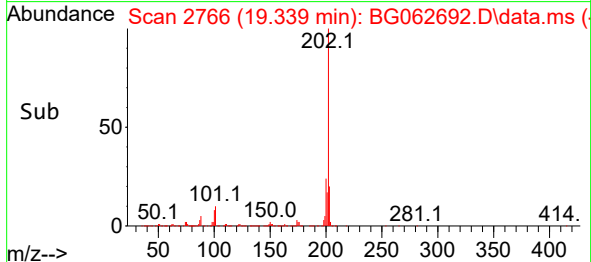

#82
Pyrene
Concen: 71.854 ng/ul
RT: 19.703 min Scan# 2828
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:202 Resp: 2977359
Ion Ratio Lower Upper
202 100
101 11.5 7.7 11.5
100 9.9 6.5 9.7#









#83
Butylbenzylphthalate
Concen: 86.108 ng/ul
RT: 20.590 min Scan# 2979
Delta R.T. 0.000 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:149 Resp: 1059183
Ion Ratio Lower Upper
149 100
91 74.5 57.3 85.9
206 23.7 20.4 30.6



#84
3,3'-Dichlorobenzidine
Concen: 74.990 ng/ul
RT: 21.431 min Scan# 3122
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:252 Resp: 975129
Ion Ratio Lower Upper
252 100
254 64.5 51.8 77.6
126 7.8 6.0 9.0









#85
Benzo(a)anthracene
Concen: 74.916 ng/ul
RT: 21.513 min Scan# 3135
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04




Instrument :
BNA_G
ClientSampleId :
SSTD080442


Tgt Ion:228 Resp: 3218186
Ion Ratio Lower Upper
228 100
229 22.9 15.8 23.8
226 31.1 21.6 32.4



#86
Bis(2-ethylhexyl)phthalate
Concen: 82.211 ng/ul
RT: 21.431 min Scan# 3122
Delta R.T. 0.006 min
Lab File: BG062692.D
Acq: 9 Sep 2024 17:04

Tgt Ion:149 Resp: 1489030
Ion Ratio Lower Upper
149 100
167 27.8 21.3 31.9
279 4.7 3.8 5.6





#87

Chrysene

Concen: 74.519 ng/ul

RT: 21.577 min Scan# 3146

Delta R.T. 0.006 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :

SSTD080442





Tgt Ion:228 Resp: 3036918

Ion Ratio Lower Upper

228 100

226 34.9 24.2 36.2

229 22.7 15.4 23.0

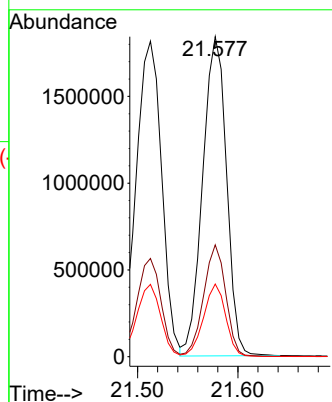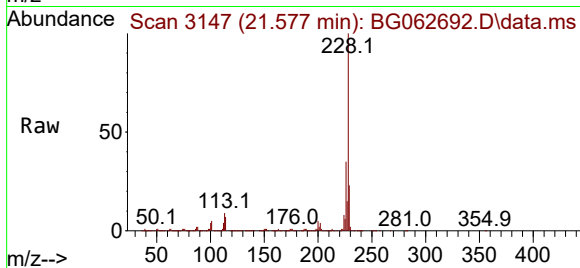

#89

Di-n-octyl phthalate

Concen: 83.931 ng/ul




RT: 22.588 min Scan# 3319


Delta R.T. 0.006 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Tgt Ion:149 Resp: 2598020

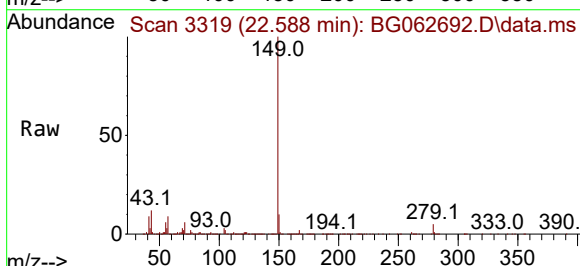



#90

Benzo(b)fluoranthene

Concen: 80.518 ng/ul

RT: 23.634 min Scan# 3497

Delta R.T. 0.012 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :

SSTD080442





Tgt Ion:252 Resp: 3308197

Ion Ratio Lower Upper

252 100

253 22.9 17.0 25.6

125 7.1 5.4 8.0

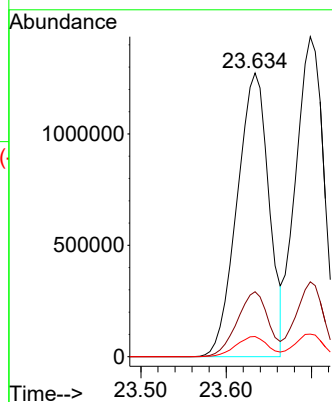

#91

Benzo(k)fluoranthene

Concen: 78.174 ng/ul

RT: 23.698 min Scan# 3508

Delta R.T. 0.012 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04




Tgt Ion:252 Resp: 3288814


Ion Ratio Lower Upper

252 100

253 23.4 16.9 25.3

125 7.1 5.7 8.5





#93

Benzo(a)pyrene

Concen: 80.053 ng/ul

RT: 24.468 min Scan# 3

Delta R.T. 0.024 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04

Instrument :

BNA_G

ClientSampleId :

SSTD080442





Tgt Ion:252 Resp: 3102286

Ion Ratio Lower Upper

252 100

253 22.8 17.4 26.0

125 8.1 6.1 9.1

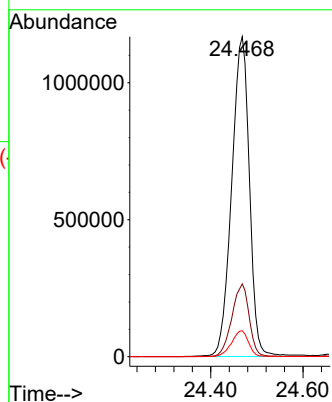

#94

Indeno(1,2,3-cd)pyrene

Concen: 83.137 ng/ul

RT: 28.070 min Scan# 4252

Delta R.T. 0.024 min

Lab File: BG062692.D

Acq: 9 Sep 2024 17:04




Tgt Ion:276 Resp: 3969549


Ion Ratio Lower Upper

276 100

138 13.0 11.4 17.2

277 24.1 18.9 28.3









#95
 Dibenzo(a,h)anthracene
 Concen: 83.127 ng/ul
 RT: 28.134 min Scan# 41
 Delta R.T. 0.035 min
 Lab File: BG062692.D
 Acq: 9 Sep 2024 17:04

Instrument :
 BNA_G
 ClientSampleId :
 SSTD080442

Tgt Ion:278 Resp: 3188093
 Ion Ratio Lower Upper
 278 100
 139 11.0 7.8 11.8
 279 24.0 18.6 28.0



#96
 Benzo(g,h,i)perylene
 Concen: 82.594 ng/ul
 RT: 29.163 min Scan# 4438
 Delta R.T. 0.035 min
 Lab File: BG062692.D
 Acq: 9 Sep 2024 17:04

Tgt Ion:276 Resp: 3045796
 Ion Ratio Lower Upper
 276 100
 138 14.1 11.8 17.6
 277 22.8 18.4 27.6

