

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090924\
 Data File : BG062694.D
 Acq On : 9 Sep 2024 19:08
 Operator : JU/RC
 Sample : SSTDICV020
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SICV444

Quant Time: Sep 10 01:31:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	70512	20.000	ng/u1	0.00
20) Naphthalene-d8	10.696	136	300531	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.532	164	243920	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.276	188	646077	20.000	ng/u1	0.00
79) Chrysene-d12	21.524	240	712351	20.000	ng/u1	0.00
88) Perylene-d12	24.579	264	767266	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	11553	7.407	ng/uL	0.00
4) Pyridine-d5	3.768	84	88098	17.743	ng/u1	0.00
7) Phenol-d5	7.070	99	112554	18.204	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.235	67	68132	18.379	ng/u1	0.00
11) 2-Chlorophenol-d4	7.435	132	88025	19.545	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	97150	18.855	ng/u1	0.00
21) Nitrobenzene-d5	9.056	128	42999	20.019	ng/u1	0.00
24) 2-Nitrophenol-d4	9.779	143	50863	21.652	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.319	165	102302	19.997	ng/u1	0.00
31) 4-Chloroaniline-d4	10.831	131	134547	19.134	ng/u1	0.00
46) Dimethylphthalate-d6	13.939	166	378680	20.160	ng/u1	0.00
49) Acenaphthylene-d8	14.221	160	410893	19.696	ng/u1	0.00
54) 4-Nitrophenol-d4	14.726	143	63056	19.761	ng/u1	0.00
60) Fluorene-d10	15.525	176	334365	19.754	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.643	200	72265	19.445	ng/u1	0.00
73) Anthracene-d10	17.376	188	603844	19.804	ng/u1	0.00
81) Pyrene-d10	19.661	212	773394	19.293	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.374	264	793724	19.591	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.398	88	13824	7.907	ng/uL#	88
5) Pyridine	3.786	79	97283	18.680	ng/u1	93
6) Benzaldehyde	7.041	77	78312	23.036	ng/u1	97
8) Phenol	7.094	94	120600	18.763	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.323	93	89638	18.449	ng/u1	98
12) 2-Chlorophenol	7.470	128	90306	19.611	ng/u1	96
13) 2-Methylphenol	8.345	108	88955	18.456	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.422	45	165222	18.892	ng/u1	99
16) Acetophenone	8.721	105	159912	19.095	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.704	70	83096	18.955	ng/u1	93
18) 4-Methylphenol	8.668	108	101598	18.737	ng/u1	99
19) Hexachloroethane	8.986	117	36476	19.676	ng/u1	89
22) Nitrobenzene	9.097	77	117723	20.260	ng/u1	95
23) Isophorone	9.620	82	235842	19.852	ng/u1	99
25) 2-Nitrophenol	9.808	139	54573	21.078	ng/u1	91
26) 2,4-Dimethylphenol	9.873	107	108943	19.692	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.102	93	132235	19.917	ng/u1	95
29) 2,4-Dichlorophenol	10.343	162	102521	20.347	ng/u1	94
30) Naphthalene	10.748	128	314521	19.519	ng/u1	98
32) 4-Chloroaniline	10.848	127	134351	19.211	ng/u1	99
33) Hexachlorobutadiene	11.036	225	85727	20.423	ng/u1	95
34) Caprolactam	11.600	113	23208	12.497	ng/u1	91
35) 4-Chloro-3-methylphenol	11.976	107	109566	19.934	ng/u1	97
36) 2-Methylnaphthalene	12.352	142	236553	19.891	ng/u1	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090924\
 Data File : BG062694.D
 Acq On : 9 Sep 2024 19:08
 Operator : JU/RC
 Sample : SSTDICV020
 Misc :
 ALS Vial : 10 Sample Multiplier: 1


Instrument :
 BNA_G
 ClientSampleId :
 SICV444


Quant Time: Sep 10 01:31:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 01:28:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.576	142	241308	19.808	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.723	216	164885	19.663	ng/ul	98
40) Hexachlorocyclopentadiene	12.705	237	81121	18.906	ng/ul	97
41) 2,4,6-Trichlorophenol	12.963	196	100123	19.712	ng/ul	97
42) 2,4,5-Trichlorophenol	13.034	196	111315	20.412	ng/ul	95
43) 1,1'-Biphenyl	13.363	154	334420	19.497	ng/ul	99
44) 2-Chloronaphthalene	13.404	162	276438	19.819	ng/ul	98
45) 2-Nitroaniline	13.604	65	76811	20.069	ng/ul	96
47) Dimethylphthalate	13.986	163	383588	19.830	ng/ul	98
48) 2,6-Dinitrotoluene	14.103	165	70204	20.600	ng/ul	92
50) Acenaphthylene	14.250	152	434074	19.709	ng/ul	99
51) 3-Nitroaniline	14.426	138	73906	21.660	ng/ul	95
52) Acenaphthene	14.597	153	305887	19.607	ng/ul	99
53) 2,4-Dinitrophenol	14.638	184	43338	19.258	ng/ul	93
55) 4-Nitrophenol	14.744	109	56547	19.715	ng/ul	99
56) Dibenzofuran	14.926	168	458556	19.786	ng/ul	98
57) 2,4-Dinitrotoluene	14.891	165	111183	20.866	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.155	232	112507	20.357	ng/ul#	97
59) Diethylphthalate	15.349	149	381183	19.975	ng/ul	99
61) Fluorene	15.578	166	358146	19.672	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.572	204	207735	19.452	ng/ul	99
63) 4-Nitroaniline	15.590	138	79670	21.699	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.654	198	74286	19.284	ng/ul	96
67) N-Nitrosodiphenylamine	15.784	169	331358	19.998	ng/ul	97
68) 4-Bromophenyl-phenylether	16.465	248	146101	19.652	ng/ul	97
69) Hexachlorobenzene	16.583	284	165528	19.500	ng/ul	97
70) Atrazine	16.735	200	147720	20.017	ng/ul	98
71) Pentachlorophenol	16.924	266	100436	19.782	ng/ul	97
72) Phenanthrene	17.317	178	666152	19.827	ng/ul	99
74) Anthracene	17.411	178	677920	19.792	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.328	216	174528	19.781	ng/ul	99
76) Pentachlorobenzene	14.849	250	186843	19.110	ng/ul	95
77) Carbazole	17.676	167	580986	20.455	ng/ul	98
78) Di-n-butylphthalate	18.240	149	681677	20.293	ng/ul	99
80) Fluoranthene	19.332	202	864704	19.477	ng/ul	100
82) Pyrene	19.697	202	936419	19.594	ng/ul	100
83) Butylbenzylphthalate	20.584	149	284973	20.087	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.424	252	321199	21.417	ng/ul	97
85) Benzo(a)anthracene	21.500	228	972600	19.631	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.424	149	416996	19.962	ng/ul	99
87) Chrysene	21.565	228	921302	19.601	ng/ul	99
89) Di-n-octyl phthalate	22.582	149	720786	20.196	ng/ul	100
90) Benzo(b)fluoranthene	23.616	252	922907	19.482	ng/ul	99
91) Benzo(k)fluoranthene	23.680	252	958746	19.766	ng/ul	97
93) Benzo(a)pyrene	24.438	252	877350	19.636	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	28.034	276	1068626	19.412	ng/ul	98
95) Dibenzo(a,h)anthracene	28.093	278	869687	19.668	ng/ul	99
96) Benzo(g,h,i)perylene	29.109	276	816121	19.195	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 10 01:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG090924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 01:28:17 2024
Response via : Initial Calibration




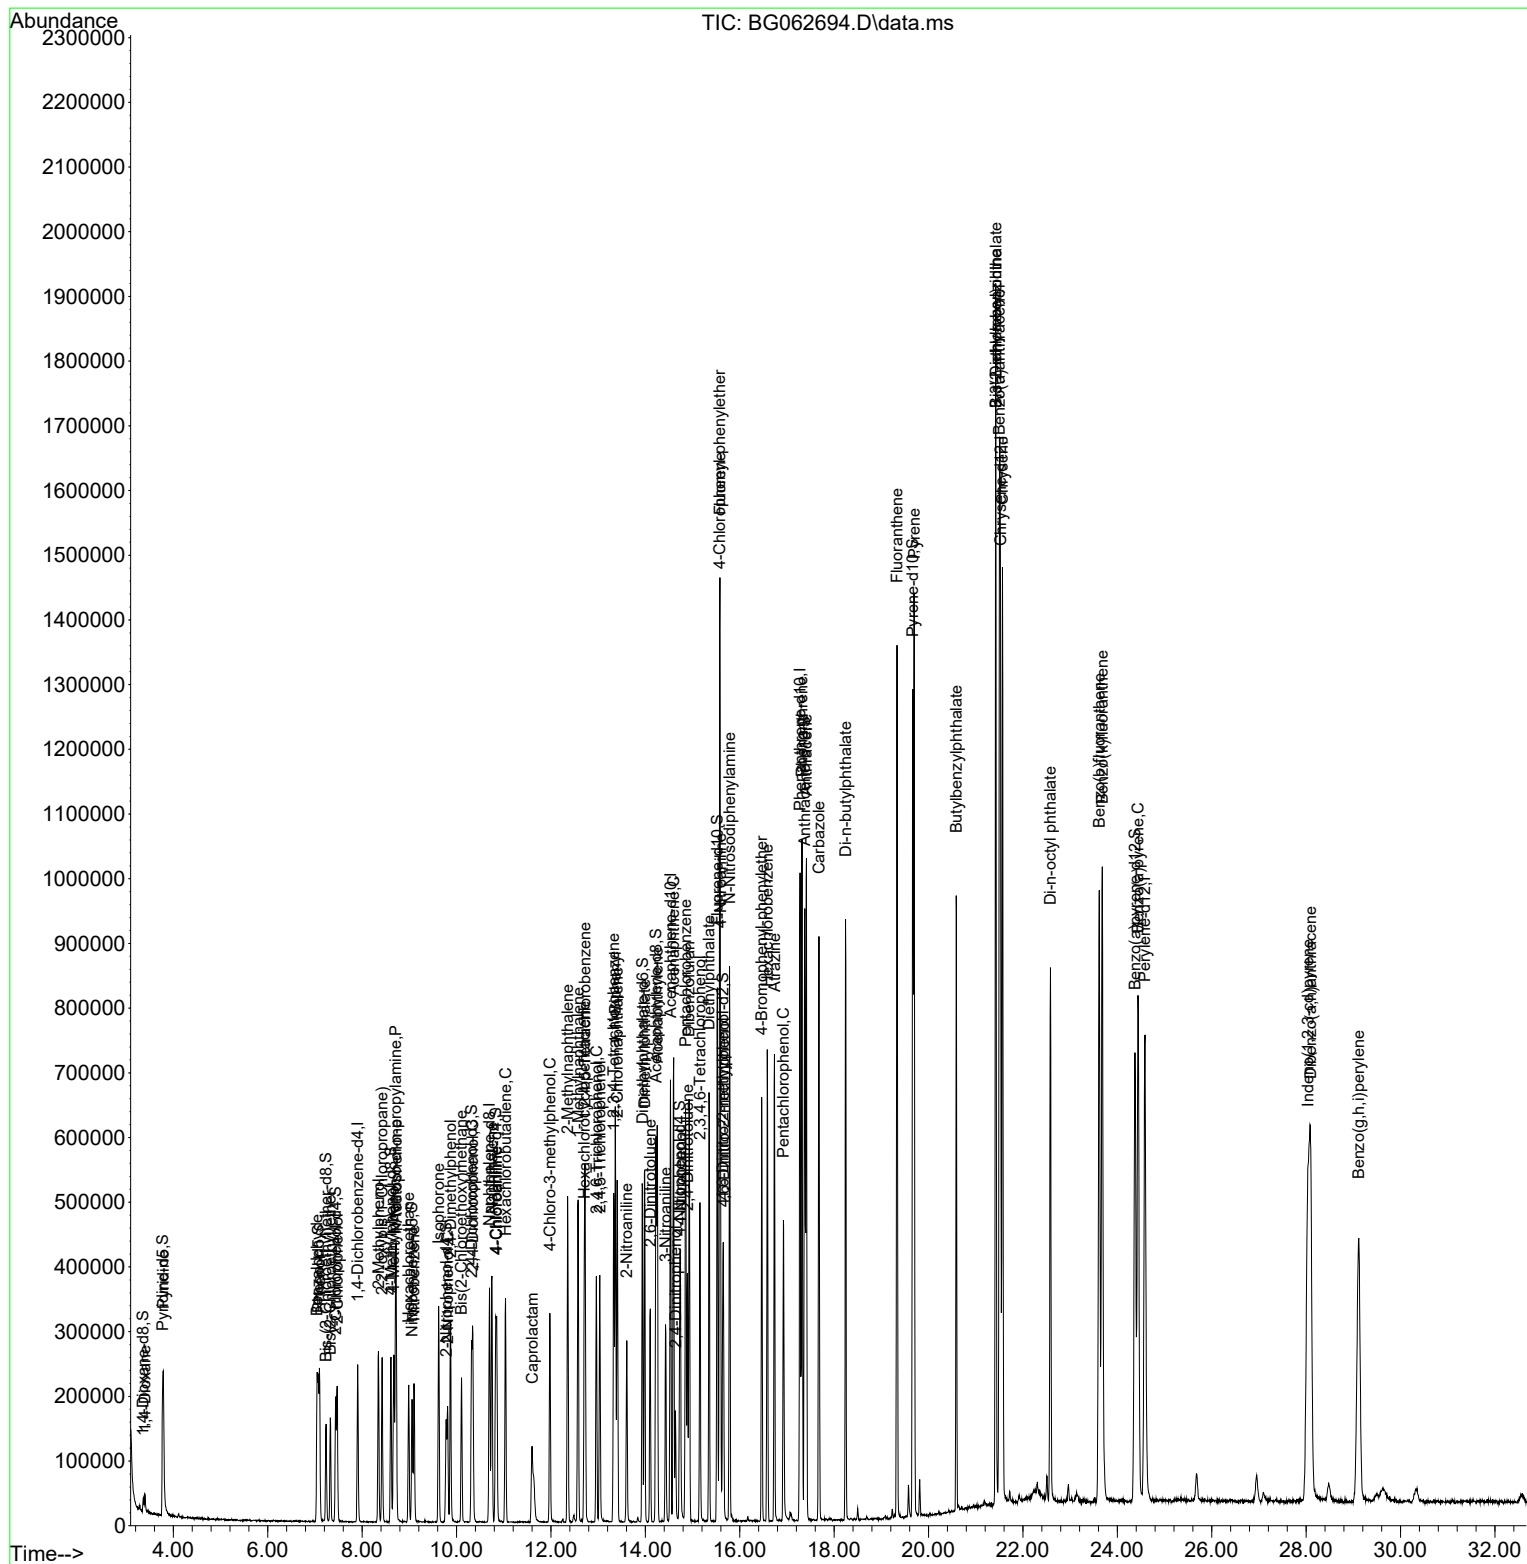




#2
1,4-Dioxane
Concen: 7.907 ng/uL
RT: 3.398 min Scan# 51
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion: 88 Resp: 13824
Ion Ratio Lower Upper
88 100
43 34.8 23.1 34.7#
58 61.6 57.2 85.8



#5
Pyridine
Concen: 18.680 ng/uL
RT: 3.786 min Scan# 119
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion: 79 Resp: 97283
Ion Ratio Lower Upper
79 100
52 96.0 69.8 104.8
51 41.8 34.0 51.0









#6
Benzaldehyde
Concen: 23.036 ng/ul
RT: 7.041 min Scan# 61
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion: 77 Resp: 78312
Ion Ratio Lower Upper
77 100
105 94.8 79.0 118.4
106 83.6 69.0 103.6

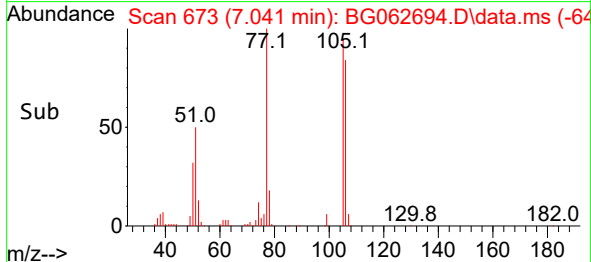

#8
Phenol
Concen: 18.763 ng/ul
RT: 7.094 min Scan# 682
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion: 94 Resp: 120600
Ion Ratio Lower Upper
94 100
65 30.2 25.1 37.7
66 38.8 30.8 46.2




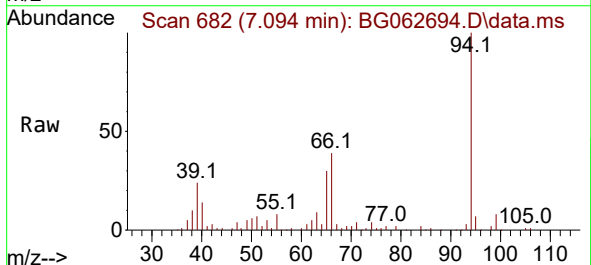




#10
Bis(2-Chloroethyl)ether
Concen: 18.449 ng/ul
RT: 7.323 min Scan# 721
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion: 93 Resp: 89638
Ion Ratio Lower Upper
93 100
63 80.0 62.0 93.0
95 33.1 25.9 38.9

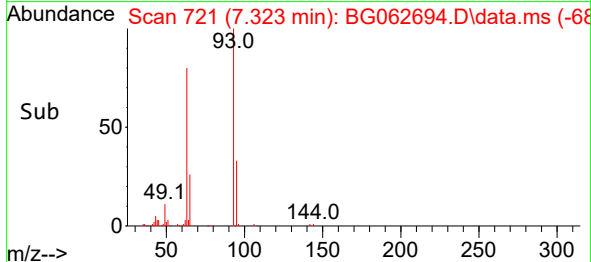

#12
2-Chlorophenol
Concen: 19.611 ng/ul
RT: 7.470 min Scan# 746
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:128 Resp: 90306
Ion Ratio Lower Upper
128 100
64 53.4 42.0 63.0
130 34.8 24.0 36.0

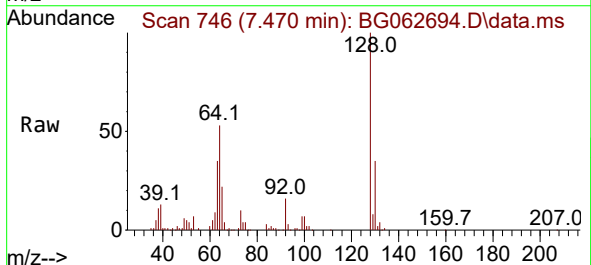



#13

2-Methylphenol

Concen: 18.456 ng/ul

RT: 8.345 min Scan# 895

Delta R.T. -0.001 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :





SICV444

Tgt Ion:108 Resp: 88955

Ion Ratio Lower Upper

108 100

107 89.4 72.1 108.1



#14

2,2'-oxybis(1-Chloropropane)

Concen: 18.892 ng/ul

RT: 8.422 min Scan# 908

Delta R.T. -0.001 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08




Tgt Ion: 45 Resp: 165222


Ion Ratio Lower Upper

45 100

77 11.1 9.0 13.6

79 8.6 6.6 9.8









#16
Acetophenone
Concen: 19.095 ng/ul
RT: 8.721 min Scan# 91
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:105 Resp: 159912
Ion Ratio Lower Upper
105 100
77 80.2 63.3 94.9
51 31.2 26.5 39.7



#17
N-Nitroso-di-n-propylamine
Concen: 18.955 ng/ul
RT: 8.704 min Scan# 956
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion: 70 Resp: 83096
Ion Ratio Lower Upper
70 100
42 69.1 50.2 75.2
101 8.8 6.2 9.4
130 20.0 15.1 22.7


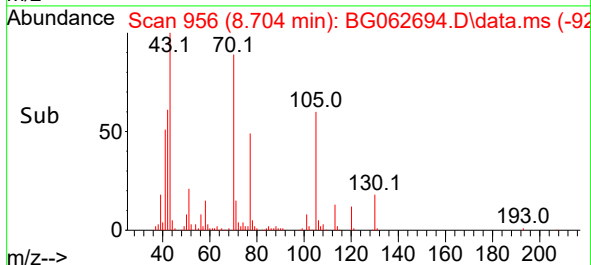
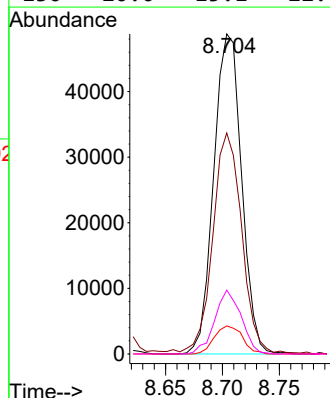





#18
4-Methylphenol
Concen: 18.737 ng/ul
RT: 8.668 min Scan# 91
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:108 Resp: 101598
Ion Ratio Lower Upper
108 100
107 106.8 86.4 129.6

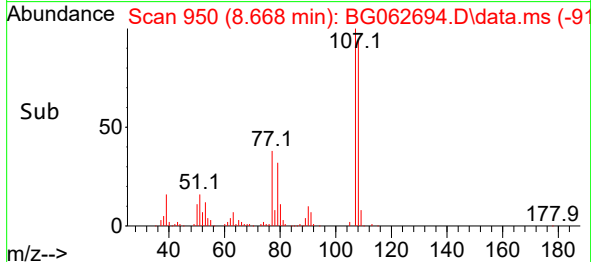

#19
Hexachloroethane
Concen: 19.676 ng/ul
RT: 8.986 min Scan# 1004
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:117 Resp: 36476
Ion Ratio Lower Upper
117 100
201 145.2 106.6 160.0
199 88.0 62.0 93.0




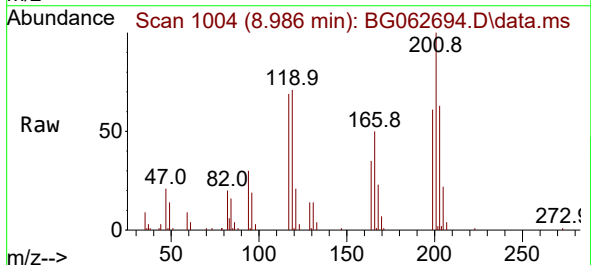




#22
Nitrobenzene
Concen: 20.260 ng/ul
RT: 9.097 min Scan# 1102
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion: 77 Resp: 117723
Ion Ratio Lower Upper
77 100
123 41.7 30.9 46.3
65 13.8 9.7 14.5

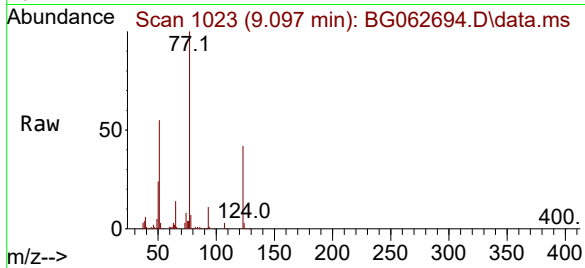

#23
Isophorone
Concen: 19.852 ng/ul
RT: 9.620 min Scan# 1112
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion: 82 Resp: 235842
Ion Ratio Lower Upper
82 100
95 7.5 5.8 8.8
138 16.6 13.0 19.6




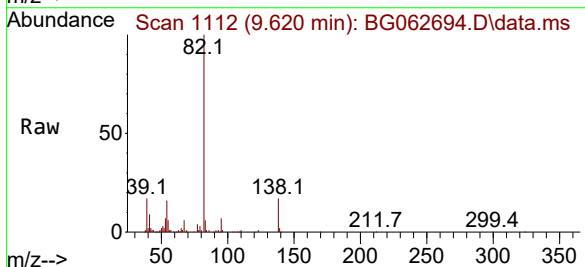




#25
2-Nitrophenol
Concen: 21.078 ng/ul
RT: 9.808 min Scan# 1144
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:139 Resp: 54573
Ion Ratio Lower Upper
139 100
65 47.1 45.4 68.0
109 28.4 23.9 35.9



#26
2,4-Dimethylphenol
Concen: 19.692 ng/ul
RT: 9.873 min Scan# 1155
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:107 Resp: 108943
Ion Ratio Lower Upper
107 100
121 48.2 38.8 58.2
122 84.1 70.5 105.7









#27
Bis(2-Chloroethoxy)methane
Concen: 19.917 ng/ul
RT: 10.102 min Scan# 1194
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion: 93 Resp: 132235
Ion Ratio Lower Upper
93 100
95 31.1 27.4 41.2
123 9.8 9.1 13.7



#29
2,4-Dichlorophenol
Concen: 20.347 ng/ul
RT: 10.343 min Scan# 1235
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:162 Resp: 102521
Ion Ratio Lower Upper
162 100
164 69.4 51.9 77.9
98 33.3 23.8 35.6









#30
Naphthalene
Concen: 19.519 ng/ul
RT: 10.748 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:128 Resp: 314521
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.6
127 14.4 10.7 16.1



#32
4-Chloroaniline
Concen: 19.211 ng/ul
RT: 10.848 min Scan# 1321
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:127 Resp: 134351
Ion Ratio Lower Upper
127 100
129 33.1 25.8 38.8





#33

Hexachlorobutadiene

Concen: 20.423 ng/ul

RT: 11.036 min Scan# 1

Delta R.T. -0.000 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:225 Resp: 85727

Ion Ratio Lower Upper

225 100

223 62.8 52.3 78.5

227 65.6 56.4 84.6



#34

Caprolactam

Concen: 12.497 ng/ul

RT: 11.600 min Scan# 1449

Delta R.T. -0.001 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08




Tgt Ion:113 Resp: 23208


Ion Ratio Lower Upper

113 100

55 175.7 150.8 226.2

56 145.6 125.0 187.6









#35
4-Chloro-3-methylphenol
Concen: 19.934 ng/ul
RT: 11.976 min Scan# 11
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:107 Resp: 109566
Ion Ratio Lower Upper
107 100
144 25.9 21.8 32.6
142 77.9 64.8 97.2



#36
2-Methylnaphthalene
Concen: 19.891 ng/ul
RT: 12.352 min Scan# 1577
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:142 Resp: 236553
Ion Ratio Lower Upper
142 100
141 87.9 73.4 110.2







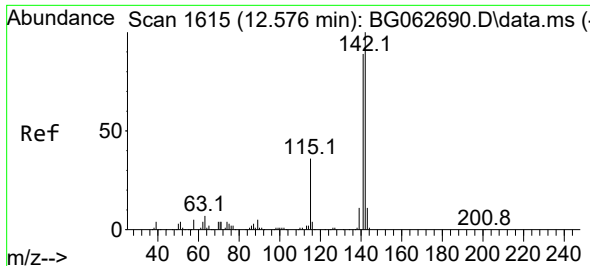

#37
1-Methylnaphthalene
Concen: 19.808 ng/ul
RT: 12.576 min Scan# 1
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:142 Resp: 241308
Ion Ratio Lower Upper
142 100
141 89.4 71.1 106.7
116 4.2 3.0 4.6

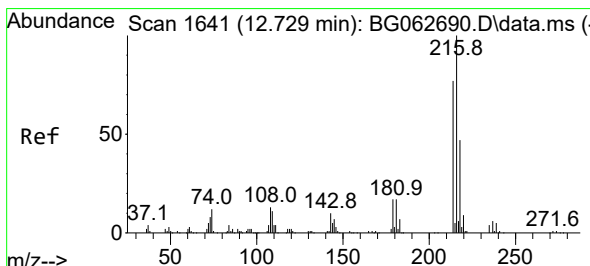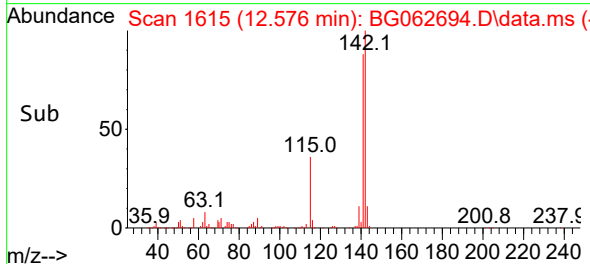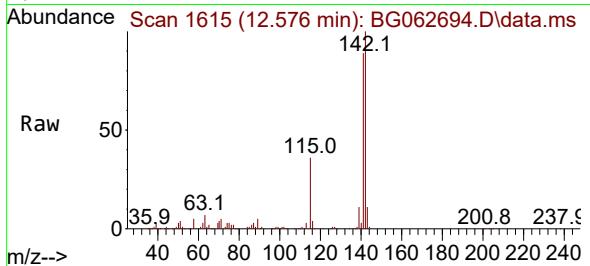

#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.663 ng/ul
RT: 12.723 min Scan# 1640
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:216 Resp: 164885
Ion Ratio Lower Upper
216 100
214 75.0 61.8 92.8
179 17.8 13.6 20.4
108 13.6 10.7 16.1


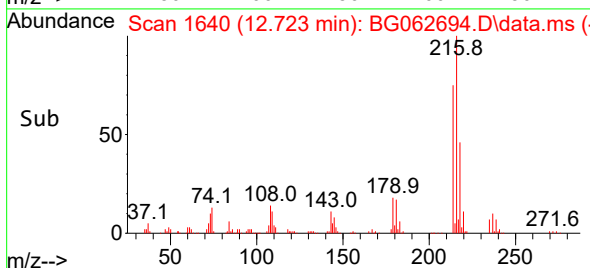
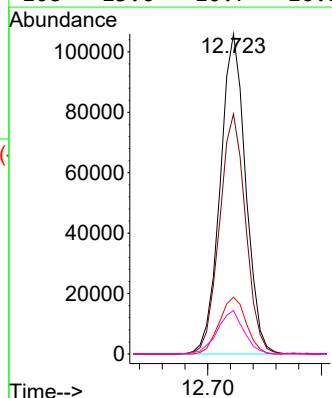
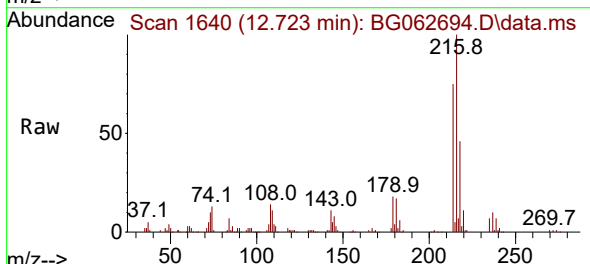




#40
Hexachlorocyclopentadiene
Concen: 18.906 ng/ul
RT: 12.705 min Scan# 1637
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:237 Resp: 81121
Ion Ratio Lower Upper
237 100
235 60.8 47.0 70.6
272 11.1 9.4 14.0

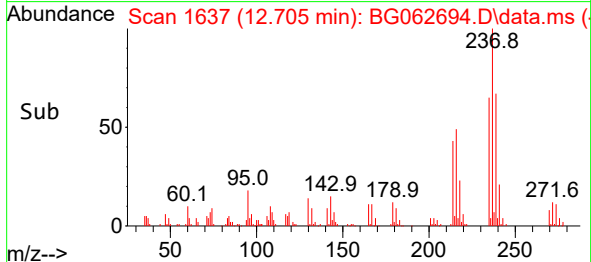

#41
2,4,6-Trichlorophenol
Concen: 19.712 ng/ul
RT: 12.963 min Scan# 1681
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:196 Resp: 100123
Ion Ratio Lower Upper
196 100
198 99.7 76.2 114.4
200 32.7 26.0 39.0









#42
2,4,5-Trichlorophenol
Concen: 20.412 ng/ul
RT: 13.034 min Scan# 1
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:196 Resp: 111315
Ion Ratio Lower Upper
196 100
198 94.6 71.2 106.8
200 28.7 24.6 37.0



#43
1,1'-Biphenyl
Concen: 19.497 ng/ul
RT: 13.363 min Scan# 1749
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:154 Resp: 334420
Ion Ratio Lower Upper
154 100
153 41.3 33.4 50.0
76 13.3 10.1 15.1









#44
2-Chloronaphthalene
Concen: 19.819 ng/ul
RT: 13.404 min Scan# 1756
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:162 Resp: 276438
Ion Ratio Lower Upper
162 100
164 33.3 27.1 40.7
127 34.2 28.5 42.7

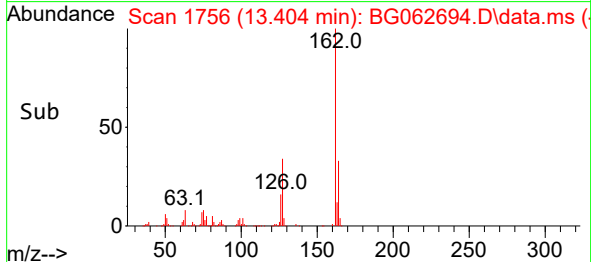

#45
2-Nitroaniline
Concen: 20.069 ng/ul
RT: 13.604 min Scan# 1790
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion: 65 Resp: 76811
Ion Ratio Lower Upper
65 100
92 66.4 55.0 82.4
138 105.4 80.0 120.0




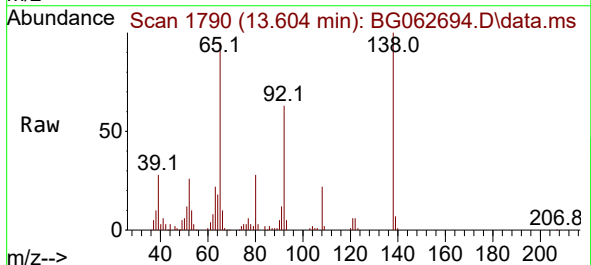




#47
Dimethylphthalate
Concen: 19.830 ng/ul
RT: 13.986 min Scan# 1855
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:163 Resp: 383588
Ion Ratio Lower Upper
163 100
194 3.8 3.0 4.6
164 9.5 8.3 12.5



#48
2,6-Dinitrotoluene
Concen: 20.600 ng/ul
RT: 14.103 min Scan# 1875
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:165 Resp: 70204
Ion Ratio Lower Upper
165 100
89 51.4 47.4 71.0
121 21.8 17.0 25.6





#50

Acenaphthylene

Concen: 19.709 ng/ul

RT: 14.250 min Scan# 1900

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:152 Resp: 434074

Ion Ratio Lower Upper

152 100

151 20.1 15.9 23.9

153 12.5 10.2 15.2



#51

3-Nitroaniline

Concen: 21.660 ng/ul

RT: 14.426 min Scan# 1930

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08




Tgt Ion:138 Resp: 73906


Ion Ratio Lower Upper

138 100

108 8.9 7.7 11.5

92 121.1 92.6 138.8









#52
Acenaphthene
Concen: 19.607 ng/ul
RT: 14.597 min Scan# 1959
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:153 Resp: 305887
Ion Ratio Lower Upper
153 100
152 47.3 37.2 55.8
154 84.2 67.8 101.6

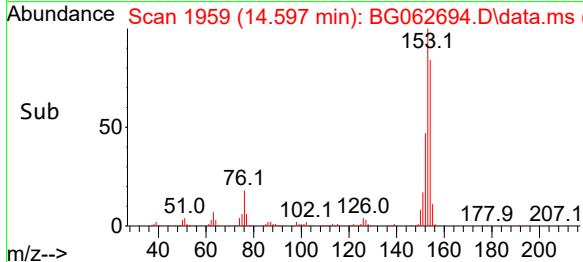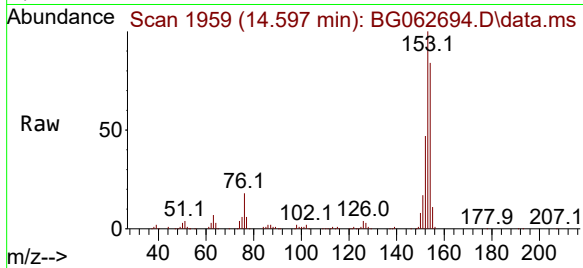

#53
2,4-Dinitrophenol
Concen: 19.258 ng/ul
RT: 14.638 min Scan# 1966
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:184 Resp: 43338
Ion Ratio Lower Upper
184 100
63 50.4 49.0 73.4
154 62.6 50.4 75.6


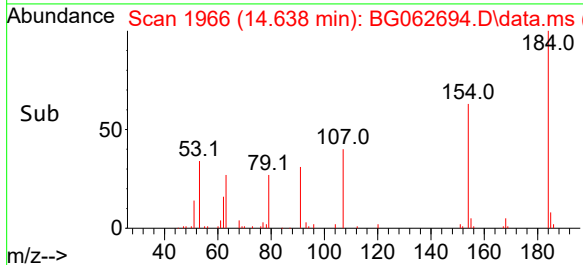

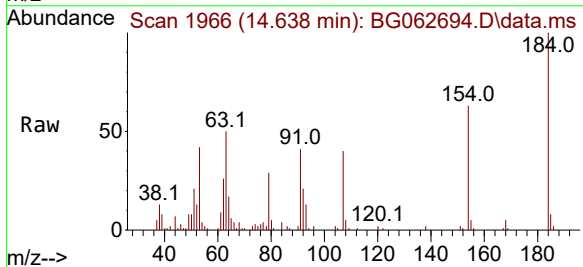




#55
4-Nitrophenol
Concen: 19.715 ng/ul
RT: 14.744 min Scan# 1984
Delta R.T. -0.001 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:109 Resp: 56547
Ion Ratio Lower Upper
109 100
139 117.9 92.5 138.7
65 122.9 97.8 146.8



#56
Dibenzofuran
Concen: 19.786 ng/ul
RT: 14.926 min Scan# 2015
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:168 Resp: 458556
Ion Ratio Lower Upper
168 100
139 33.4 27.6 41.4





#57

2,4-Dinitrotoluene

Concen: 20.866 ng/ul

RT: 14.891 min Scan# 2009

Delta R.T. -0.001 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:165 Resp: 111183

Ion Ratio Lower Upper

165 100

63 41.2 33.8 50.8

182 2.4 2.4 3.6



#58

2,3,4,6-Tetrachlorophenol

Concen: 20.357 ng/ul

RT: 15.155 min Scan# 2054

Delta R.T. -0.001 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Tgt Ion:232 Resp: 112507




Ion Ratio Lower Upper


232 100

131 34.8 26.6 40.0

130 2.5 1.6 2.4#

166 27.0 20.6 31.0









#59
Diethylphthalate
Concen: 19.975 ng/ul
RT: 15.349 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:149 Resp: 381183
Ion Ratio Lower Upper
149 100
177 22.7 18.4 27.6
150 12.2 9.7 14.5

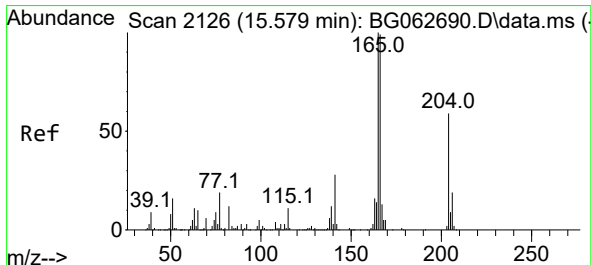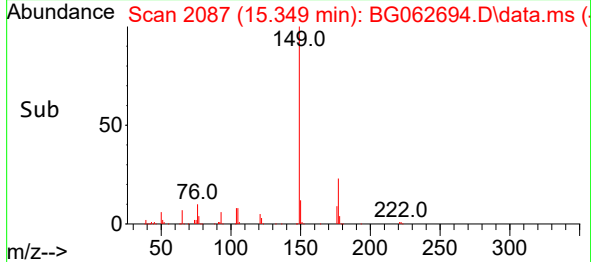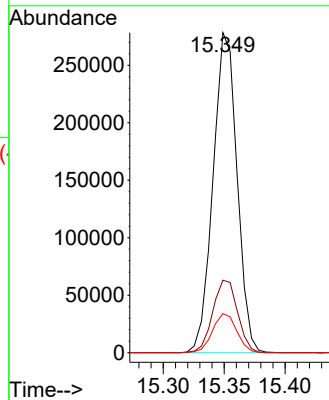

#61
Fluorene
Concen: 19.672 ng/ul
RT: 15.578 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:166 Resp: 358146
Ion Ratio Lower Upper
166 100
165 101.3 80.9 121.3
167 13.3 10.9 16.3



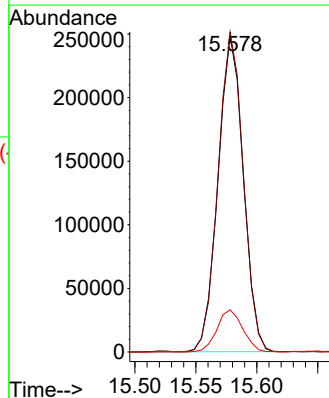
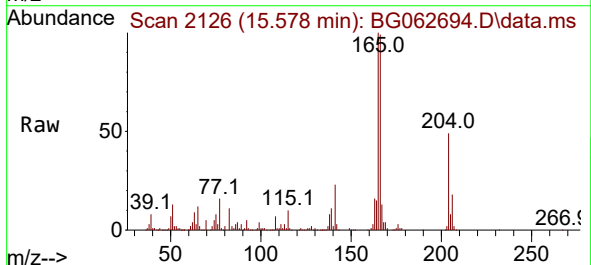




#62
4-Chlorophenyl-phenylether
Concen: 19.452 ng/ul
RT: 15.572 min Scan# 2125
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:204 Resp: 207735
Ion Ratio Lower Upper
204 100
206 32.5 25.3 37.9
141 46.3 37.4 56.0



#63
4-Nitroaniline
Concen: 21.699 ng/ul
RT: 15.590 min Scan# 2128
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:138 Resp: 79670
Ion Ratio Lower Upper
138 100
92 57.7 42.8 64.2
108 88.6 71.0 106.4









#66
4,6-Dinitro-2-methylphenol
Concen: 19.284 ng/ul
RT: 15.654 min Scan# 2140
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:198 Resp: 74286
Ion Ratio Lower Upper
198 100
182 4.5 3.3 4.9
77 20.6 15.0 22.6

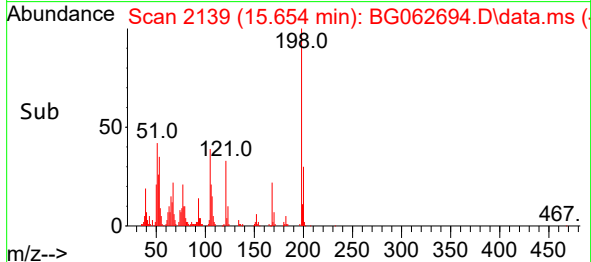

#67
N-Nitrosodiphenylamine
Concen: 19.998 ng/ul
RT: 15.784 min Scan# 2161
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:169 Resp: 331358
Ion Ratio Lower Upper
169 100
168 66.9 55.7 83.5
167 36.7 28.9 43.3









#68
4-Bromophenyl-phenylether
Concen: 19.652 ng/ul
RT: 16.465 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:248 Resp: 146101
Ion Ratio Lower Upper
248 100
250 94.2 77.9 116.9
141 58.1 47.9 71.9



#69
Hexachlorobenzene
Concen: 19.500 ng/ul
RT: 16.583 min Scan# 2297
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:284 Resp: 165528
Ion Ratio Lower Upper
284 100
142 25.9 18.6 27.8
249 29.8 23.7 35.5





#70

Atrazine

Concen: 20.017 ng/ul

RT: 16.735 min Scan# 21

Delta R.T. -0.001 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:200 Resp: 147720

Ion Ratio Lower Upper

200 100

173 24.4 18.6 27.8

215 48.0 37.6 56.4



#71

Pentachlorophenol

Concen: 19.782 ng/ul

RT: 16.924 min Scan# 2355

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08




Tgt Ion:266 Resp: 100436


Ion Ratio Lower Upper

266 100

264 58.0 48.6 72.8

268 63.9 49.5 74.3







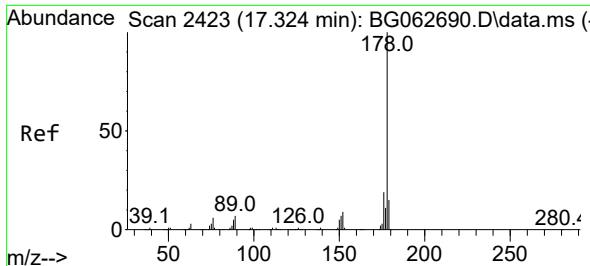

#72
Phenanthrene
Concen: 19.827 ng/ul
RT: 17.317 min Scan# 2422
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:178 Resp: 666152
Ion Ratio Lower Upper
178 100
179 15.4 12.1 18.1
176 19.2 14.9 22.3

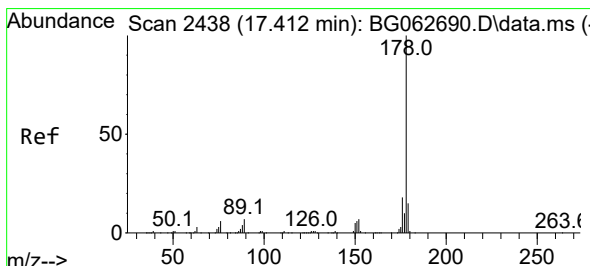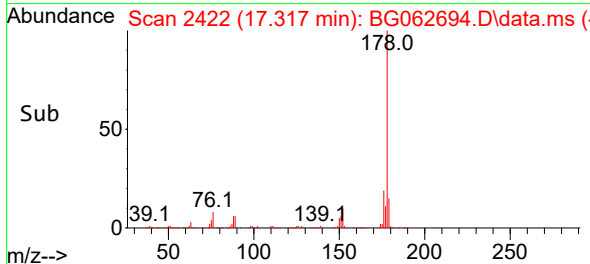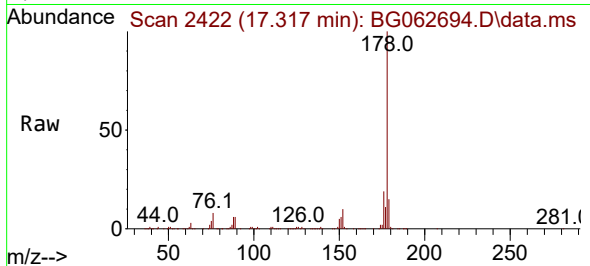

#74
Anthracene
Concen: 19.792 ng/ul
RT: 17.411 min Scan# 2438
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:178 Resp: 677920
Ion Ratio Lower Upper
178 100
179 15.5 12.4 18.6
176 18.5 14.4 21.6


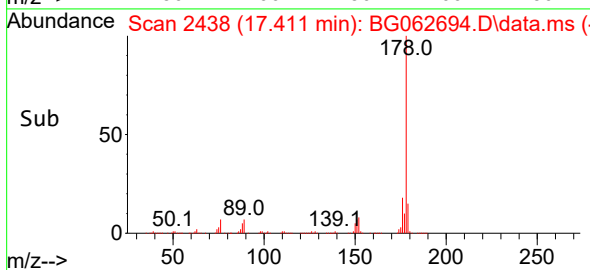

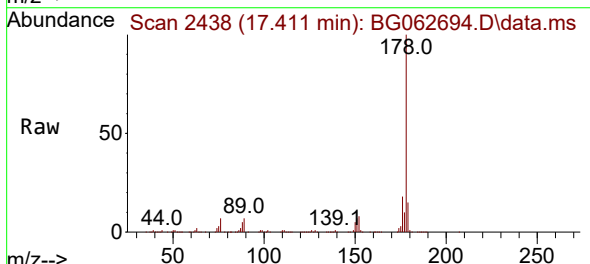




#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.781 ng/ul
RT: 13.328 min Scan# 1
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:216 Resp: 174528
Ion Ratio Lower Upper
216 100
214 75.4 61.5 92.3
218 48.0 38.0 57.0

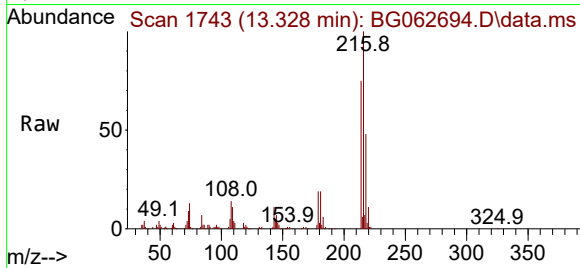

#76
Pentachlorobenzene
Concen: 19.110 ng/ul
RT: 14.849 min Scan# 2002
Delta R.T. -0.006 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:250 Resp: 186843
Ion Ratio Lower Upper
250 100
248 60.9 51.5 77.3
252 68.0 50.8 76.2




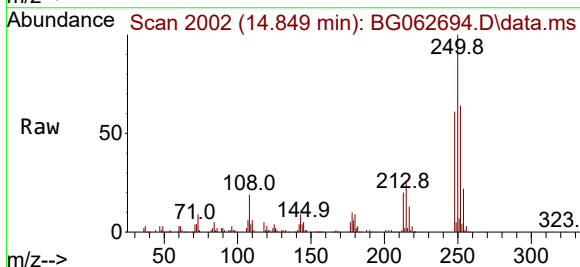




#77
 Carbazole
 Concen: 20.455 ng/ul
 RT: 17.676 min Scan# 2483
 Delta R.T. -0.006 min
 Lab File: BG062694.D
 Acq: 9 Sep 2024 19:08




Instrument :
 BNA_G
 ClientSampleId :
 SICV444


Tgt Ion:167 Resp: 580986
 Ion Ratio Lower Upper
 167 100
 166 22.5 17.2 25.8
 139 12.0 9.0 13.6

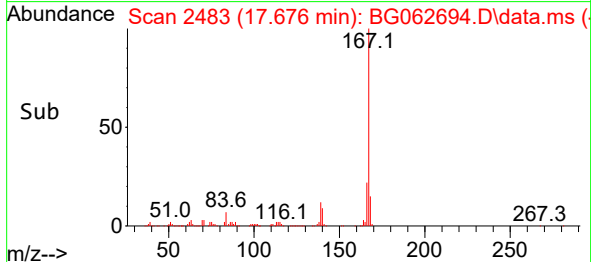

#78
 Di-n-butylphthalate
 Concen: 20.293 ng/ul
 RT: 18.240 min Scan# 2579
 Delta R.T. -0.006 min
 Lab File: BG062694.D
 Acq: 9 Sep 2024 19:08

Tgt Ion:149 Resp: 681677
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.0 10.6
 104 5.0 4.1 6.1




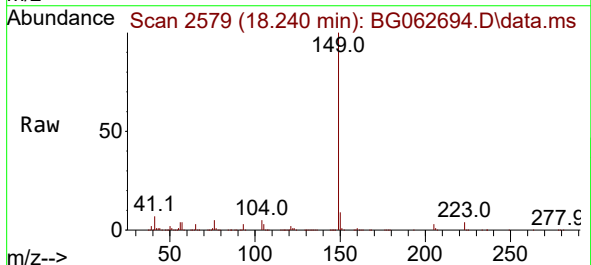


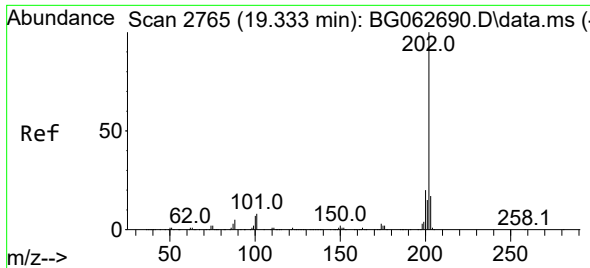

#80
Fluoranthene
Concen: 19.477 ng/ul
RT: 19.332 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08




Instrument :
BNA_G
ClientSampleId :
SICV444


Tgt Ion:202 Resp: 864704
Ion Ratio Lower Upper
202 100
101 8.3 6.6 10.0
100 6.3 5.3 7.9

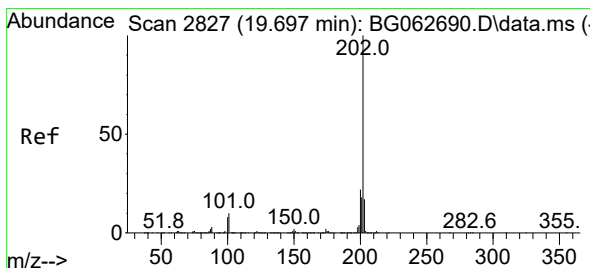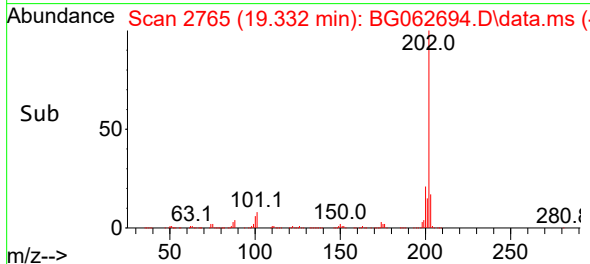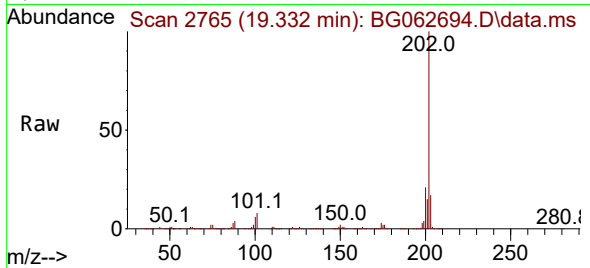

#82
Pyrene
Concen: 19.594 ng/ul
RT: 19.697 min Scan# 2827
Delta R.T. -0.000 min
Lab File: BG062694.D
Acq: 9 Sep 2024 19:08

Tgt Ion:202 Resp: 936419
Ion Ratio Lower Upper
202 100
101 9.4 7.7 11.5
100 7.9 6.5 9.7

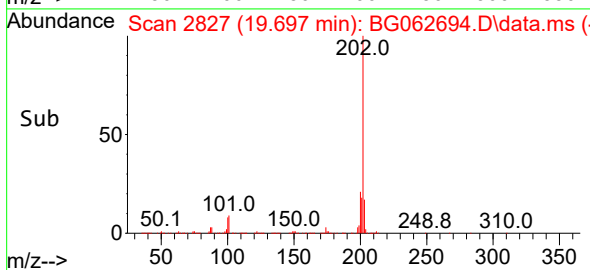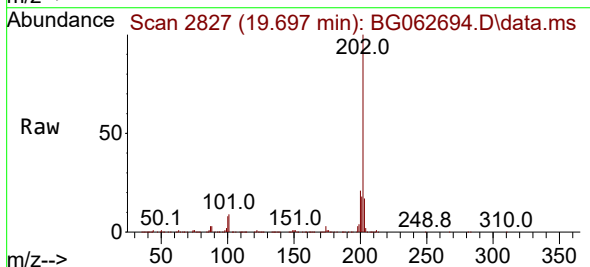



#83

Butylbenzylphthalate

Concen: 20.087 ng/ul

RT: 20.584 min Scan# 2978

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:149 Resp: 284973

Ion Ratio Lower Upper

149 100

91 71.5 57.3 85.9

206 23.5 20.4 30.6



#84

3,3'-Dichlorobenzidine

Concen: 21.417 ng/ul

RT: 21.424 min Scan# 3121

Delta R.T. -0.000 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08




Tgt Ion:252 Resp: 321199


Ion Ratio Lower Upper

252 100

254 67.7 51.8 77.6

126 7.5 6.0 9.0





#85

Benzo(a)anthracene

Concen: 19.631 ng/ul

RT: 21.500 min Scan# 3135

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:228 Resp: 972600

Ion Ratio Lower Upper

228 100

229 19.3 15.8 23.8

226 27.8 21.6 32.4



#86

Bis(2-ethylhexyl)phthalate

Concen: 19.962 ng/ul

RT: 21.424 min Scan# 3121

Delta R.T. -0.000 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08




Tgt Ion:149 Resp: 416996


Ion Ratio Lower Upper

149 100

167 26.0 21.3 31.9

279 4.4 3.8 5.6





#87

Chrysene

Concen: 19.601 ng/ul

RT: 21.565 min Scan# 3145

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:228 Resp: 921302

Ion Ratio Lower Upper

228 100

226 30.8 24.2 36.2

229 20.1 15.4 23.0



#89

Di-n-octyl phthalate

Concen: 20.196 ng/ul




RT: 22.582 min Scan# 3318


Delta R.T. -0.001 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Tgt Ion:149 Resp: 720786





#90

Benzo(b)fluoranthene

Concen: 19.482 ng/ul

RT: 23.616 min Scan# 3494

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:252 Resp: 922907

Ion Ratio Lower Upper

252 100

253 21.7 17.0 25.6

125 7.0 5.4 8.0



#91

Benzo(k)fluoranthene

Concen: 19.766 ng/ul

RT: 23.680 min Scan# 3505

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08




Tgt Ion:252 Resp: 958746


Ion Ratio Lower Upper

252 100

253 22.8 16.9 25.3

125 7.0 5.7 8.5





#93

Benzo(a)pyrene

Concen: 19.636 ng/ul

RT: 24.438 min Scan# 3

Delta R.T. -0.006 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08

Instrument :

BNA_G

ClientSampleId :

SICV444





Tgt Ion:252 Resp: 877350

Ion Ratio Lower Upper

252 100

253 22.6 17.4 26.0

125 7.9 6.1 9.1



#94

Indeno(1,2,3-cd)pyrene

Concen: 19.412 ng/ul

RT: 28.034 min Scan# 4246

Delta R.T. -0.012 min

Lab File: BG062694.D

Acq: 9 Sep 2024 19:08




Tgt Ion:276 Resp: 1068626


Ion Ratio Lower Upper

276 100

138 13.3 11.4 17.2

277 24.6 18.9 28.3



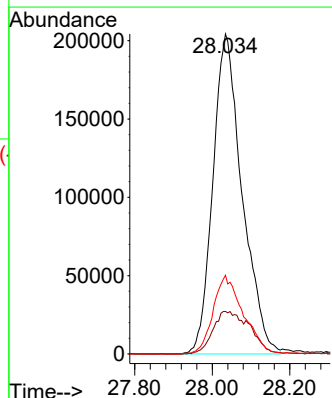





#95
 Dibenzo(a,h)anthracene
 Concen: 19.668 ng/ul
 RT: 28.093 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BG062694.D
 Acq: 9 Sep 2024 19:08

Instrument :
 BNA_G
 ClientSampleId :
 SICV444

Tgt Ion:278 Resp: 869687
 Ion Ratio Lower Upper
 278 100
 139 10.9 7.8 11.8
 279 23.1 18.6 28.0



#96
 Benzo(g,h,i)perylene
 Concen: 19.195 ng/ul
 RT: 29.109 min Scan# 4429
 Delta R.T. -0.018 min
 Lab File: BG062694.D
 Acq: 9 Sep 2024 19:08

Tgt Ion:276 Resp: 816121
 Ion Ratio Lower Upper
 276 100
 138 14.1 11.8 17.6
 277 22.6 18.4 27.6

