


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090925\
Data File : BG064316.D
Acq On : 9 Sep 2025 8:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

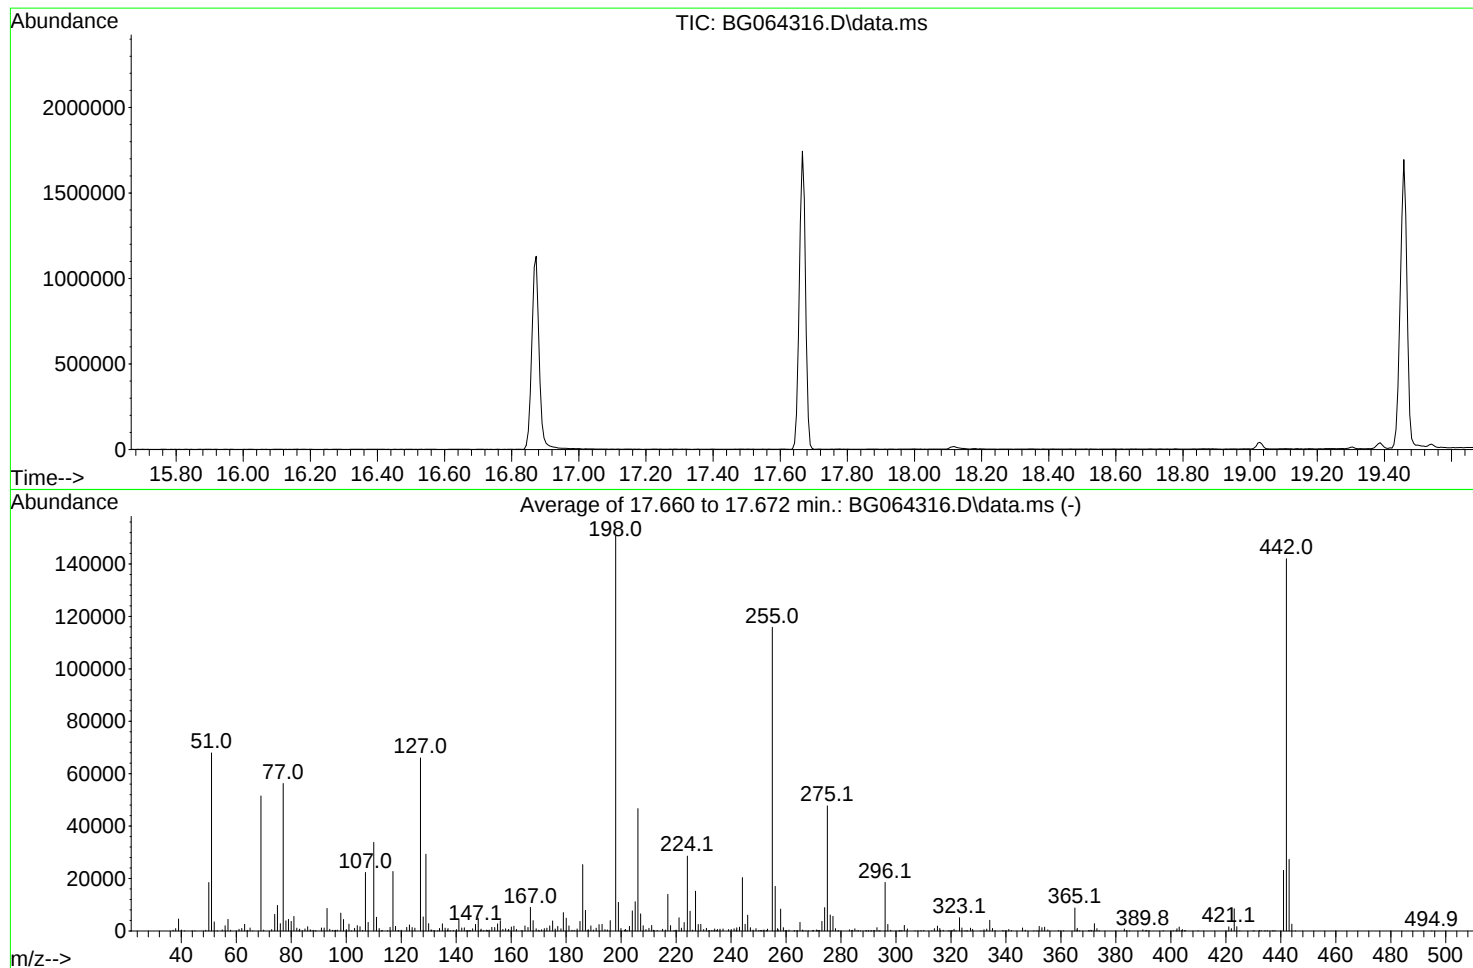




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	51533	PASS
70	69	0.00	2	0.7	351	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	150656	PASS
199	198	5	9	7.2	10891	PASS
365	198	1	100	5.8	8751	PASS
441	443	0.01	150	84.6	23088	PASS
442	442	100	100	100.0	142037	PASS
443	442	15	24	19.2	27291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090925\
Data File : BG064316.D
Acq On : 9 Sep 2025 8:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 09 11:23:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

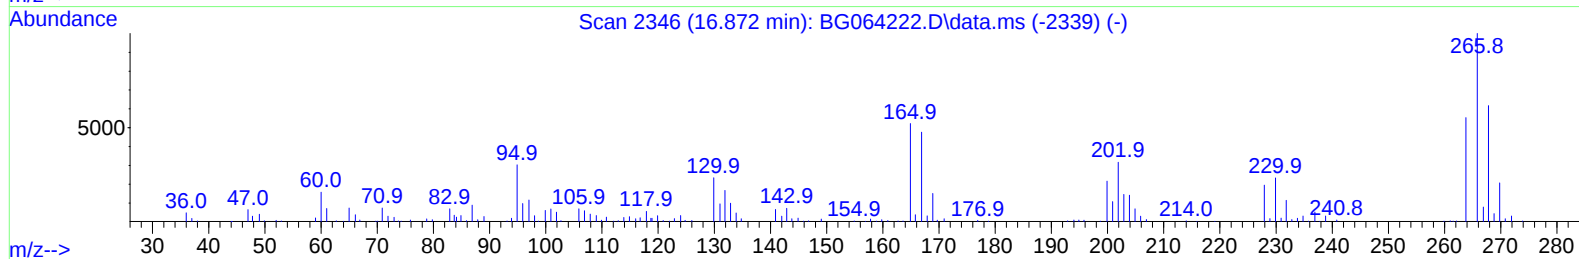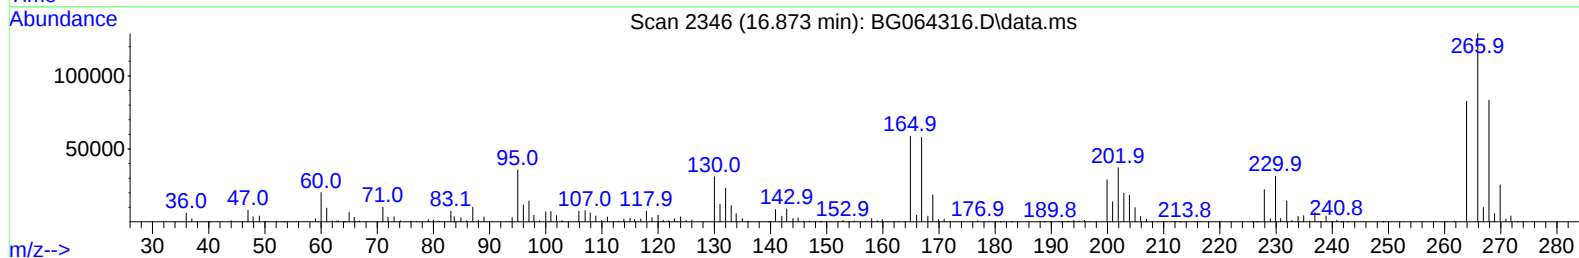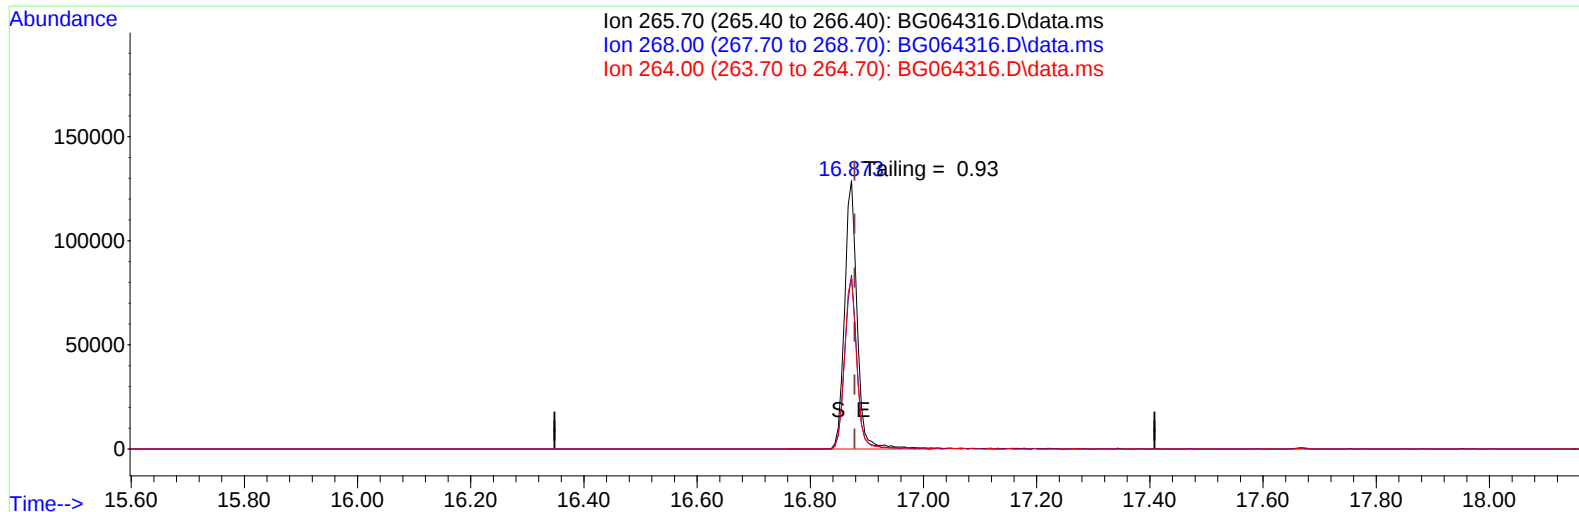

TIC: BG064316.D\data.ms

(70) Pentachlorophenol (C)

16.873min (-0.005) 401326.33 ng




response 198040

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.73
264.00	55.40	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090925\
Data File : BG064316.D
Acq On : 9 Sep 2025 8:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 09 11:23:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

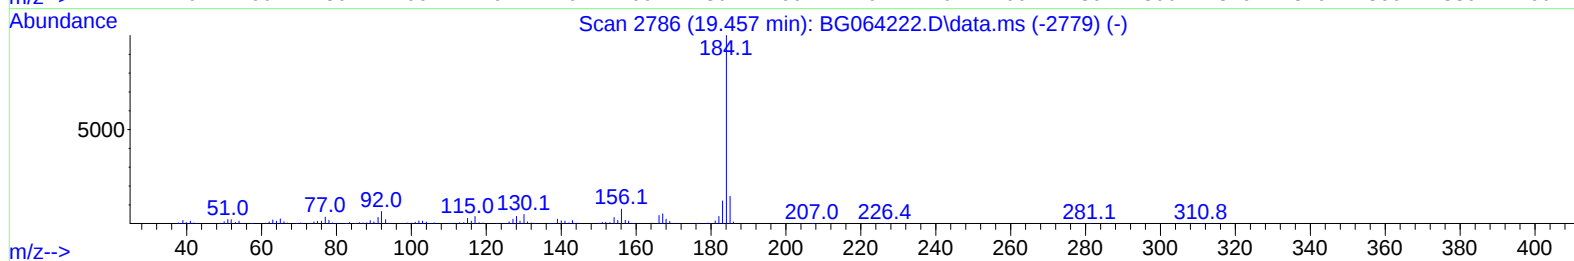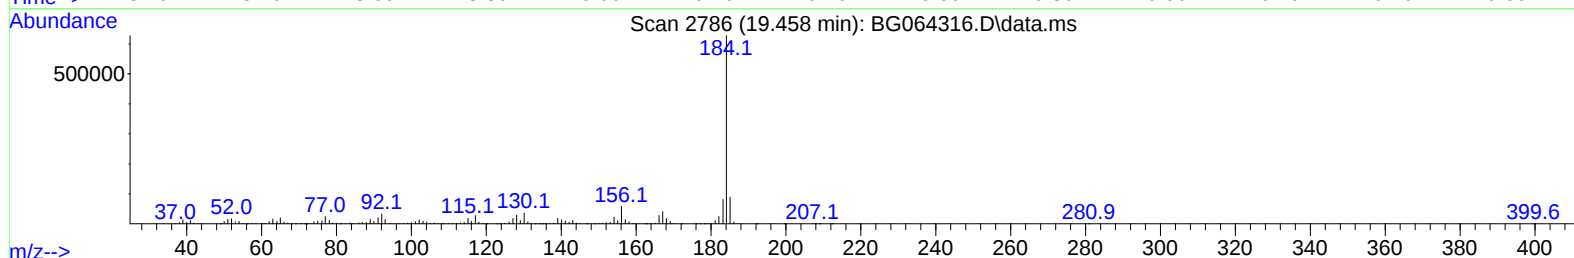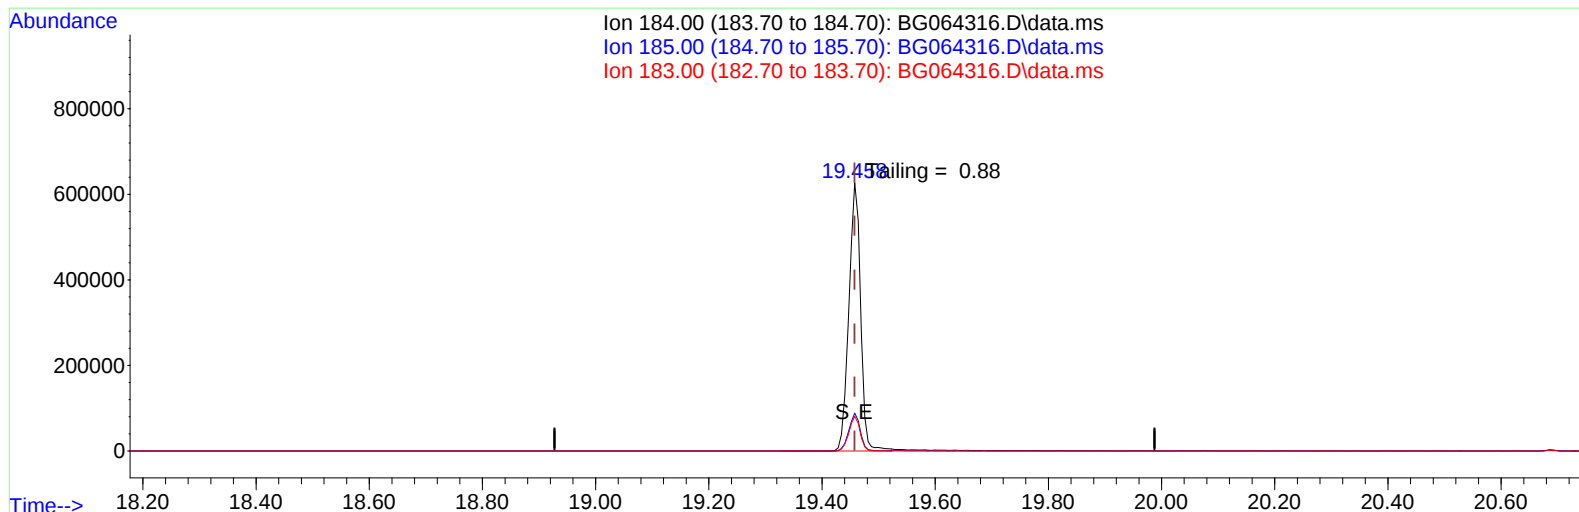

TIC: BG064316.D\data.ms

(77) Benzidine

19.458min (+ 0.001) 754140.66 ng

response 904275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.12
183.00	12.10	12.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/9/2025	BNA_G	<u>BG064316.D</u>
Compound Name	Response	Retention Time
DDT	535921	20.692
DDD	14510	20.245
DDE	798	19.746
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15308	551229	2.78

Instrument :
BNA_G
ClientSampleId :
DFTPP