

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091017\
 Data File : BG028631.D
 Acq On : 10 Sep 2017 1:31
 Operator : SJ/JU
 Sample : I5164-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SES-MS-PH4-COA9-17

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG090717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.906	387	394	406	rBV	287729	485864	12.91%	3.472%
2	7.487	656	663	674	rBV	164399	313407	8.33%	2.239%
3	7.869	720	728	740	rVB	510133	905406	24.07%	6.469%
4	8.333	800	807	816	rBV	127291	221491	5.89%	1.583%
5	8.662	854	863	871	rBV	520018	931049	24.75%	6.652%
6	9.502	998	1006	1016	rBV	420530	780501	20.75%	5.577%
7	11.153	1280	1287	1297	rBV2	162859	302779	8.05%	2.163%
8	13.562	1690	1697	1707	rBV	1250165	1969267	52.34%	14.071%
9	14.943	1925	1932	1941	rVB	267695	449189	11.94%	3.210%
10	16.435	2177	2186	2196	rBV	1051075	1639633	43.58%	11.715%
11	17.692	2392	2400	2408	rBV2	403463	631962	16.80%	4.515%
12	20.278	2834	2840	2850	rBV	2857009	3762309	100.00%	26.882%
13	22.023	3130	3137	3147	rBV	451372	825682	21.95%	5.900%
14	25.524	3723	3733	3748	rVB	244162	776973	20.65%	5.552%


Sum of corrected areas: 13995512

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG091017\
Data File : BG028631.D
Acq On : 10 Sep 2017 1:31
Operator : SJ/JU
Sample : I5164-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SES-MS-PH4-COA9-17

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG090717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

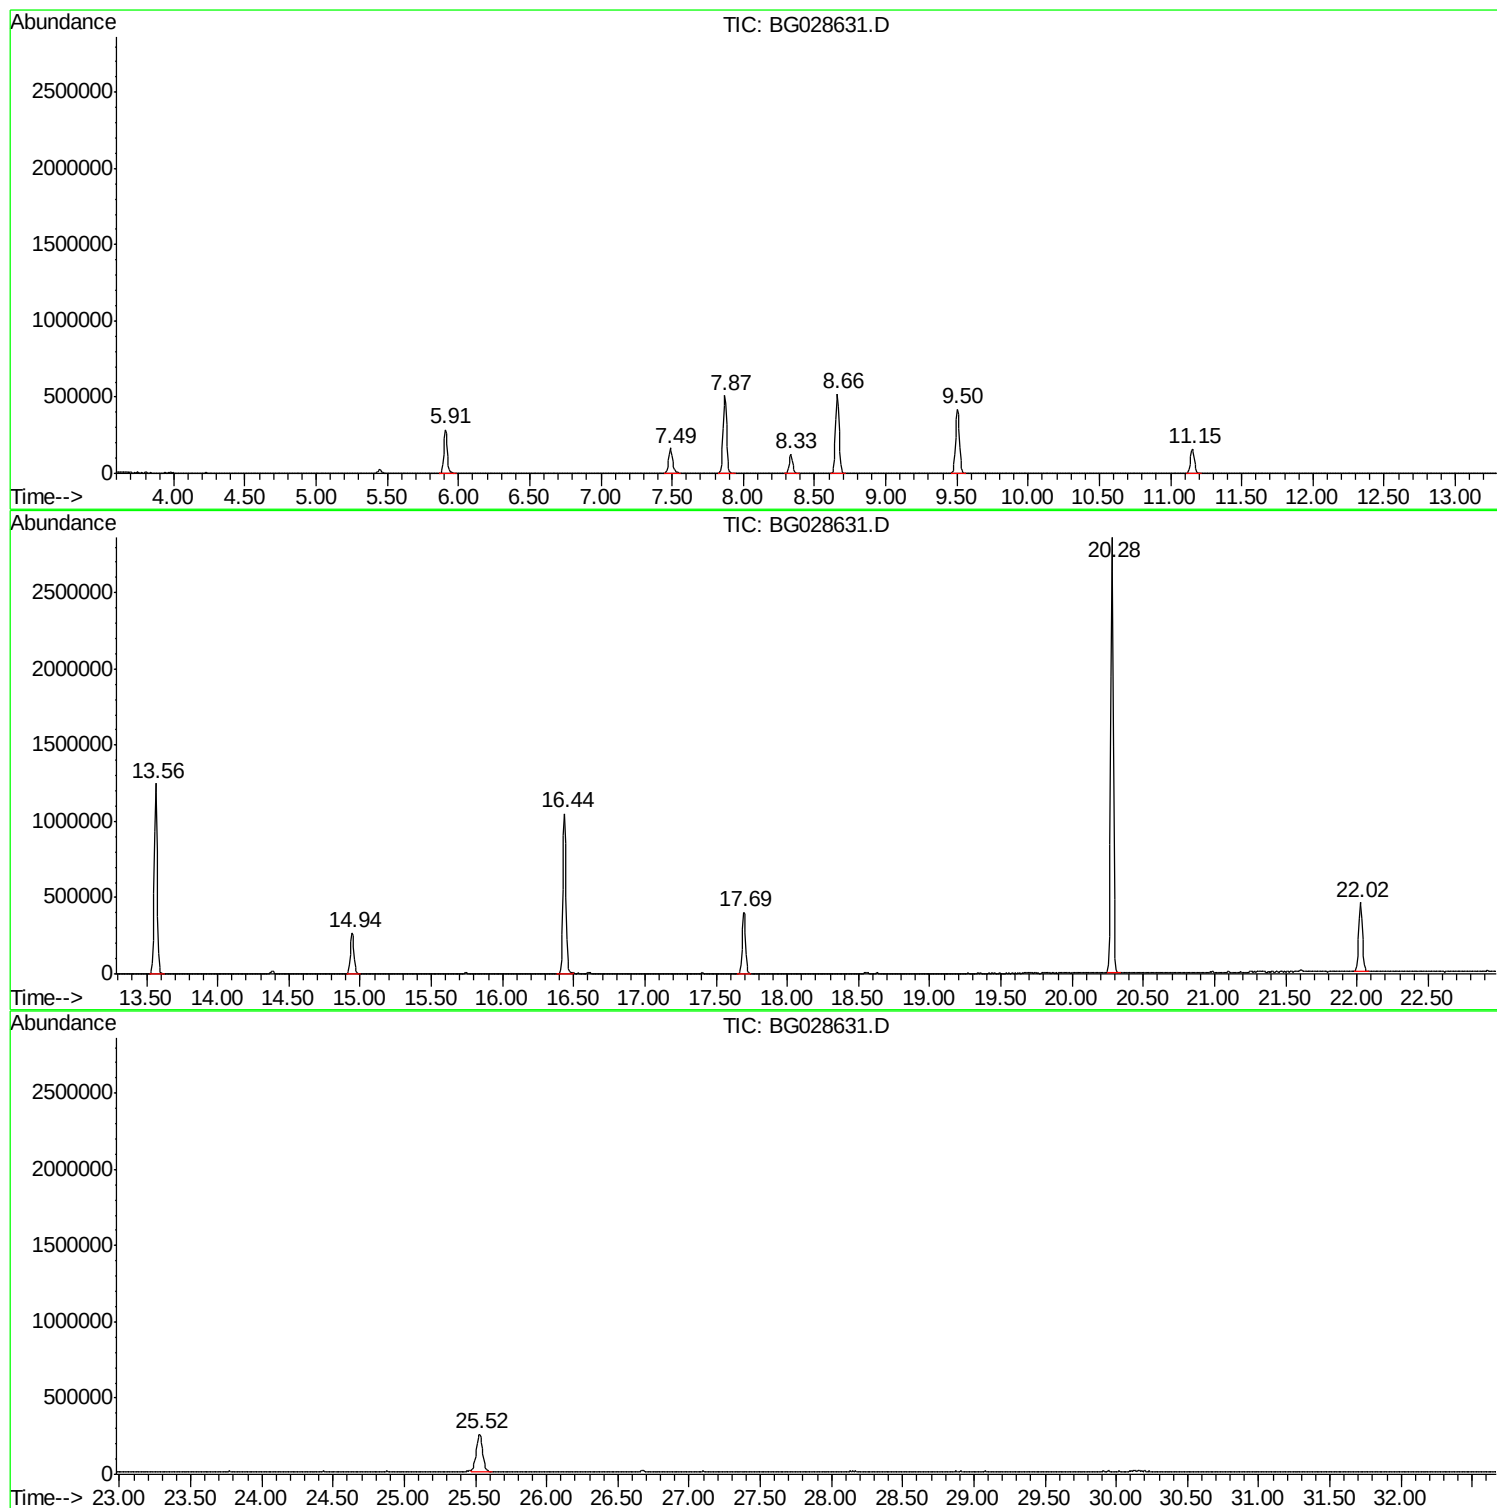

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG091017\
Data File : BG028631.D
Acq On : 10 Sep 2017 1:31
Operator : SJ/JU
Sample : I5164-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SES-MS-PH4-COA9-17










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG090717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.87 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.87	81.76 ng	905406	1,4-Dichlorobenzene-d4	8.33

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	14
5		Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	10

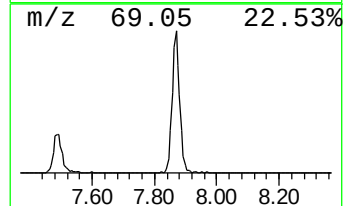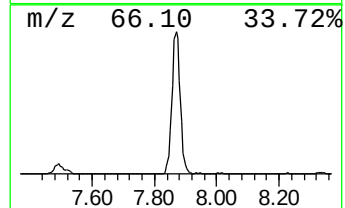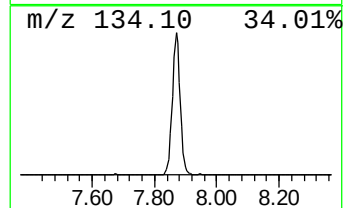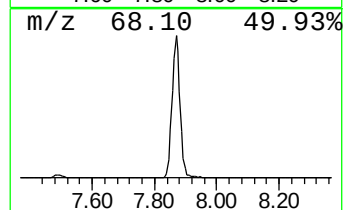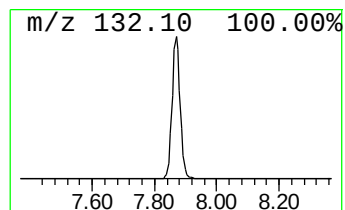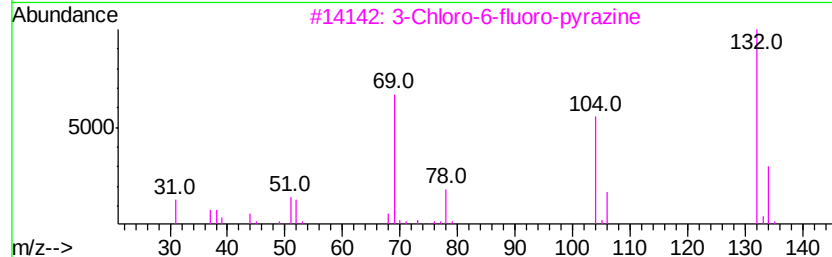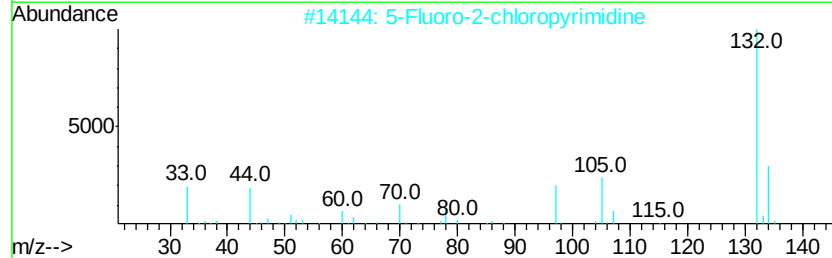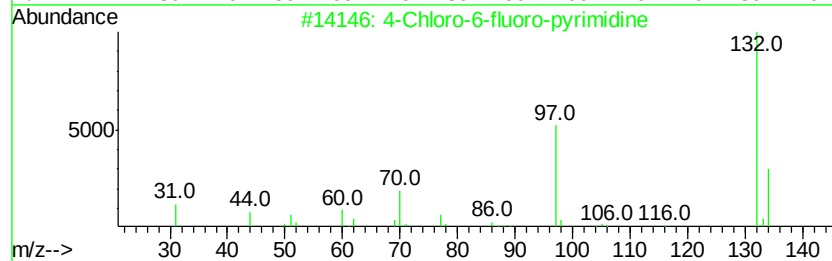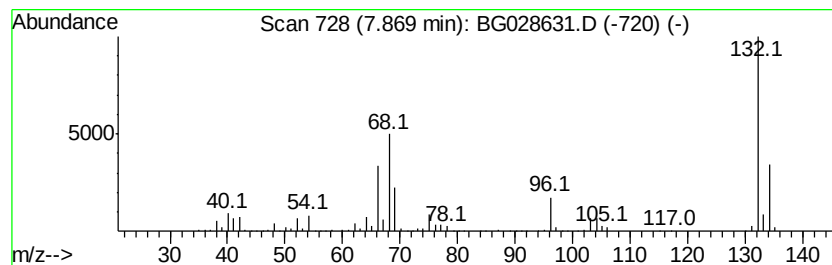

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG091017\
Data File : BG028631.D
Acq On : 10 Sep 2017 1:31
Operator : SJ/JU
Sample : I5164-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SES-MS-PH4-COA9-17

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG090717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.87	7.87	81.8	ng	905406	1	8.33	221491	20.0